

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
 Data File : PD050048.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2018 3:33
 Operator : AJ\SJ
 Sample : J5626-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EB-2018.10.19-SED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:20:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 19 07:43:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	4.061	12773349	596.9E6	21.306	23.257
28)	SA Decachlor...	9.013	9.173	8568117	222.0E6	13.910	14.046

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102318\
Data File : PD050048.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2018 3:33
Operator : AJ\SJ
Sample : J5626-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EB-2018.10.19-SED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:20:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101818.M
Quant Title : GC Extractables
QLast Update : Fri Oct 19 07:43:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

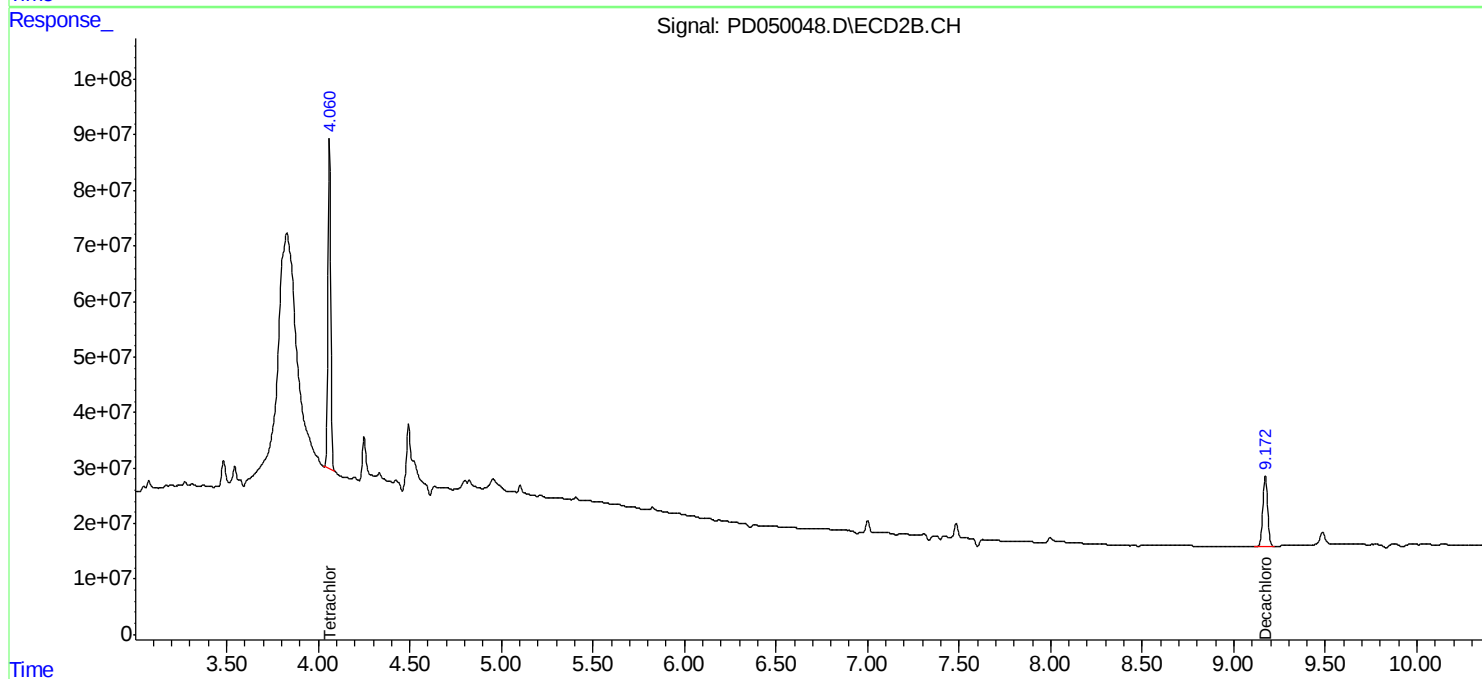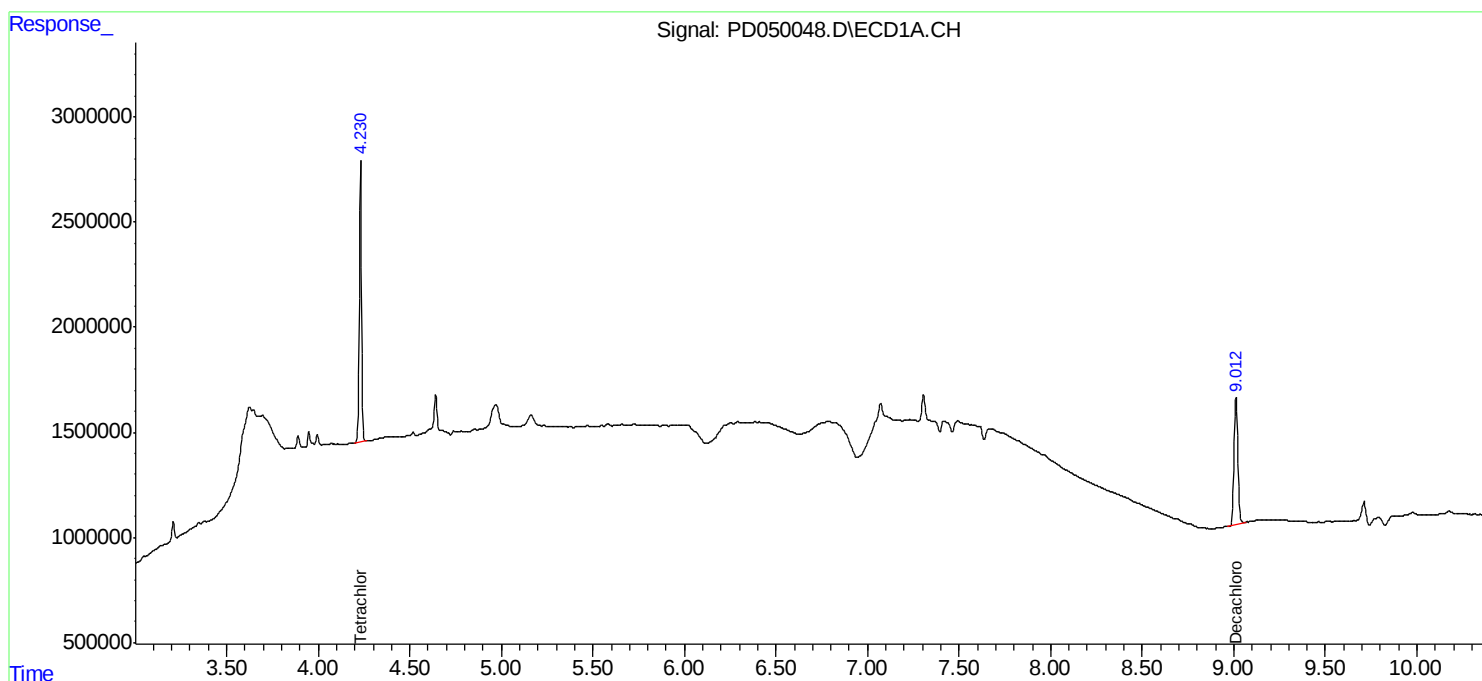


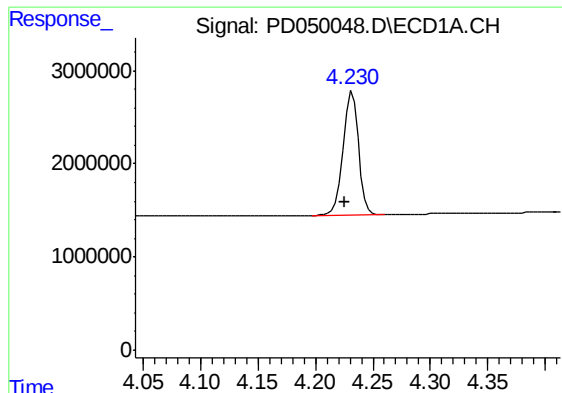

#1 Tetrachloro-m-xylene


R.T.: 4.232 min
Delta R.T.: 0.007 min
Response: 12773349
Conc: 21.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
EB-2018.10.19-SED

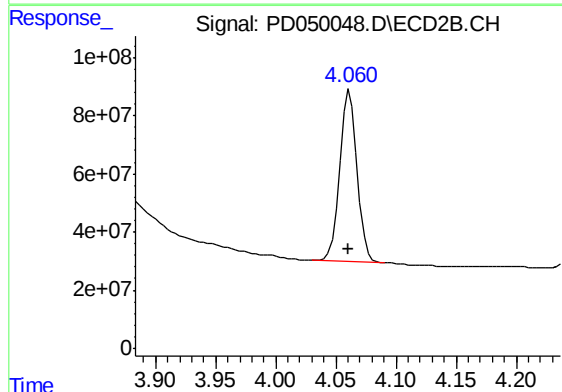


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.001 min
Response: 596850682
Conc: 23.26 ng/ml

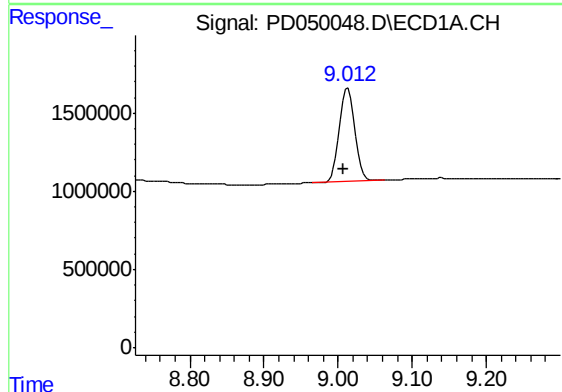

#28 Decachlorobiphenyl

R.T.: 9.013 min
Delta R.T.: 0.007 min
Response: 8568117
Conc: 13.91 ng/ml

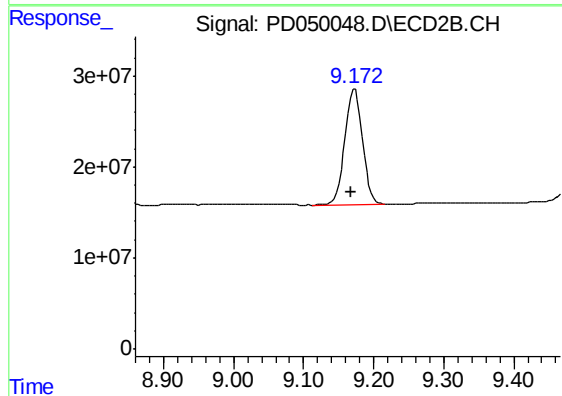

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.005 min
Response: 221950732
Conc: 14.05 ng/ml