

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
 Data File : PD055532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 09:45
 Operator : SG\AJ
 Sample : K5354-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFB86

Manual Integrations
 APPROVED

Ankita
 10/24/2019 12:57:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:15:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.290	3.962	17309335	24326388	19.414	18.068
27) SA Decachlor...	7.964	8.997	51312568	191.7E6	56.038	146.913m#
Target Compounds						
2) A alpha-BHC	3.715	4.347	6510549	13878642	5.184m	7.134m#
3) MA gamma-BHC...	3.998	4.611	36407659	62132998	30.723	33.696m
13) MA Dieldrin	5.533	6.428	98053826	27333251	88.477m	15.103 #
14) MA Endrin	5.778	6.645	39984813	14539827	44.640m	10.410m#
15) B Endosulfa...	6.058	6.849	20542902	38639684	21.459	24.854m
16) A 4,4'-DDD	5.915	6.775	60037336	245.2E6	74.077m	171.387m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
Data File : PD055532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 09:45
Operator : SG\AJ
Sample : K5354-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:15:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

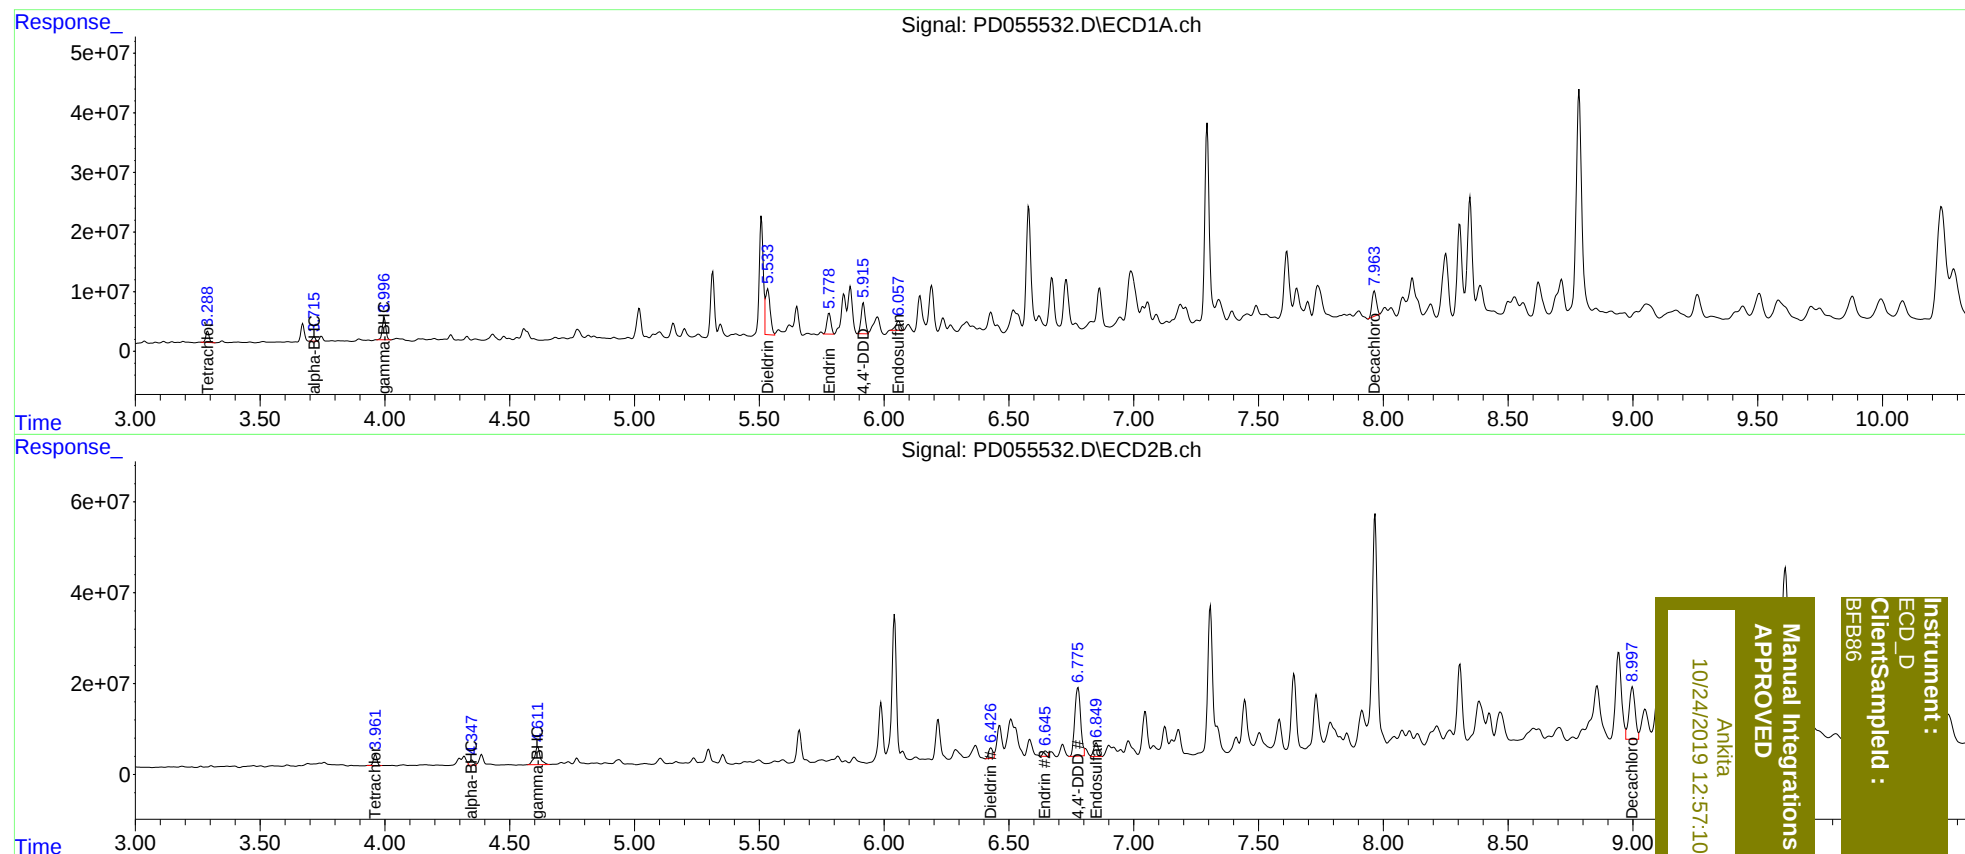

10/24/2019 12:57:10 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sample :
BFB86