

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
 Data File : PD055543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 13:44
 Operator : SG\AJ
 Sample : K5482-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ5

Manual Integrations
 APPROVED

Ankita
 10/24/2019 12:57:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:19:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.961	12782259	17539268	14.337	13.027m
27)	SA Decachlor...	7.965	8.996	26326536	41820495	28.751	32.051m
Target Compounds							
12)	B 4,4'-DDE	5.402	6.288	13211582	19280819	12.962	11.435
14)	MA Endrin	5.785	6.681	223.4E6	372.0E6	249.365	266.300
16)	A 4,4'-DDD	5.913	6.775	337.7E6	504.9E6	416.678	352.926
17)	MA 4,4'-DDT	6.149	7.073	1571.0E6	2328.3E6	2317.072	1717.758 #
21)	B Endrin ke...	6.914	7.680	45747095	94805247	46.806	59.193m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
Data File : PD055543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 13:44
Operator : SG\AJ
Sample : K5482-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:19:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

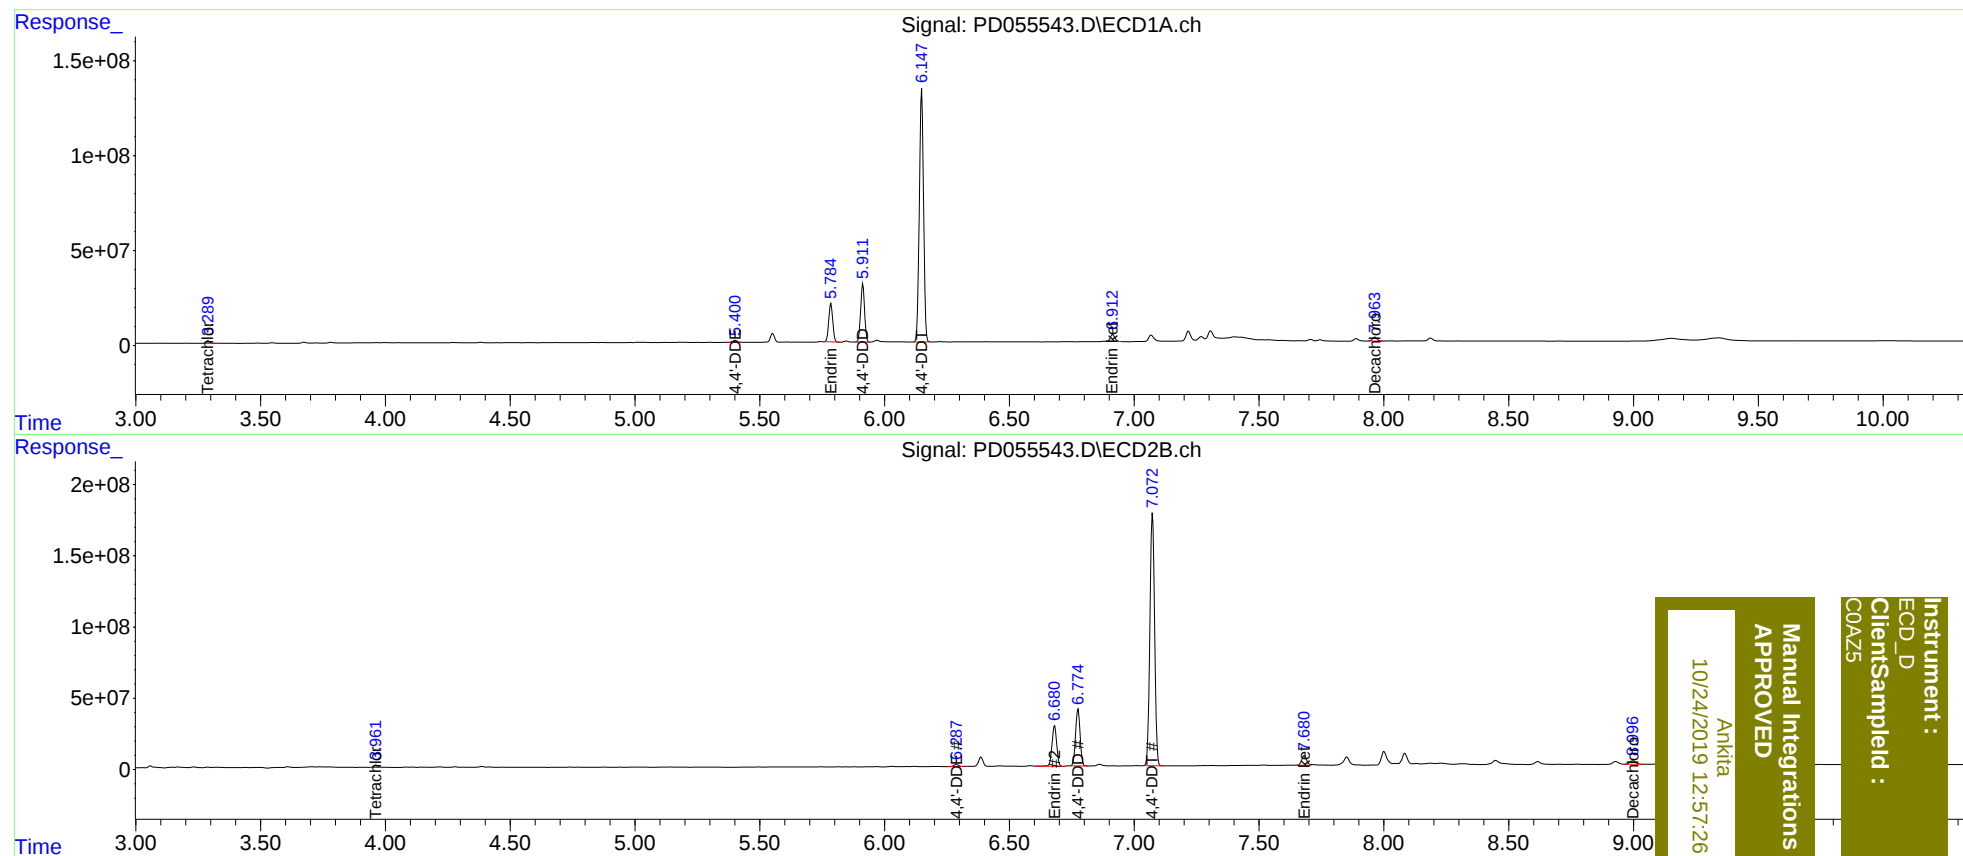

Manual Integrations
APPROVED

Ankita
10/24/2019 12:57:26 PM

Instrument :
ECD_D
Client Sampled :
C0A25