

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
 Data File : PD055549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 15:38
 Operator : SG\AJ
 Sample : K5482-01DL 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ4DL1

Manual Integrations
 APPROVED

Ankita
 10/24/2019 12:57:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:21:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
9) A	Endosulfan I	5.291	6.191	2392761	1186988	2.489m 0.724 #
12) B	4,4'-DDE	5.401	6.287	21465186	28351014	21.060 16.814
14) MA	Endrin	5.785	6.680	1002.7E6	1573.4E6	1119.392 1126.414m
16) A	4,4'-DDD	5.912	6.775	235.1E6	357.9E6	290.045 250.147
17) MA	4,4'-DDT	6.149	7.074	4962.5E6	6958.1E6	7319.437 5133.537 #
21) B	Endrin ke...	6.896	7.681	3513806	1492964	3.595m 0.932m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
Data File : PD055549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 15:38
Operator : SG\AJ
Sample : K5482-01DL 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:21:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

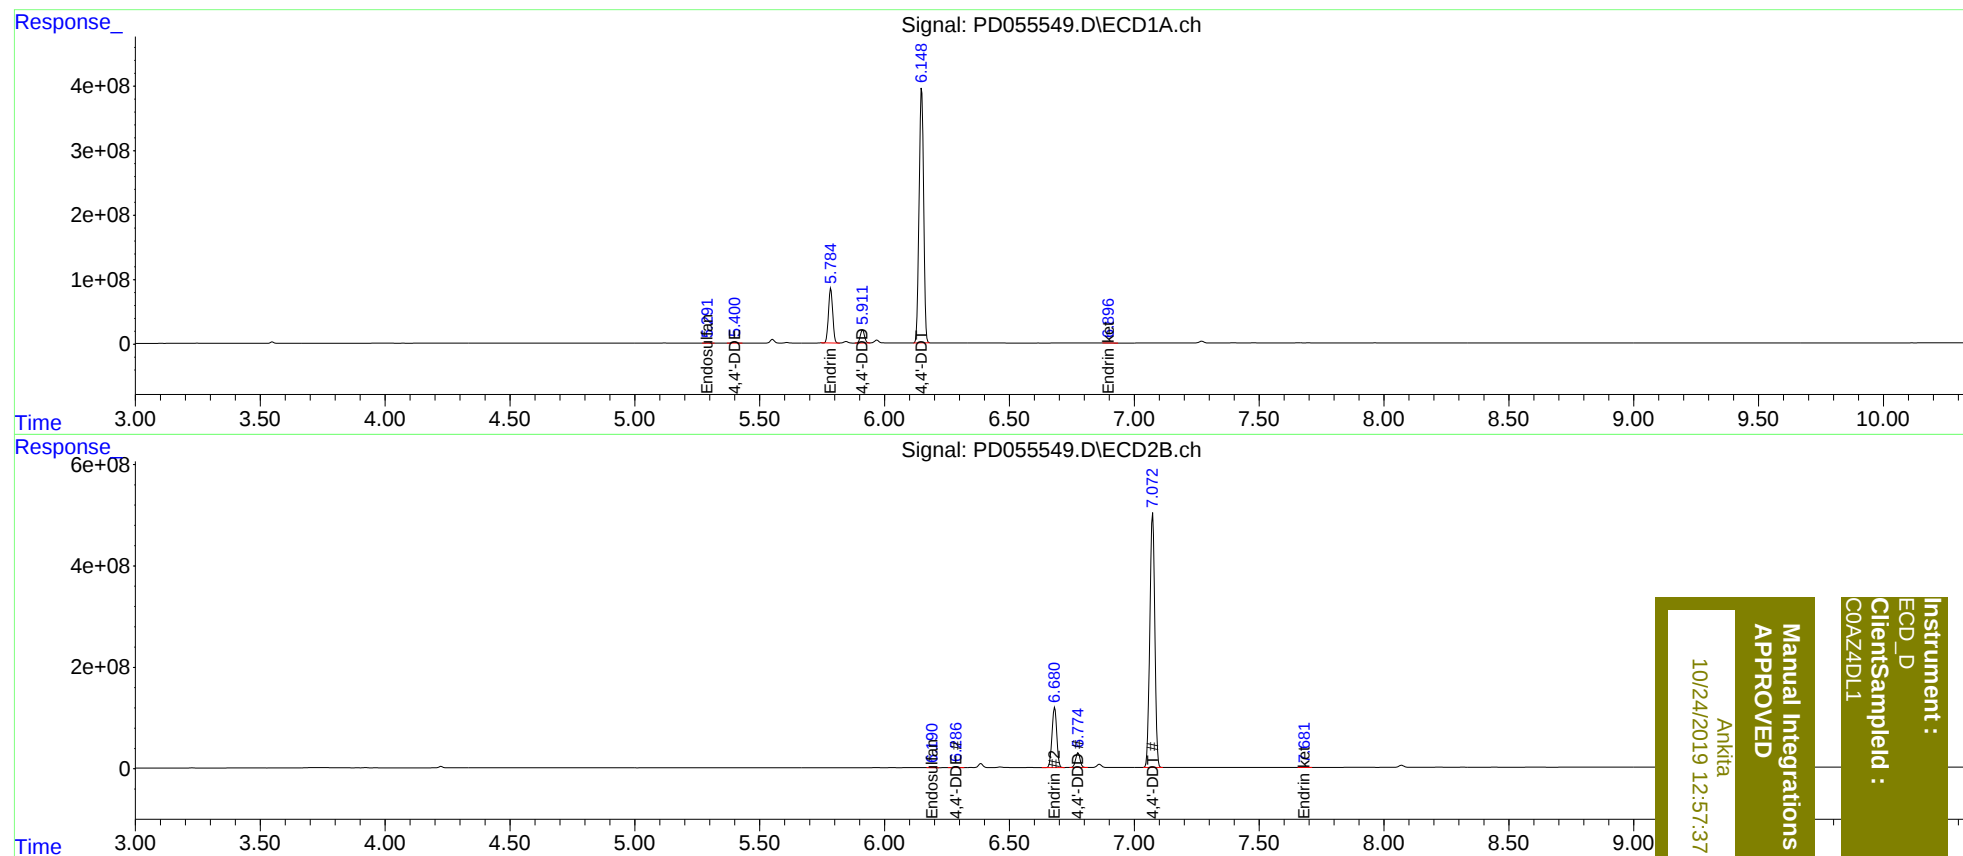

Manual Integrations
APPROVED

Ankita
10/24/2019 12:57:37 PM

Instrument :
ECD_D
Client Sampled :
C0A24DL1