

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
 Data File : PD055555.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 17:02
 Operator : SG\AJ
 Sample : K5482-04DL 2X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ5DL

Manual Integrations
 APPROVED

Ankita
 10/24/2019 12:57:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:23:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.961	7115829	9986892	7.981	7.418m
27)	SA Decachlor...	7.964	8.996	14352396	22369724	15.674	17.144m
Target Compounds							
12)	B 4,4'-DDE	5.400	6.287	7221108	10793860	7.085	6.402
14)	MA Endrin	5.783	6.681	113.1E6	187.0E6	126.292m	133.875
16)	A 4,4'-DDD	5.912	6.775	170.8E6	259.1E6	210.797	181.095
17)	MA 4,4'-DDT	6.148	7.073	785.6E6	1203.0E6	1158.697	887.547
21)	B Endrin ke...	6.913	7.681	20824374	45884186	21.306	28.649 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
Data File : PD055555.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 17:02
Operator : SG\AJ
Sample : K5482-04DL 2X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:23:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

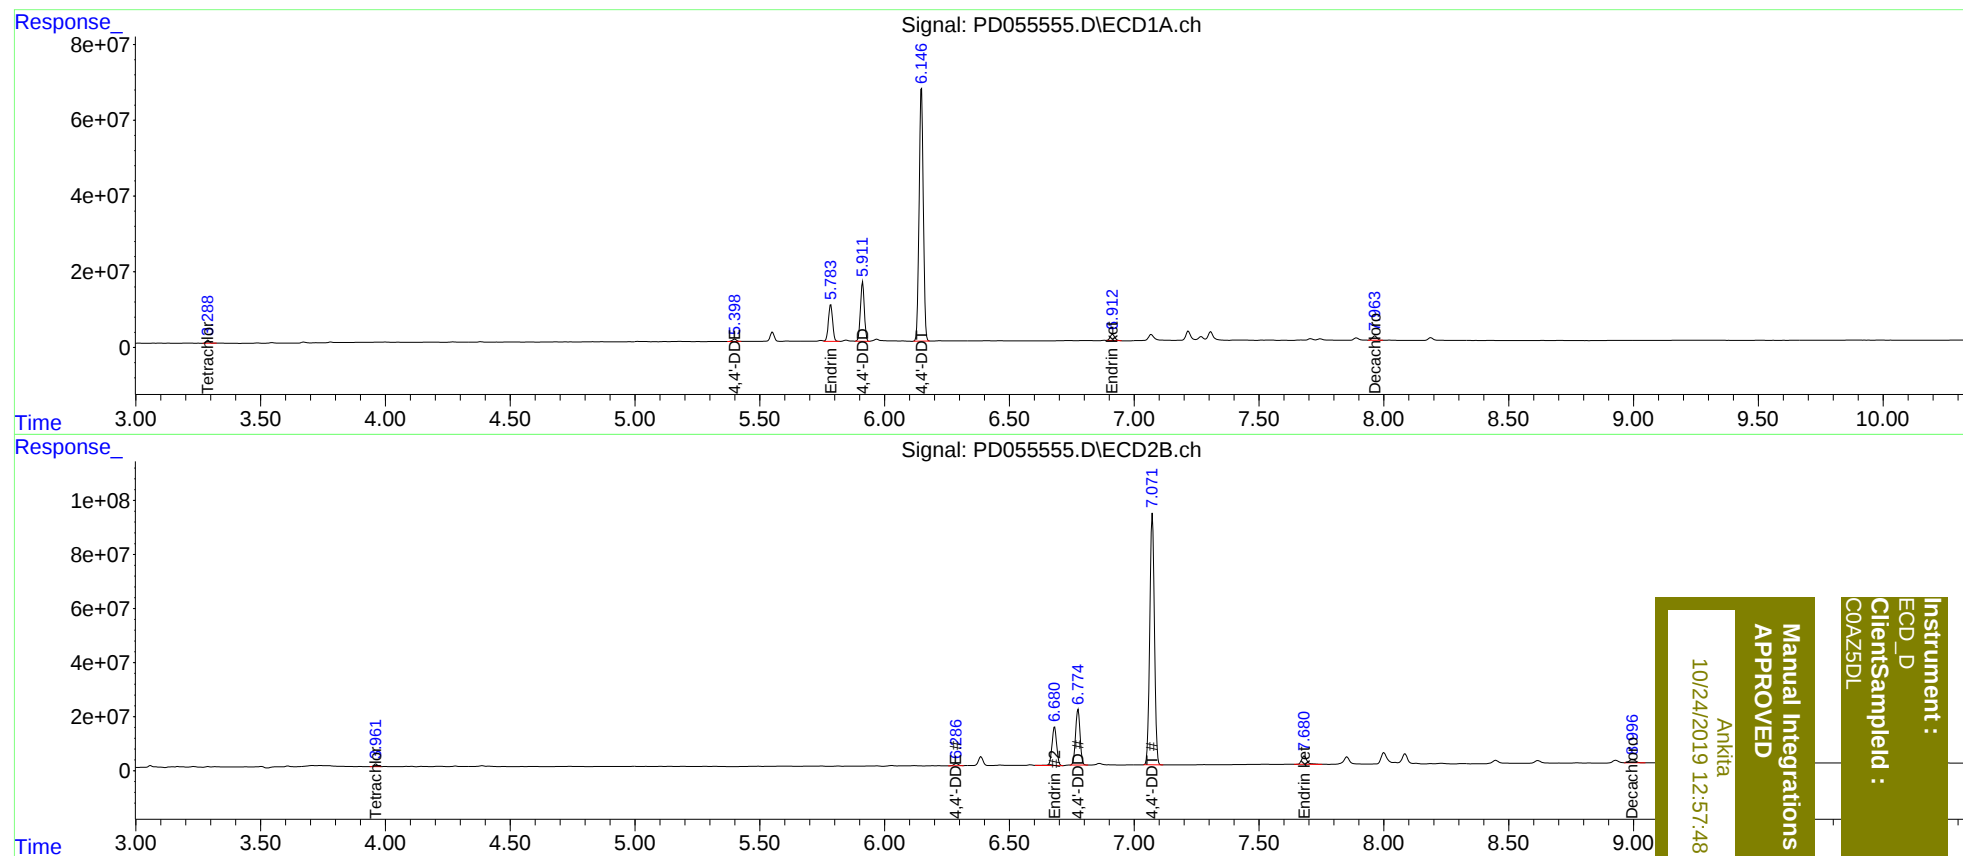

Manual Integrations
APPROVED

Ankita
10/24/2019 12:57:48 PM

Instrument :
ECD_D
Client Sampled :
C0A25DL