

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
 Data File : PD055557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 17:30
 Operator : SG\AJ
 Sample : K5482-05DL 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ6DL

Manual Integrations
 APPROVED

Ankita
 10/24/2019 12:57:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:23:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.961	2490129	3787462	2.793	2.813m
27)	SA Decachlor...	7.964	8.996	3938638	7303159	4.301	5.597m#
Target Compounds							
12)	B 4,4'-DDE	5.401	6.288	9372482	16535311	9.195	9.807
14)	MA Endrin	5.783	6.680	15982951	27985671	17.844m	20.036m
15)	B Endosulfa...	6.036	6.859	2602777	1223714	2.719m	0.787m#
16)	A 4,4'-DDD	5.911	6.775	53619523	83011549	66.159	58.025
17)	MA 4,4'-DDT	6.147	7.072	84764013	142.8E6	125.022	105.347m
21)	B Endrin ke...	6.914	7.680	24247830	46335785	24.809	28.931m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102319\
Data File : PD055557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 17:30
Operator : SG\AJ
Sample : K5482-05DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:23:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

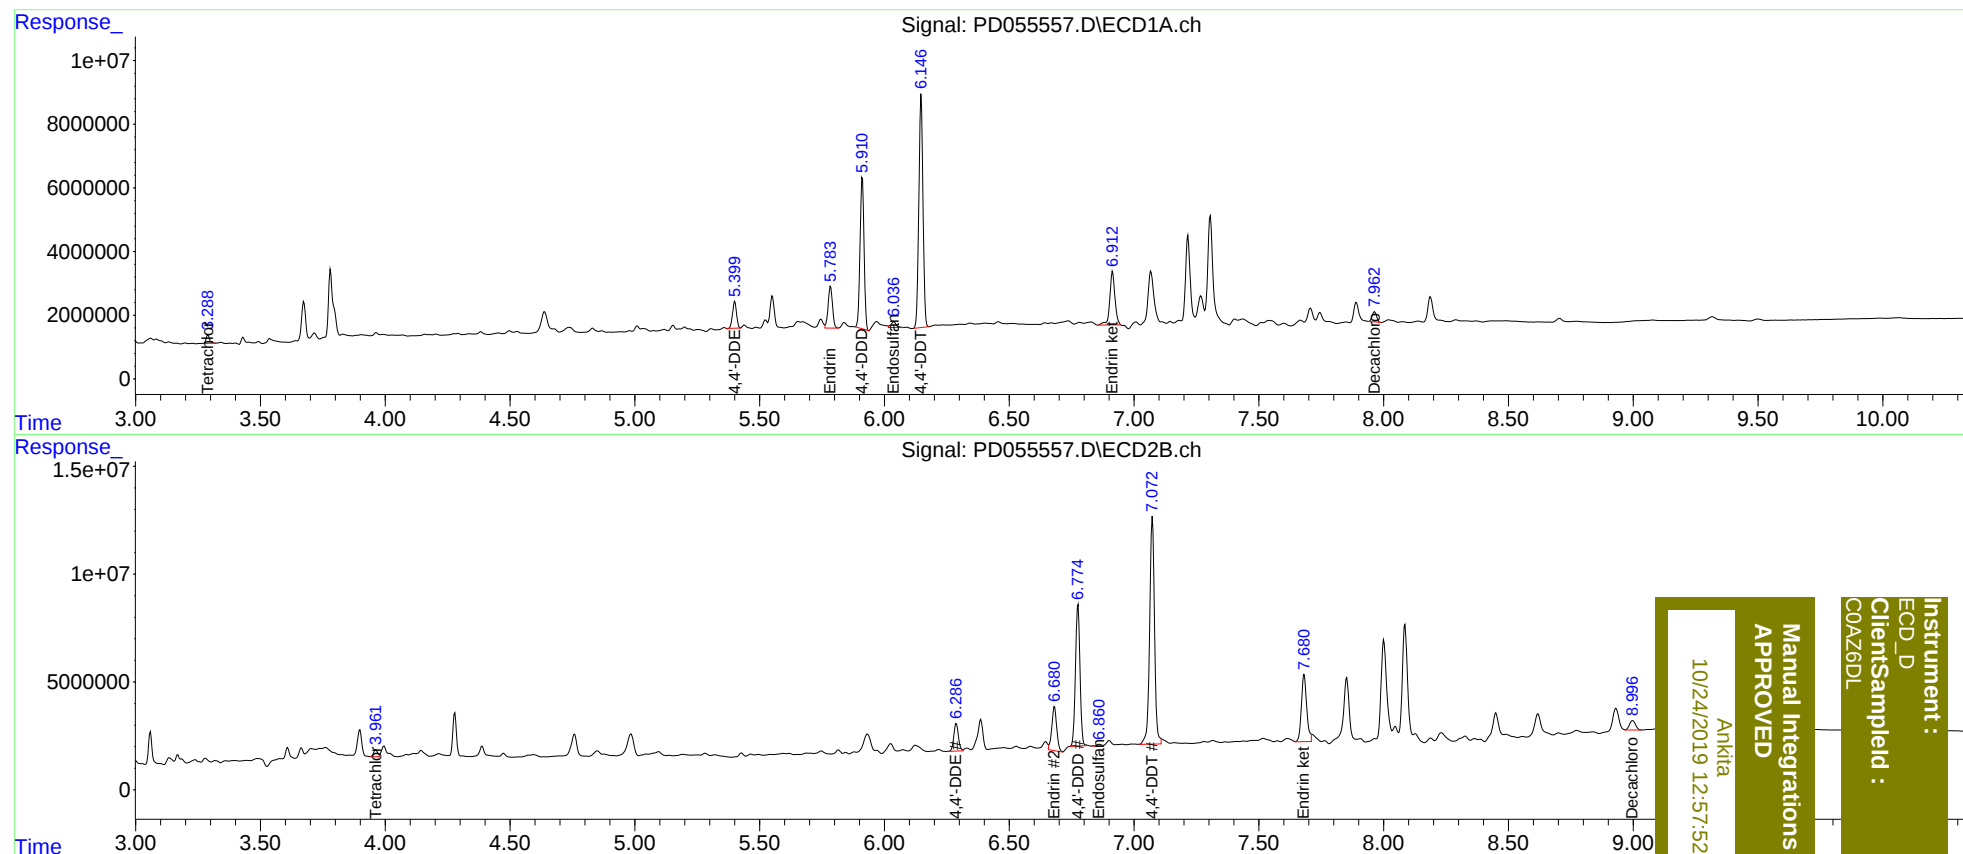

10/24/2019 12:57:52 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sample :
C0A26DL