

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102323\
 Data File : PD079078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2023 11:31
 Operator : AR\AJ
 Sample : PIBLK048
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 21:42:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.806	34315699	45713602	22.375	21.080
27)	SA Decachlor...	9.117	7.955	72374359	90636536	38.159	38.862
Target Compounds							
2)	A alpha-BHC	0.000	3.297	0	103790	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.660	0	132622	N.D.	<MDL
4)	MA Heptachlor	0.000	3.946f	0	224975	N.D.	<MDL
5)	MB Aldrin	0.000	4.270	0	704772	N.D.	0.229
6)	B beta-BHC	0.000	3.946	0	224975	N.D.	0.156
7)	B delta-BHC	4.793	0.000	2612010	0	0.996	N.D. #
8)	B Heptachlo...	0.000	4.795	0	398936	N.D.	0.138
13)	MA Dieldrin	0.000	5.453f	0	147726	N.D.	<MDL
14)	MA Endrin	0.000	5.691	0	238233	N.D.	<MDL
15)	B Endosulfa...	0.000	5.931f	0	184574	N.D.	<MDL
23)	Toxaphene-2	0.000	5.691f	0	238233	N.D.	14.500

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102323\
Data File : PD079078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2023 11:31
Operator : AR\AJ
Sample : PIBLK048
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 21:42:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

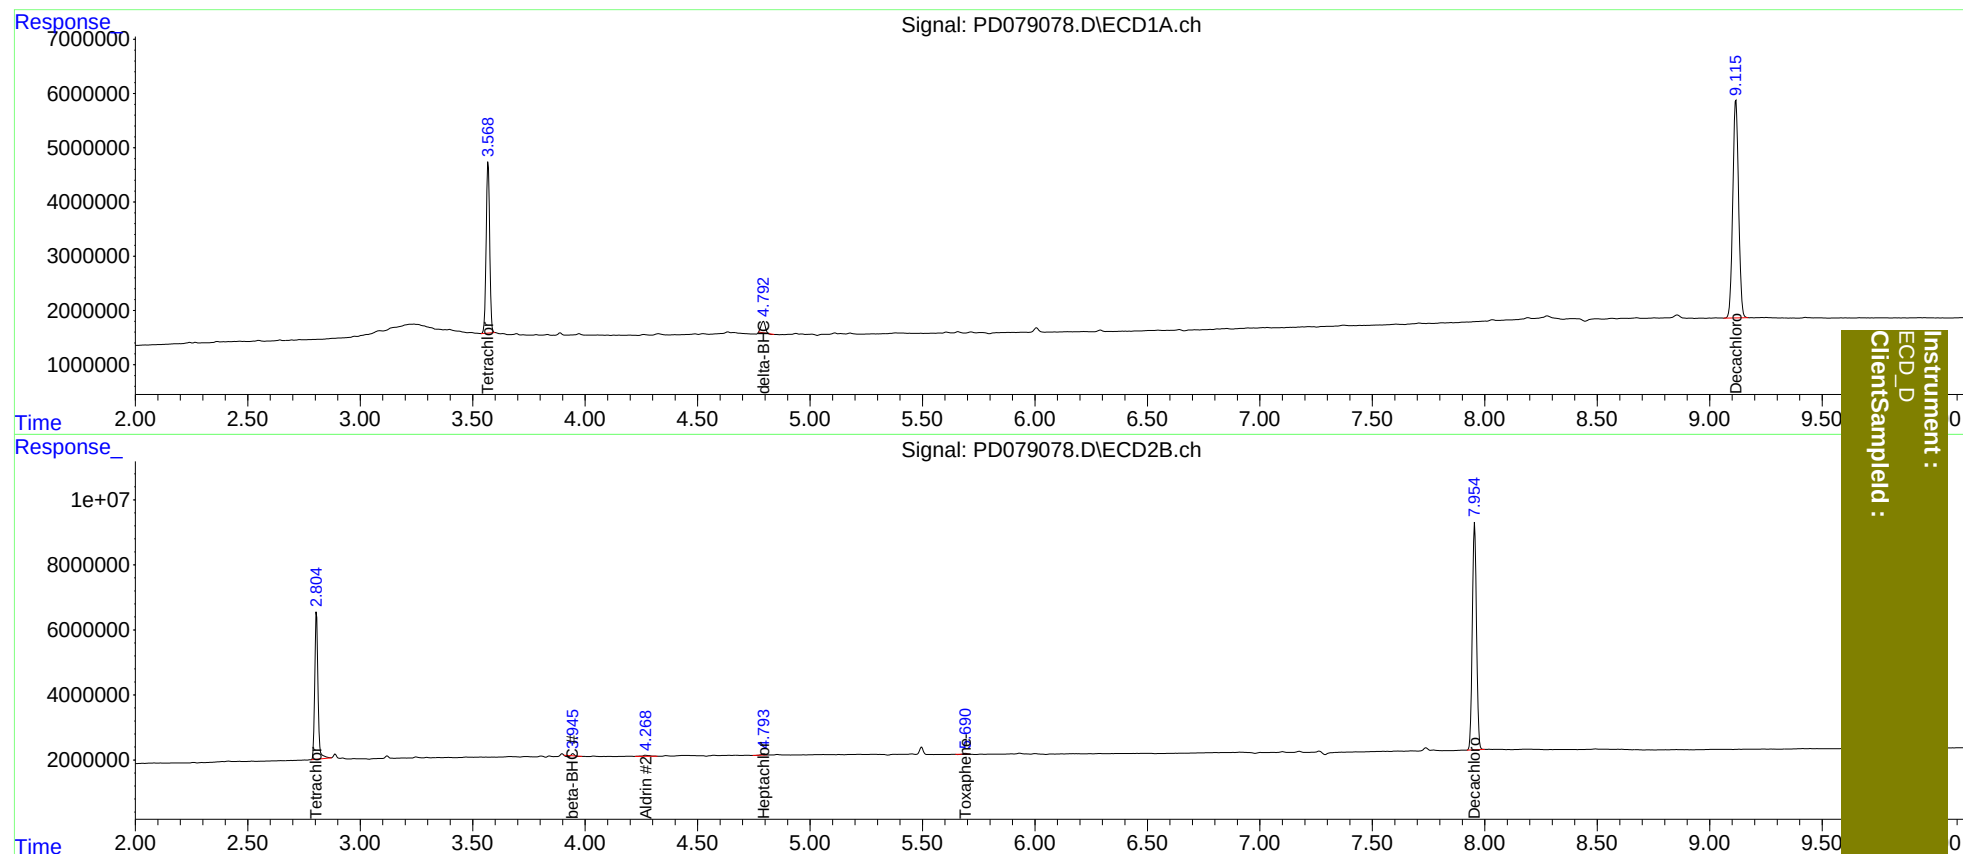


Instrument :
ECD_D
ClientSampled :
0

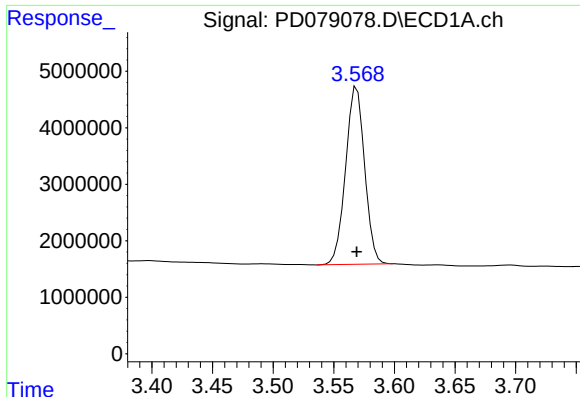

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 34315699
Conc: 22.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

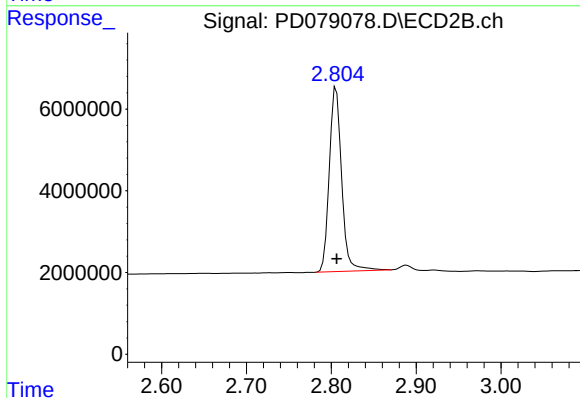


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 45713602
Conc: 21.08 ng/ml

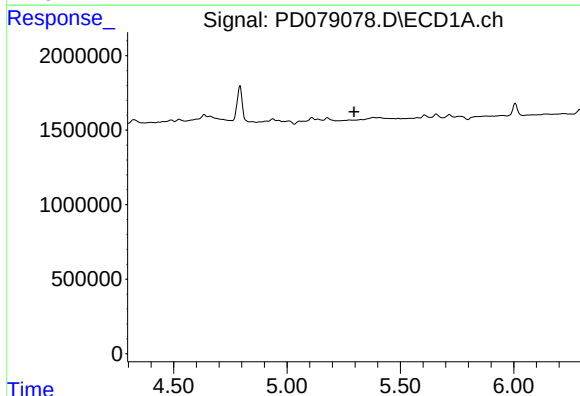


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.296 min
Response: 0
Conc: N.D.

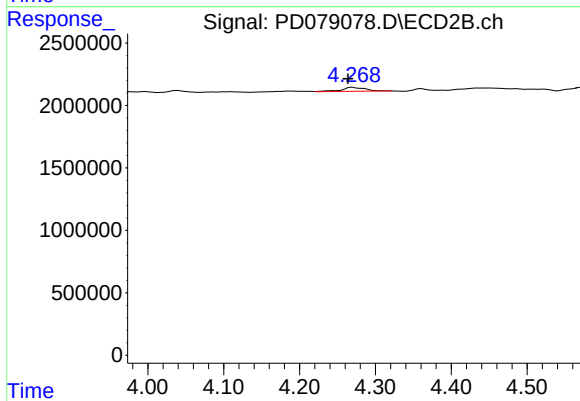

#5 Aldrin


R.T.: 4.270 min
Delta R.T.: 0.006 min
Response: 704772
Conc: 0.23 ng/ml

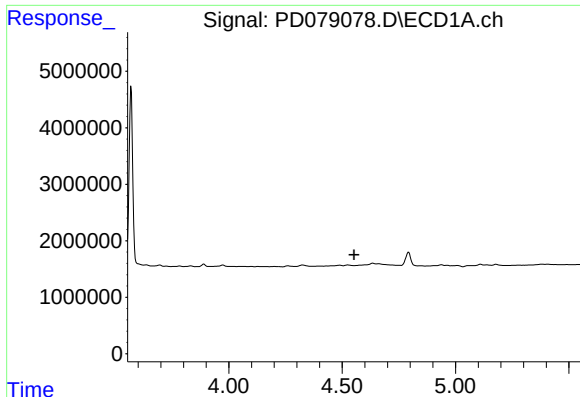

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

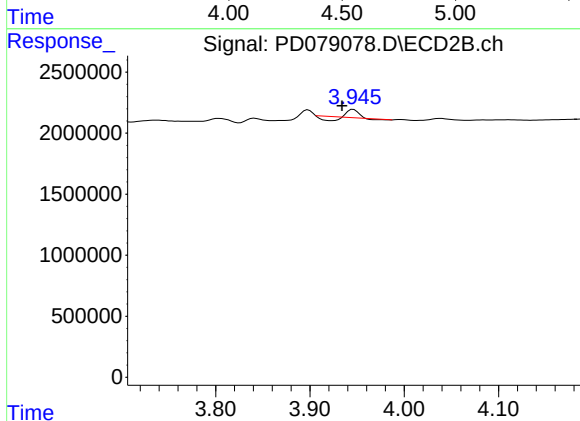


#6 beta-BHC

R.T.: 3.946 min
Delta R.T.: 0.012 min
Response: 224975
Conc: 0.16 ng/ml

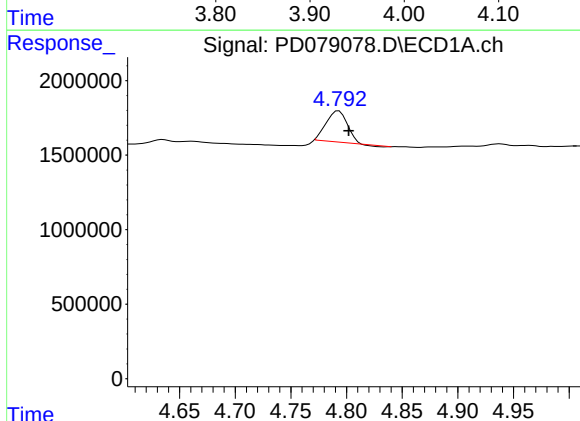


#7 delta-BHC

R.T.: 4.793 min
Delta R.T.: -0.009 min
Response: 2612010
Conc: 1.00 ng/ml

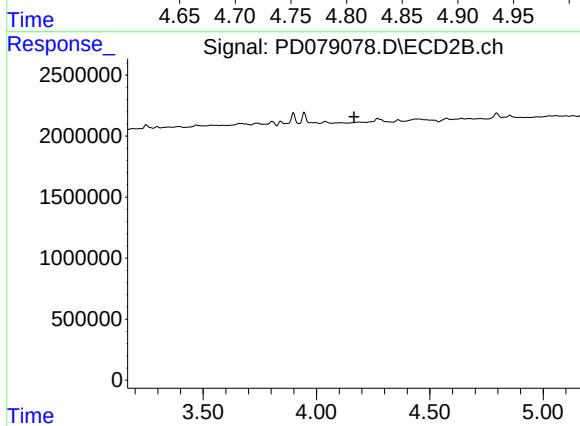

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.166 min
Response: 0
Conc: N.D.

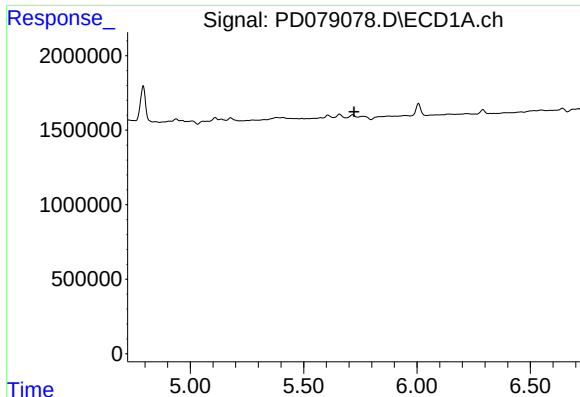

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.723 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

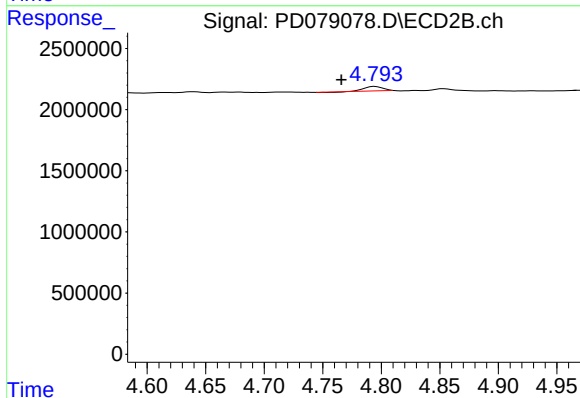


#8 Heptachlor epoxide

R.T.: 4.795 min
Delta R.T.: 0.029 min
Response: 398936
Conc: 0.14 ng/ml

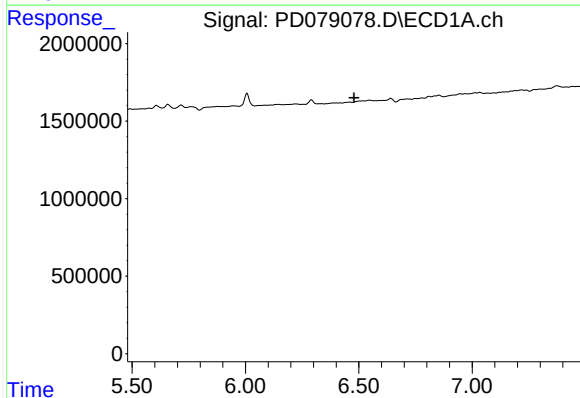


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

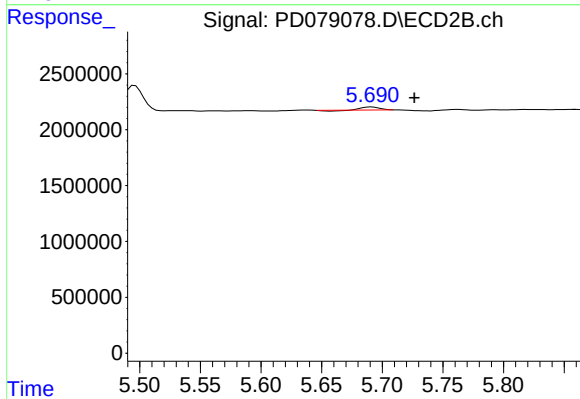

#23 Toxaphene-2


R.T.: 5.691 min
Delta R.T.: -0.035 min
Response: 238233
Conc: 14.50 ng/ml

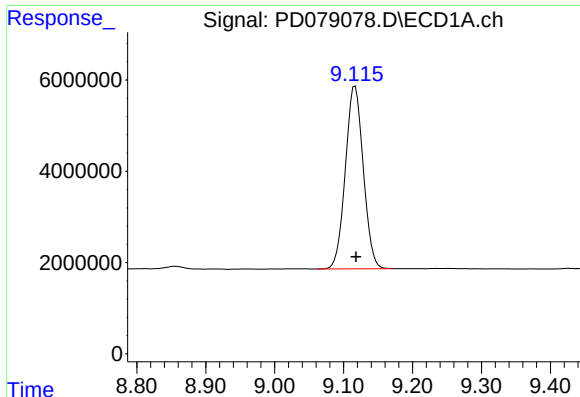

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: -0.002 min
Response: 72374359
Conc: 38.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

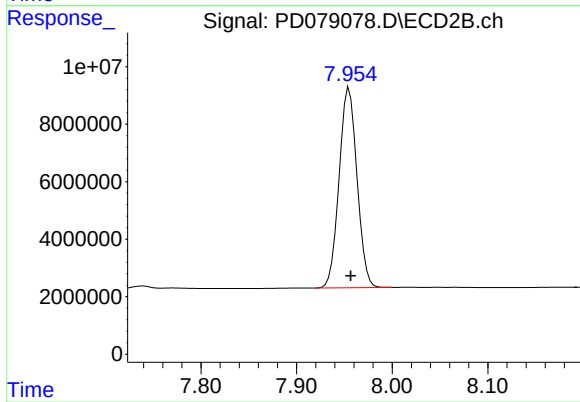

#27 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: -0.002 min
Response: 90636536
Conc: 38.86 ng/ml