

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102323\
 Data File : PD079070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2023 09:15
 Operator : AR\AJ
 Sample : 04952-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAR0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/24/2023
 Supervised By : Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 21:38:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	24754930	34231550	16.141	15.786
2)	SA Decachlor...	9.118	7.954	24492793	28673790	12.914	12.294
Target Compounds							
8)	B Heptachlo...	5.741	4.757	1258440	2178064	0.524m	0.755 #
14)	MA Endrin	6.607	5.688	1469174	2088755	0.776	0.828m
20)	A Methoxychlor	7.527	6.629	2968568	3461198	3.095	2.839

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102323\
Data File : PD079070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2023 09:15
Operator : AR\AJ
Sample : 04952-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 21:38:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

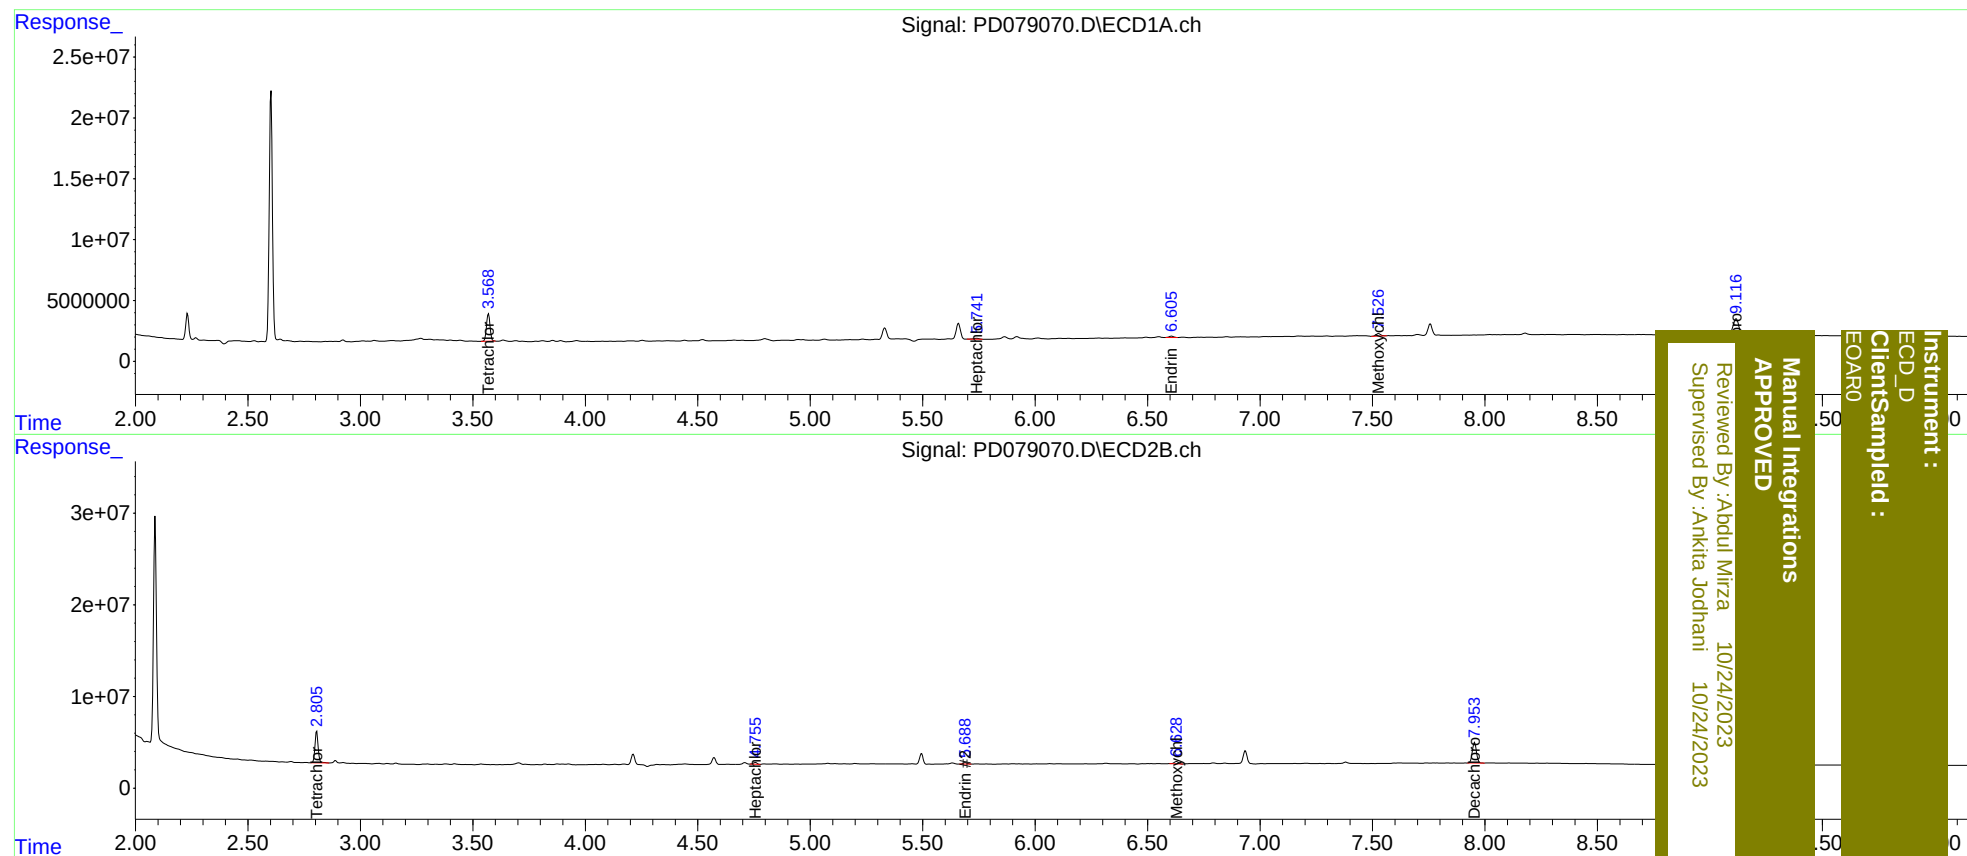

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/24/2023
Supervised By: Ankita Jodhani 10/24/2023

Instrument :
ECD_D
Client Sampled :
EOARO