

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102419\
 Data File : PD055567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 11:11
 Operator : SG\AJ
 Sample : K5482-04DL2 20X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ5DL2

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 16:24:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
27)	SA Decachlor...	7.969	8.995	1731504	2152595	1.891m	1.650m
Target Compounds							
12)	B 4,4'-DDE	5.404	6.286	1064497	1638167	1.044m	0.972
14)	MA Endrin	5.791	6.681	9080114	17327384	10.137	12.405
16)	A 4,4'-DDD	5.918	6.774	15329101	26711614	18.914	18.671
17)	MA 4,4'-DDT	6.154	7.072	57619363	109.2E6	84.985	80.551
21)	B Endrin ke...	6.919	7.681	874738	3987059	0.895m	2.489 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


mohammad

10/25/2019 8:13:12 AM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102419\
Data File : PD055567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 11:11
Operator : SG\AJ
Sample : K5482-04DL2 20X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 16:24:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

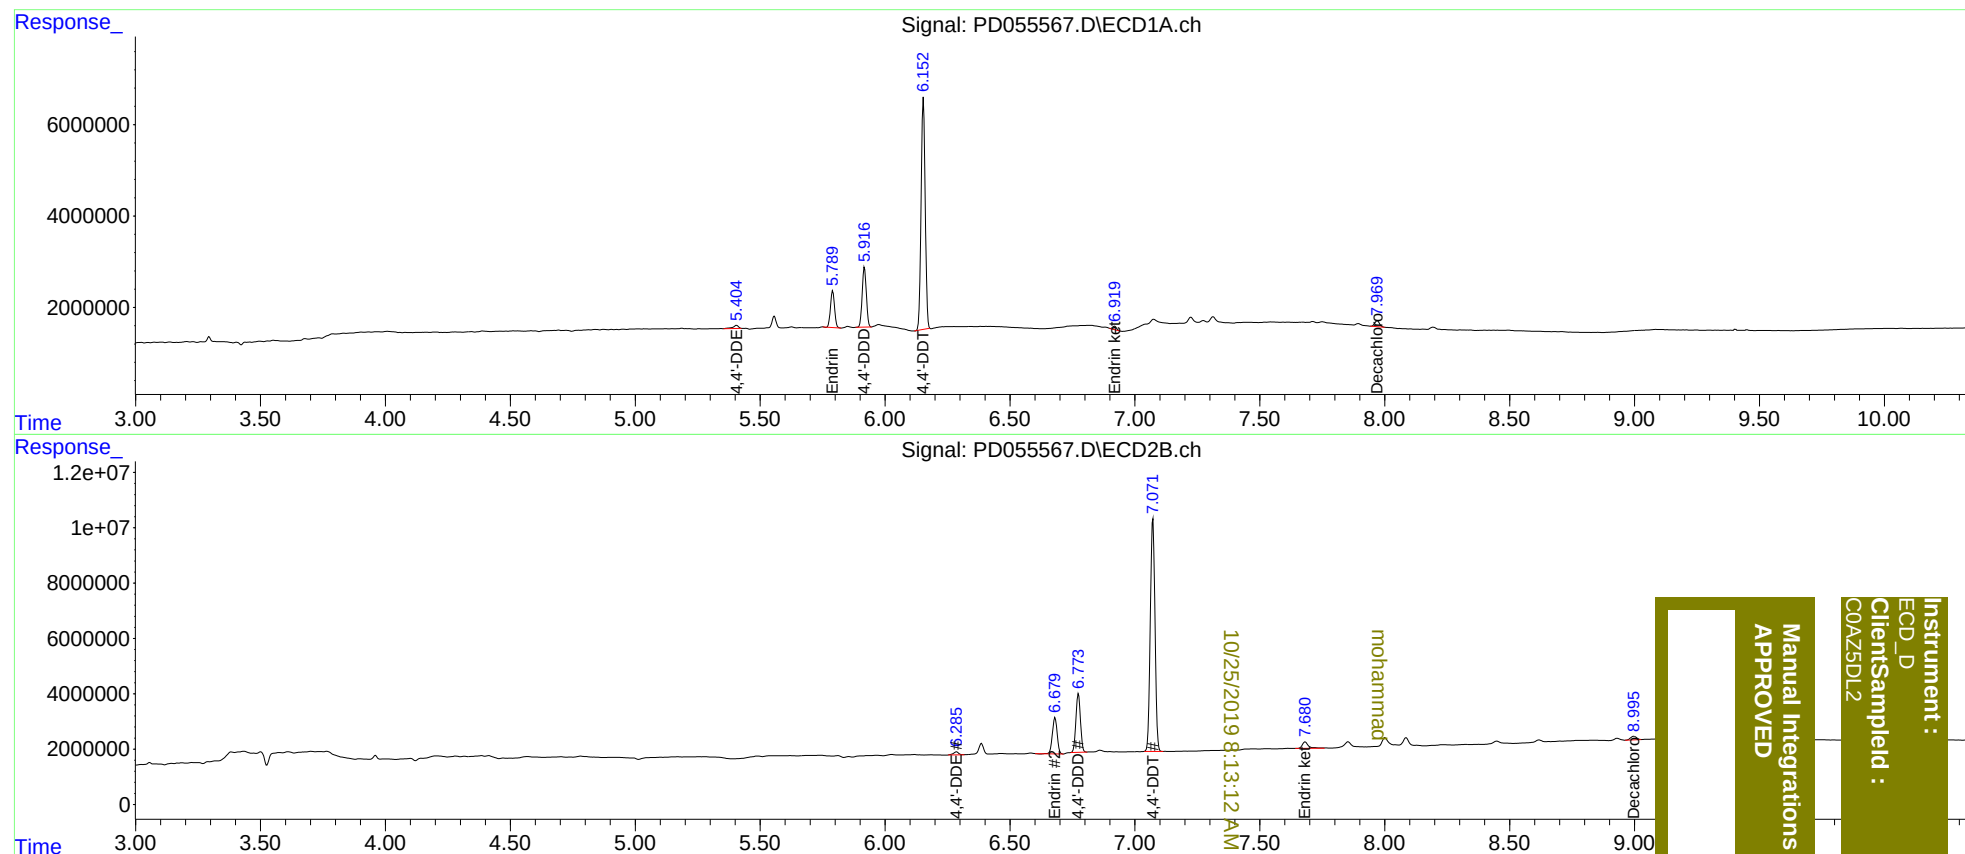

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0A25DL2