

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
 Data File : PD072588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 16:07
 Operator : AR\AJ
 Sample : N5234-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LSP-SS-03-01-03-D

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2022
 Supervised By : Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:39:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.705	3.465	28233933	234.6E6	11.332m	7.055m#
28) SA Decachlor...	7.839	8.921	28674336	135.2E6	12.740	15.025

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
Data File : PD072588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 16:07
Operator : AR\AJ
Sample : N5234-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
LSP-SS-03-01-03-D


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2022
Supervised By : Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:39:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

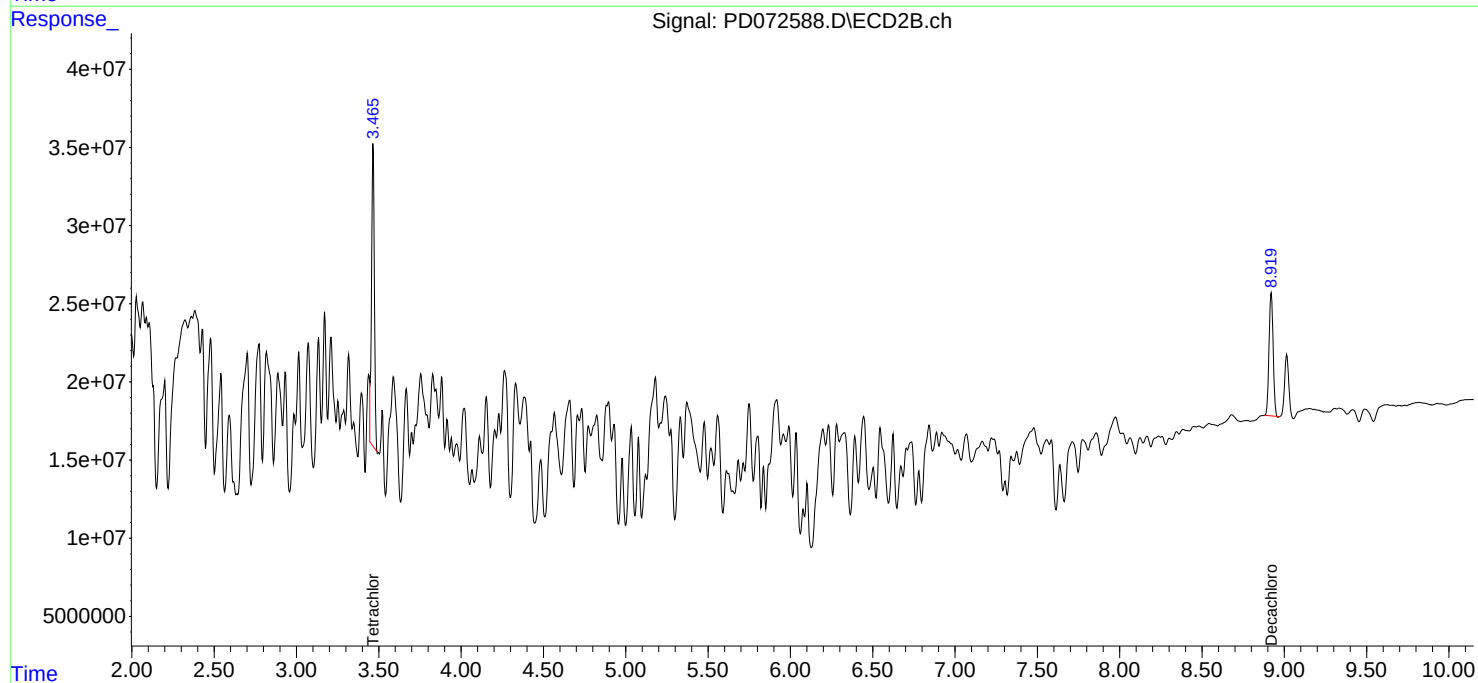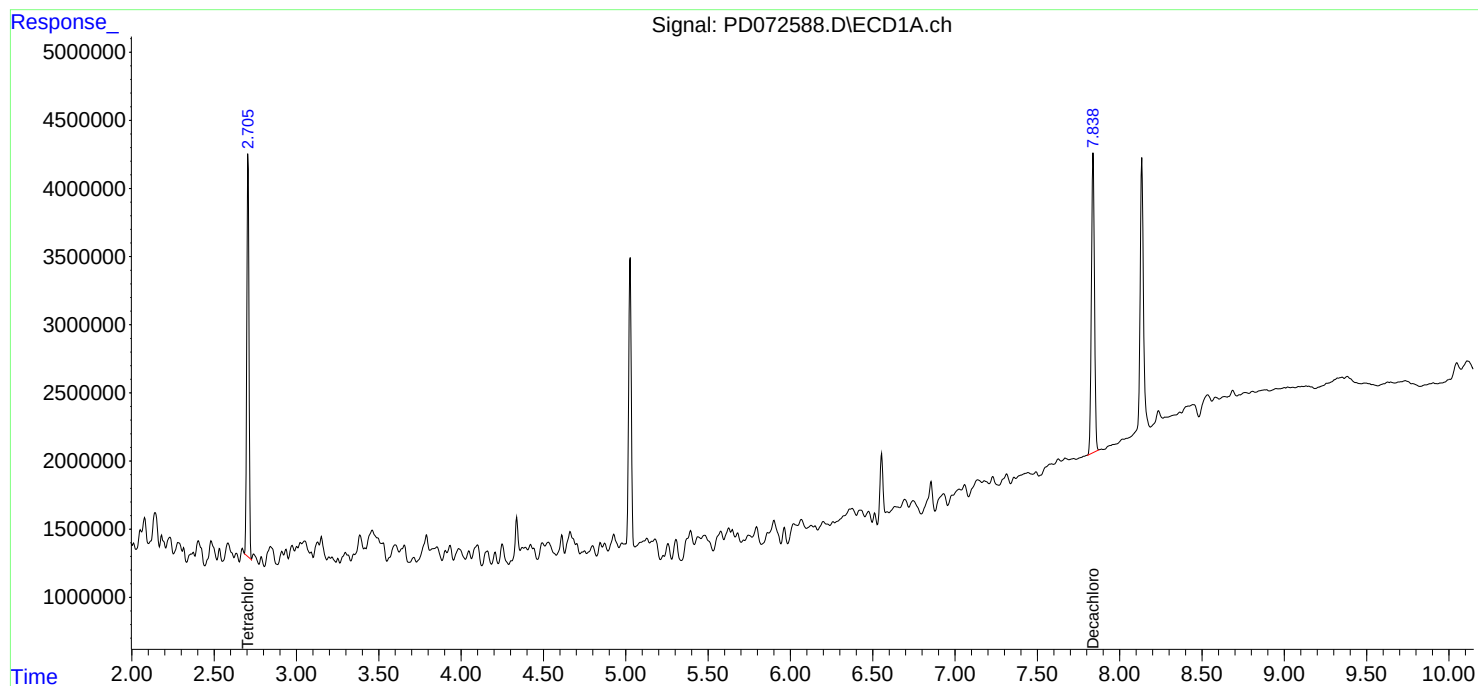

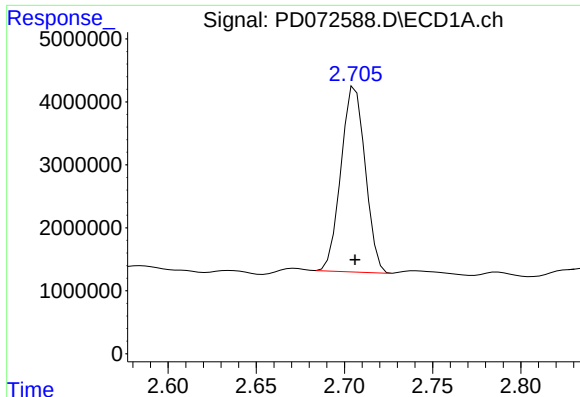


#1 Tetrachloro-m-xylene

R.T.: 2.705 min
Delta R.T.: -0.001 min
Response: 28233933
Conc: 11.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
LSP-SS-03-01-03-D


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

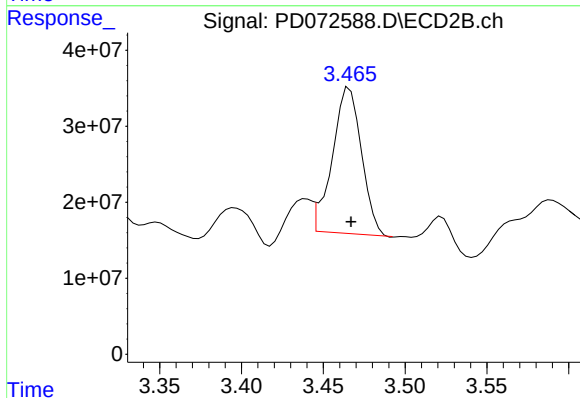


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: -0.002 min
Response: 234614115
Conc: 7.05 ng/ml m

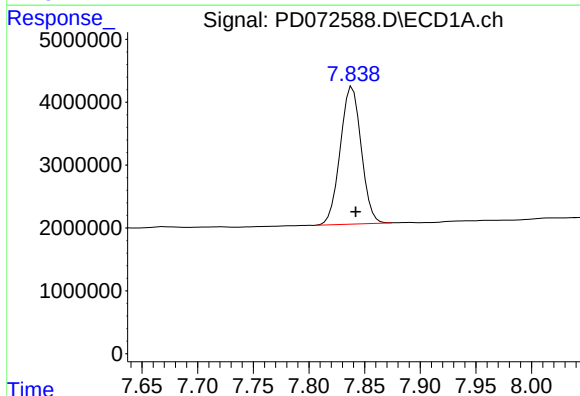

#28 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: -0.003 min
Response: 28674336
Conc: 12.74 ng/ml

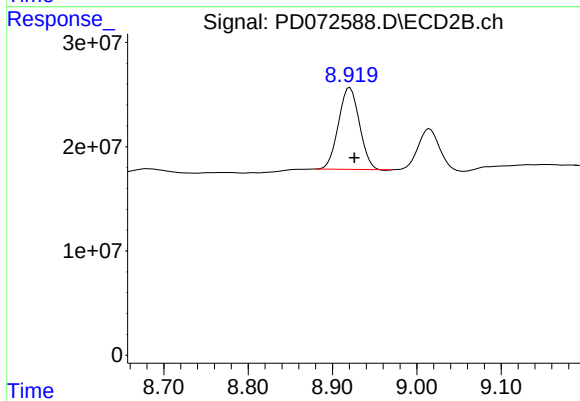

#28 Decachlorobiphenyl

R.T.: 8.921 min
Delta R.T.: -0.005 min
Response: 135177343
Conc: 15.02 ng/ml