

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
 Data File : PD072589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 16:24
 Operator : AR\AJ
 Sample : N5234-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LSP-SS-04-05-15

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2022
 Supervised By : Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:39:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.709	3.464	32028115	403.5E6	12.854m	12.134
2) SA Decachlor...	7.841	8.921	26625399	126.6E6	11.830	14.076

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
Data File : PD072589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 16:24
Operator : AR\AJ
Sample : N5234-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
LSP-SS-04-05-15


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2022
Supervised By : Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:39:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

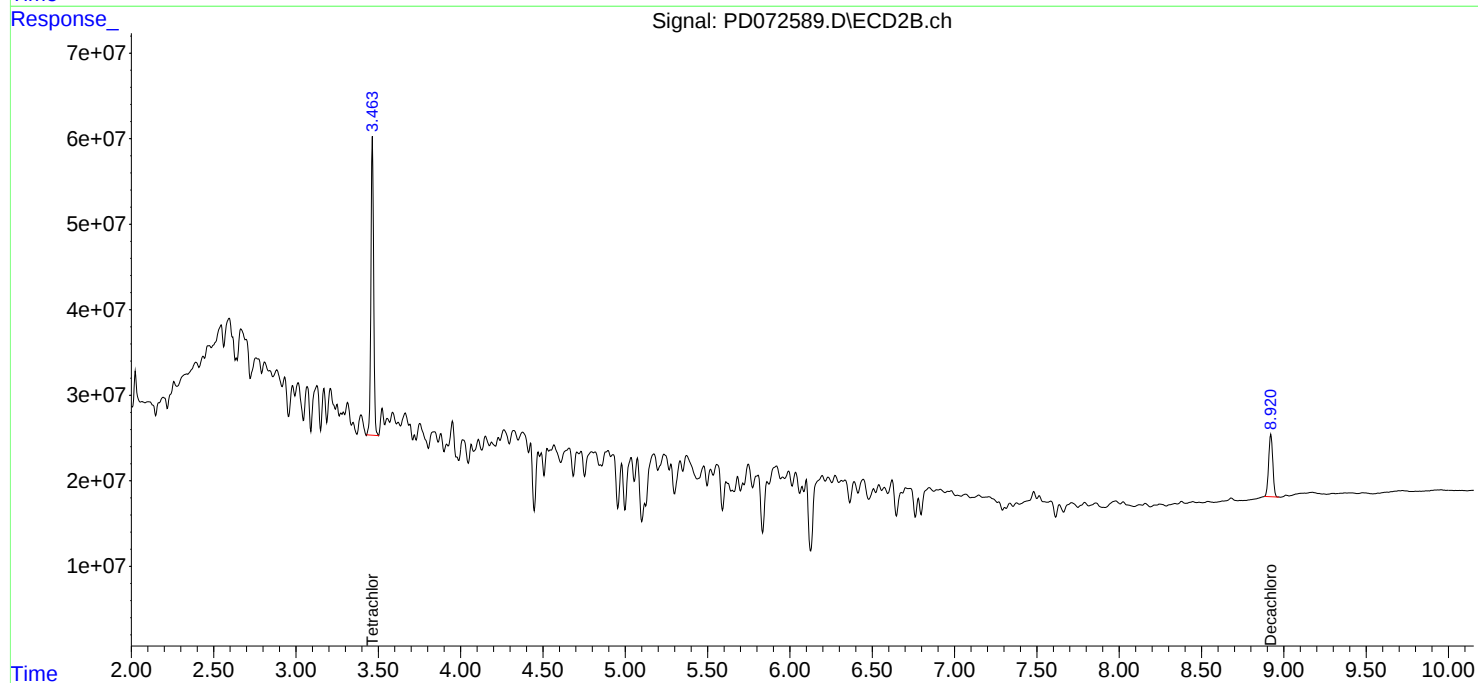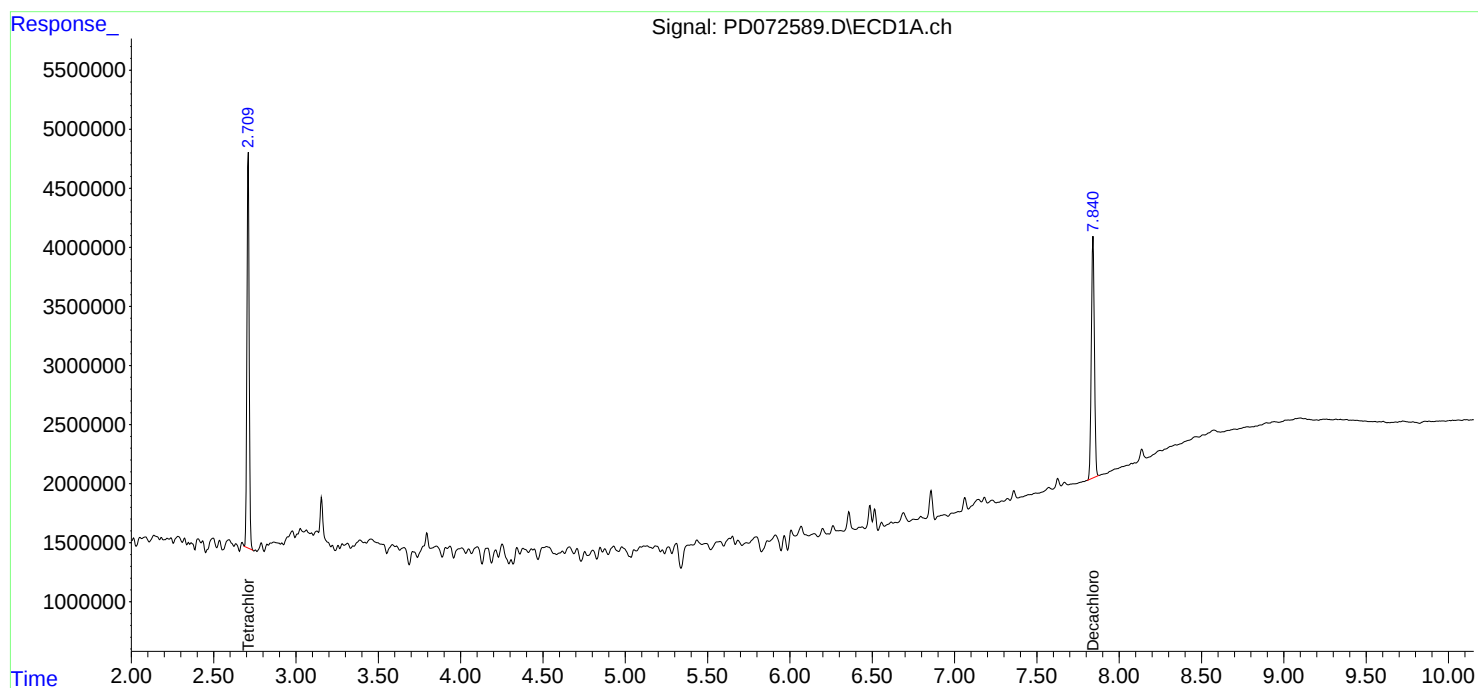

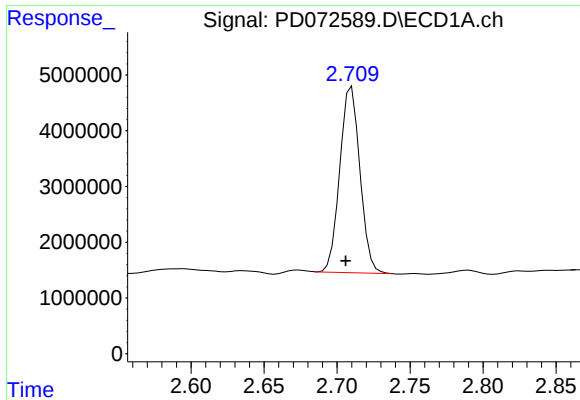


#1 Tetrachloro-m-xylene

R.T.: 2.709 min
Delta R.T.: 0.003 min
Response: 32028115
Conc: 12.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
LSP-SS-04-05-15


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

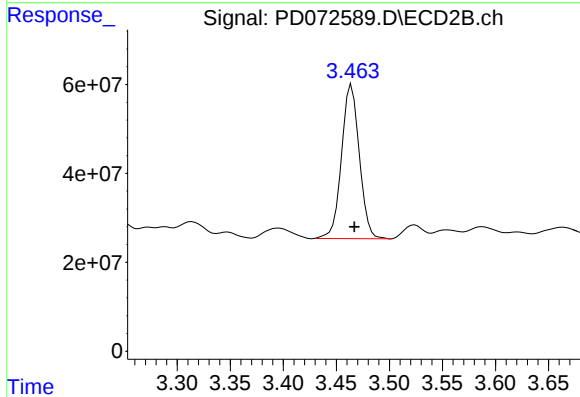


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.003 min
Response: 403529696
Conc: 12.13 ng/ml

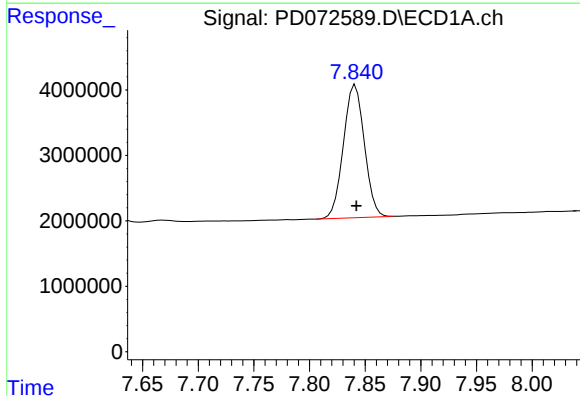

#28 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 26625399
Conc: 11.83 ng/ml

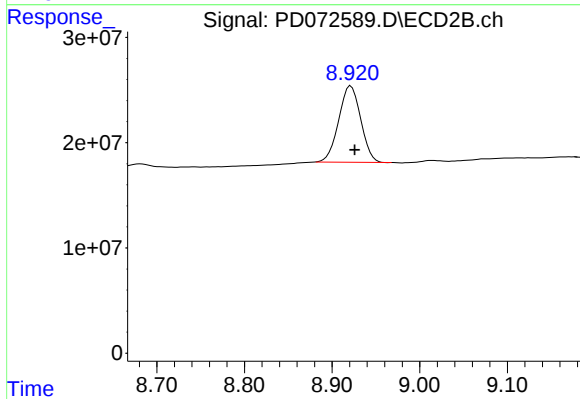

#28 Decachlorobiphenyl

R.T.: 8.921 min
Delta R.T.: -0.005 min
Response: 126642439
Conc: 14.08 ng/ml