

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
 Data File : PD072593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 17:17
 Operator : AR\AJ
 Sample : N5234-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LSP-SS-07-20-40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:43:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	33402399	464.6E6	13.406	13.969
28)	SA Decachlor...	7.837	8.920	24869862	119.3E6	11.050	13.260

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
Data File : PD072593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 17:17
Operator : AR\AJ
Sample : N5234-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LSP-SS-07-20-40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:43:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

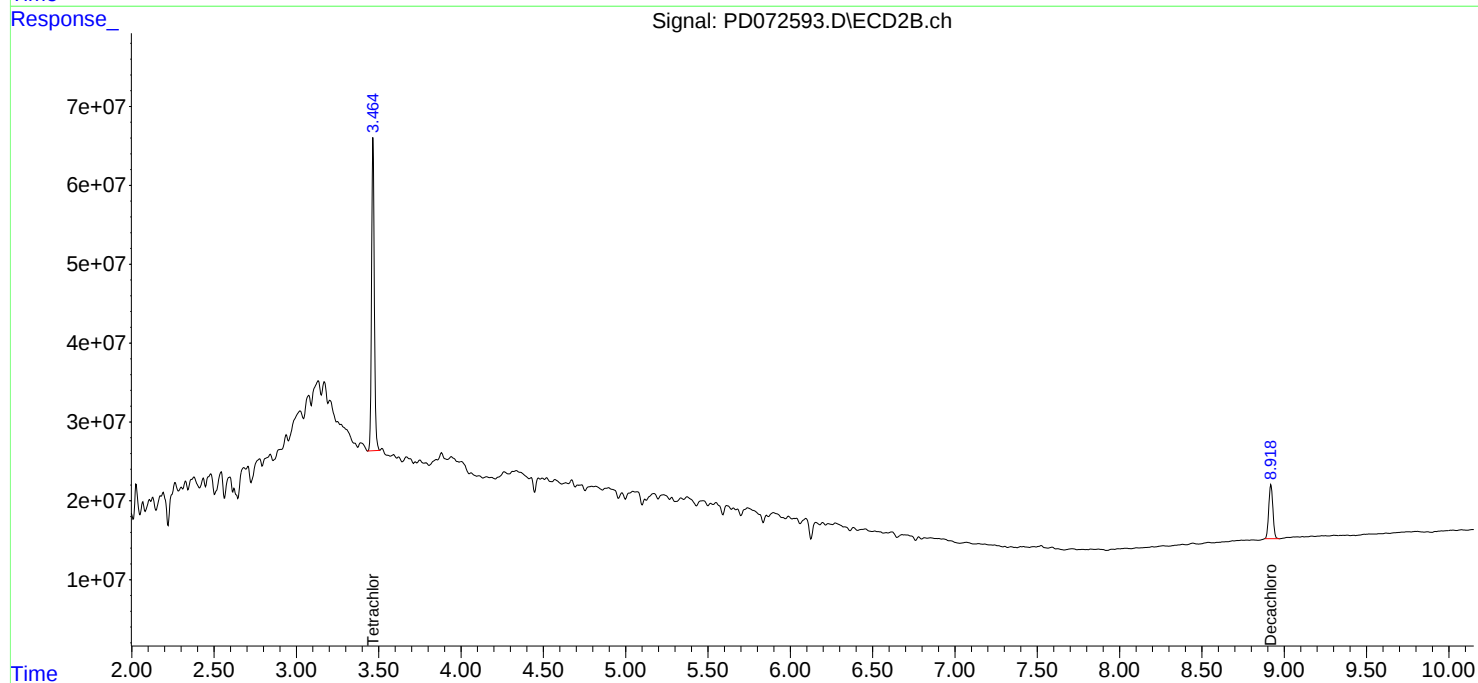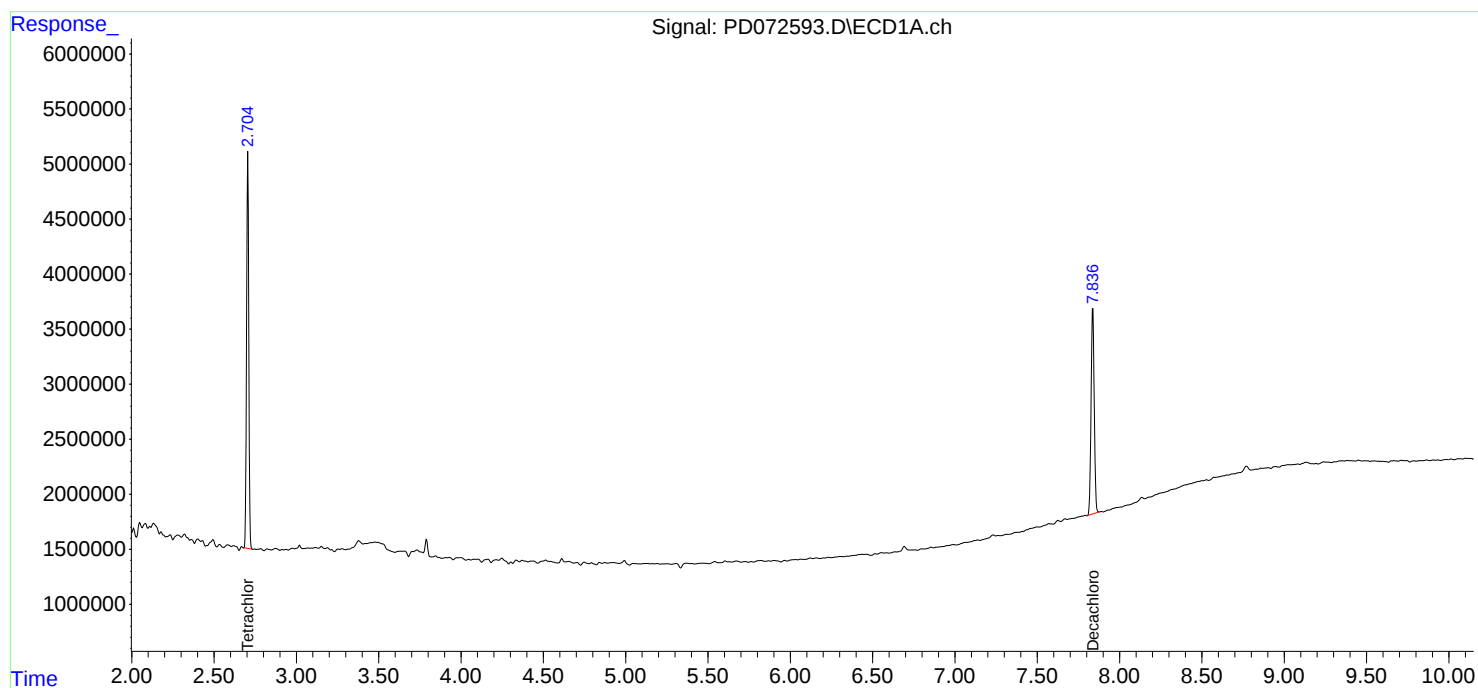


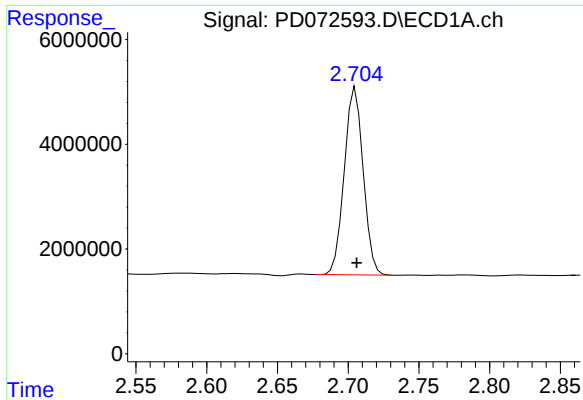

#1 Tetrachloro-m-xylene


R.T.: 2.705 min
Delta R.T.: 0.000 min
Response: 33402399
Conc: 13.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
LSP-SS-07-20-40

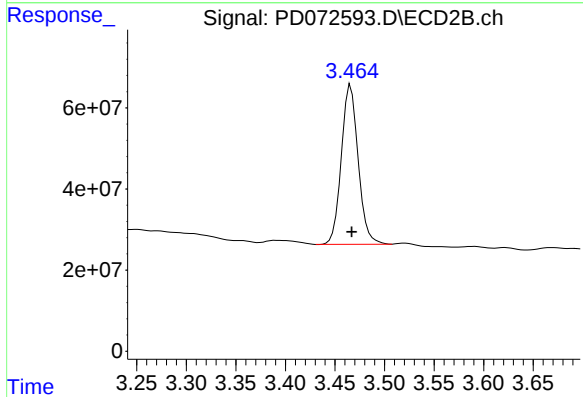


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.001 min
Response: 464566877
Conc: 13.97 ng/ml

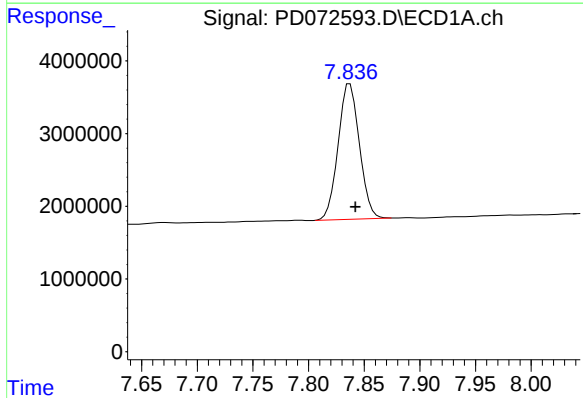

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: -0.005 min
Response: 24869862
Conc: 11.05 ng/ml

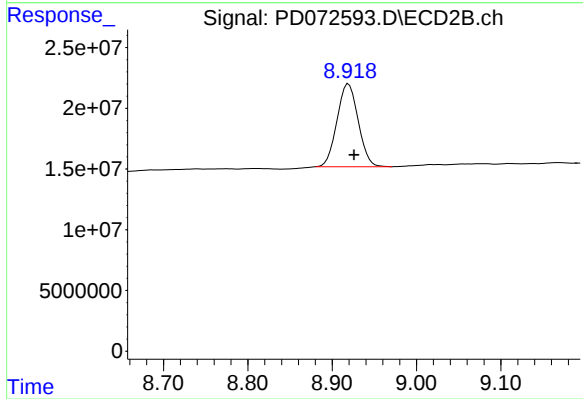

#28 Decachlorobiphenyl

R.T.: 8.920 min
Delta R.T.: -0.006 min
Response: 119298599
Conc: 13.26 ng/ml