

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
 Data File : PD072595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 17:44
 Operator : AR\AJ
 Sample : N5235-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LSP-SS-02-03-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:55:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.706	3.466	34457320	495.1E6	13.829	14.887
28) SA Decachlor...	7.837	8.920	26862079	129.4E6	11.935	14.382

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102422\
Data File : PD072595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 17:44
Operator : AR\AJ
Sample : N5235-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LSP-SS-02-03-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:55:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

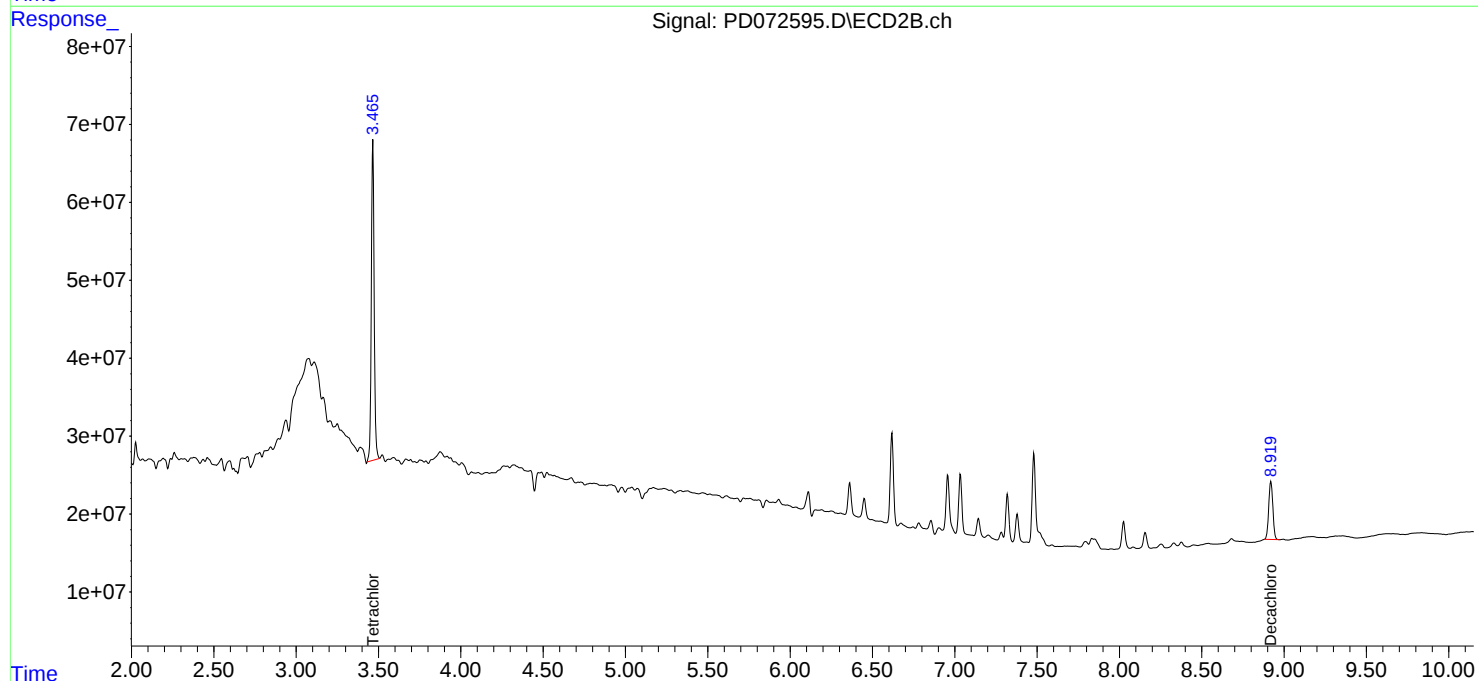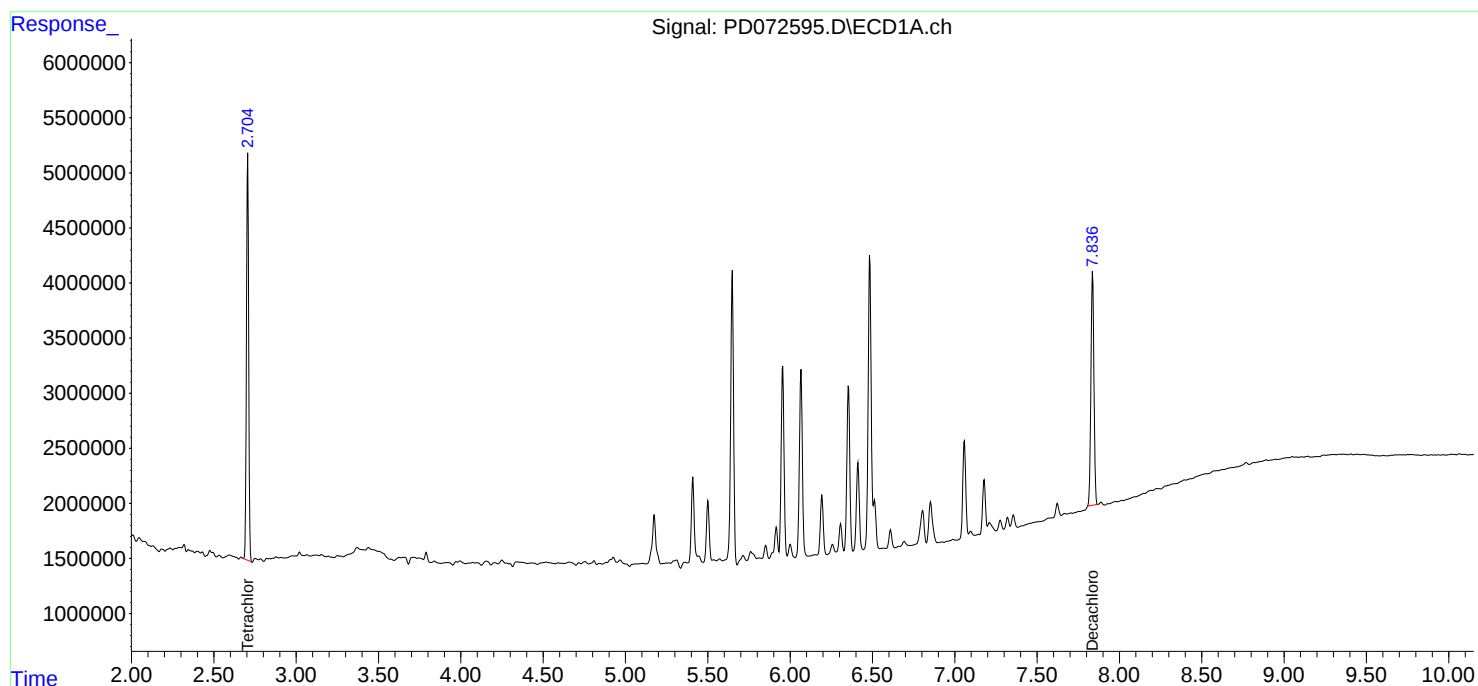


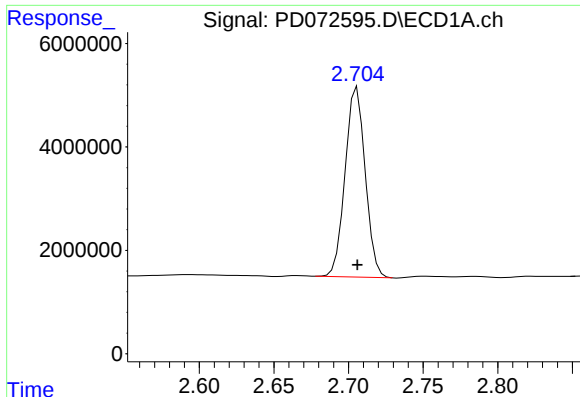

#1 Tetrachloro-m-xylene


R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 34457320
Conc: 13.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
LSP-SS-02-03-05

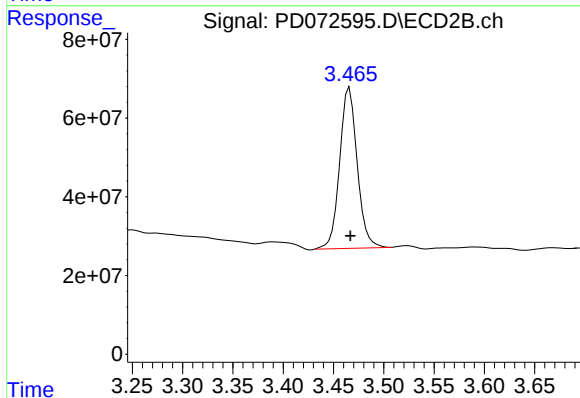


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.001 min
Response: 495083654
Conc: 14.89 ng/ml

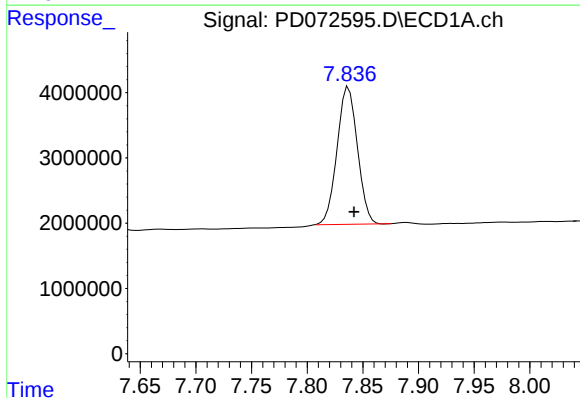

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: -0.005 min
Response: 26862079
Conc: 11.93 ng/ml

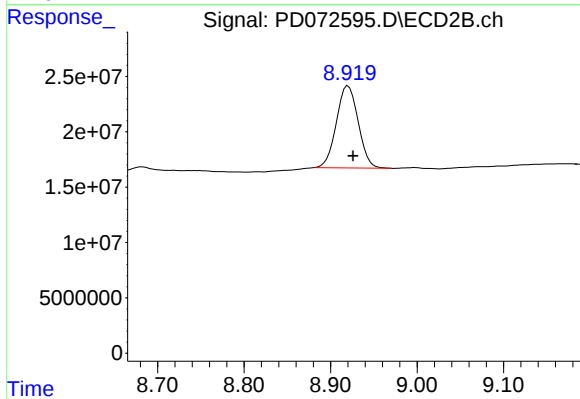

#28 Decachlorobiphenyl

R.T.: 8.920 min
Delta R.T.: -0.006 min
Response: 129395636
Conc: 14.38 ng/ml