

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
 Data File : PD079081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 08:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:17:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.798	0	99106	N.D.	<MDL
Target Compounds						
2) A alpha-BHC	0.000	3.345f	0	33475	N.D.	<MDL
3) MA gamma-BHC...	0.000	3.660	0	88466	N.D.	<MDL
4) MA Heptachlor	0.000	4.031f	0	56208	N.D.	<MDL
5) MB Aldrin	0.000	4.282	0	18167	N.D.	<MDL
12) B 4,4'-DDE	0.000	5.218f	0	205642	N.D.	<MDL
14) MA Endrin	0.000	5.689	0	500389	N.D.	0.198
21) B Endrin ke...	0.000	6.837f	0	114758	N.D.	<MDL
22) Toxaphene-1	5.852f	0.000	292478	0	40.844	N.D. #
23) Toxaphene-2	0.000	5.689f	0	500389	N.D.	30.457

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 08:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:17:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

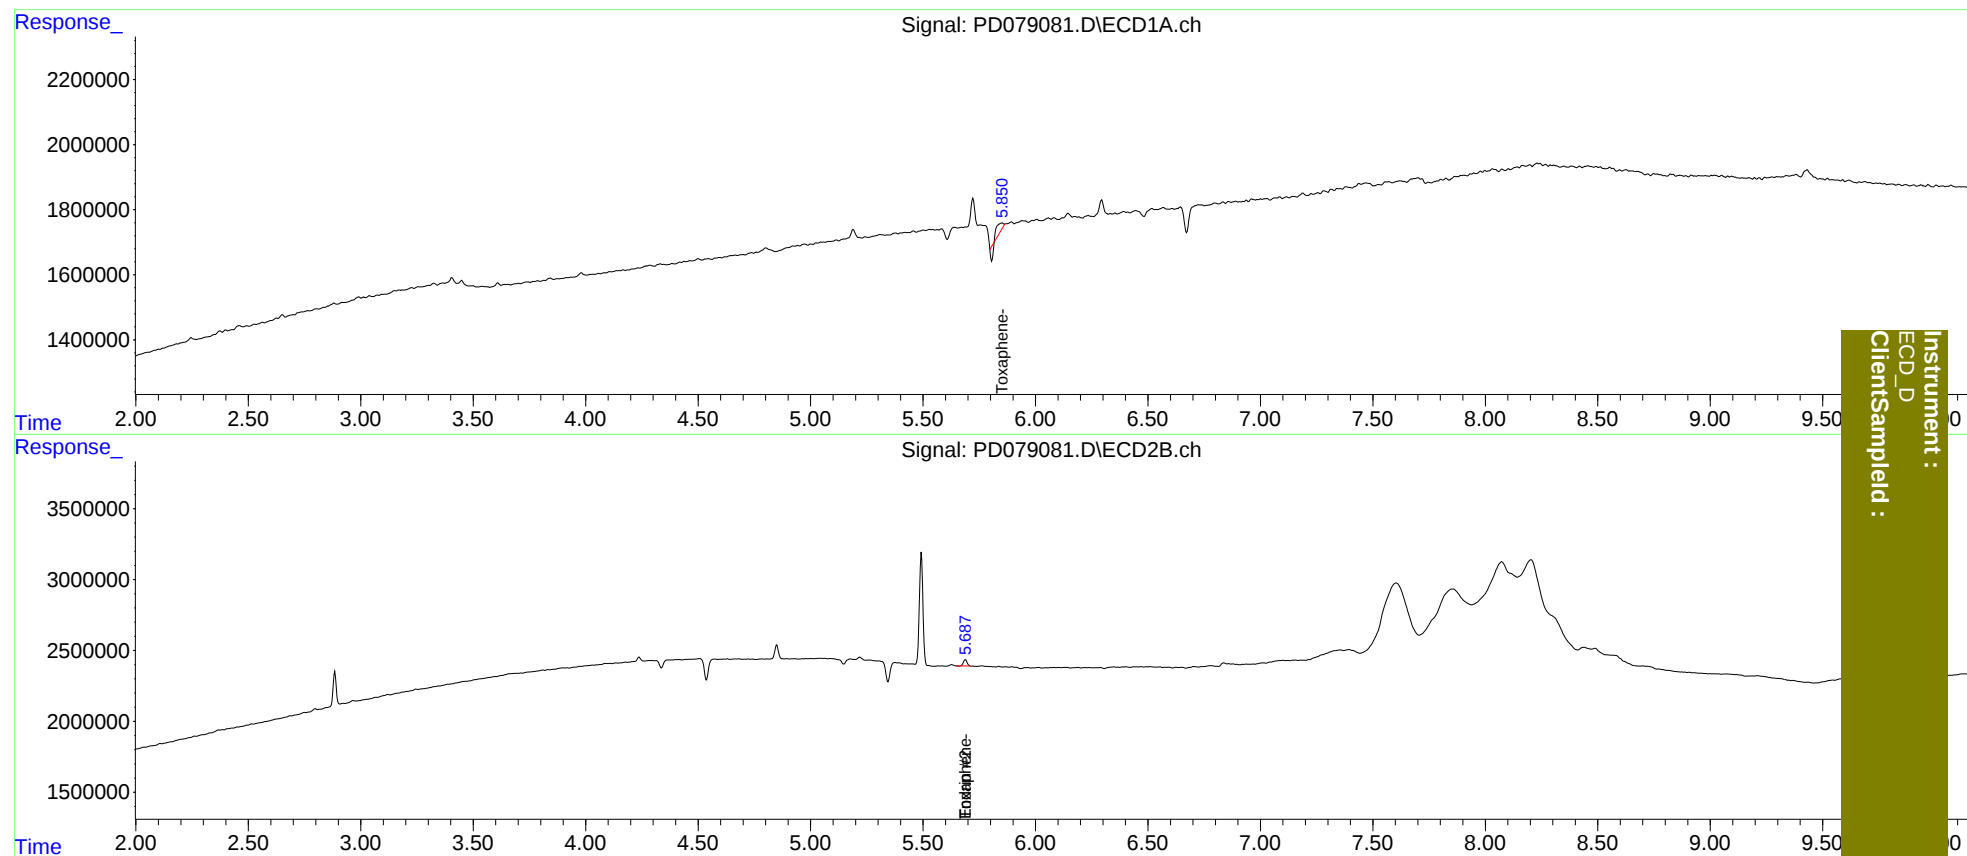


Instrument :
ECD_D
ClientSampled :
0

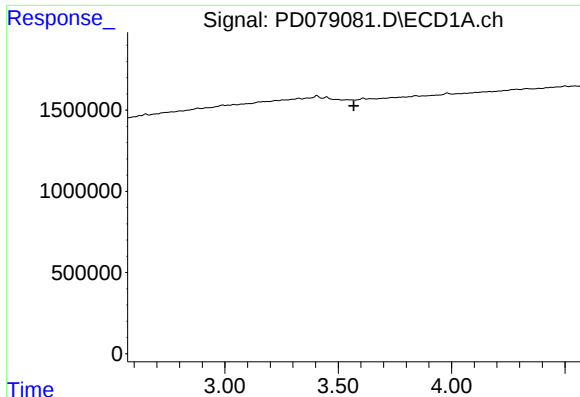

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

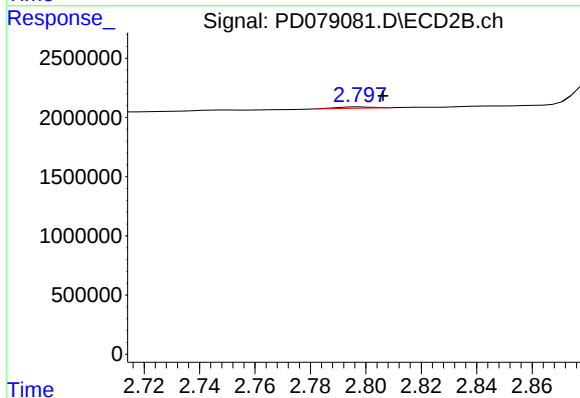


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: -0.008 min
Response: 99106
Conc: N.D.

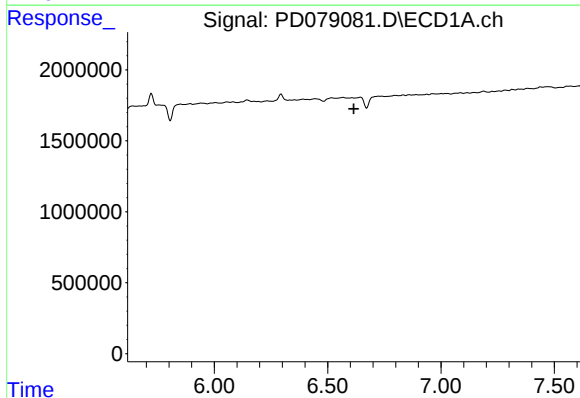


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.615 min
Response: 0
Conc: N.D.

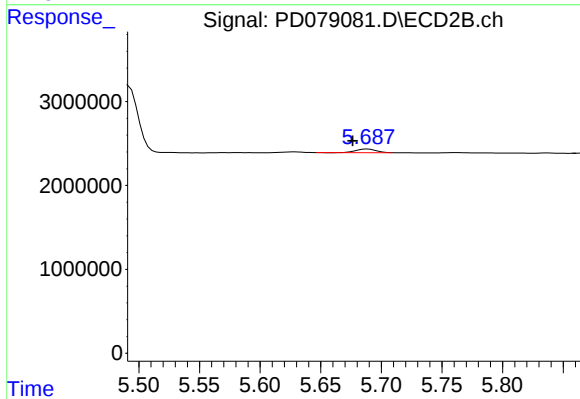

#14 Endrin


R.T.: 5.689 min
Delta R.T.: 0.012 min
Response: 500389
Conc: 0.20 ng/ml

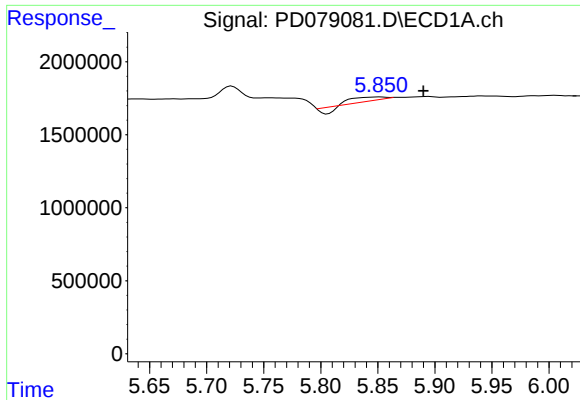

#22 Toxaphene-1


R.T.: 5.852 min
Delta R.T.: -0.038 min
Response: 292478
Conc: 40.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

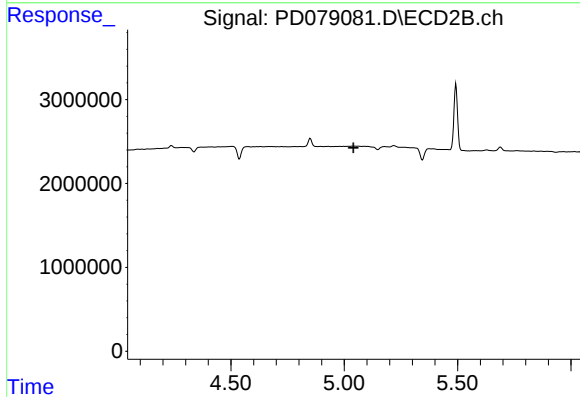


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.041 min
Response: 0
Conc: N.D.

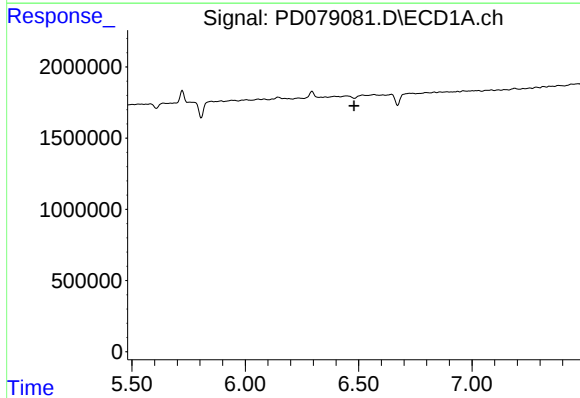


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.480 min
Response: 0
Conc: N.D.

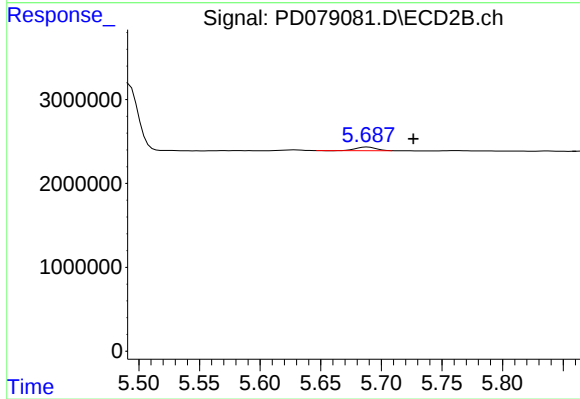

#23 Toxaphene-2


R.T.: 5.689 min
Delta R.T.: -0.038 min
Response: 500389
Conc: 30.46 ng/ml

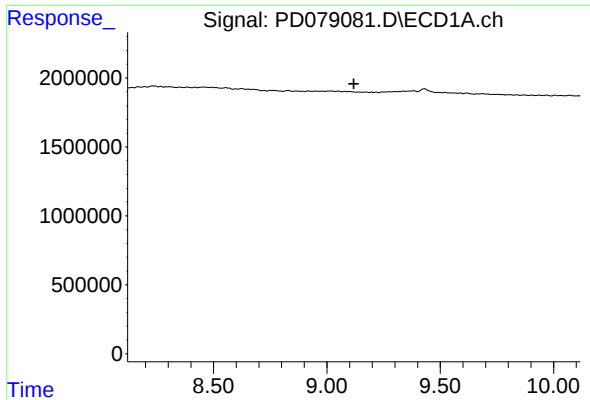

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

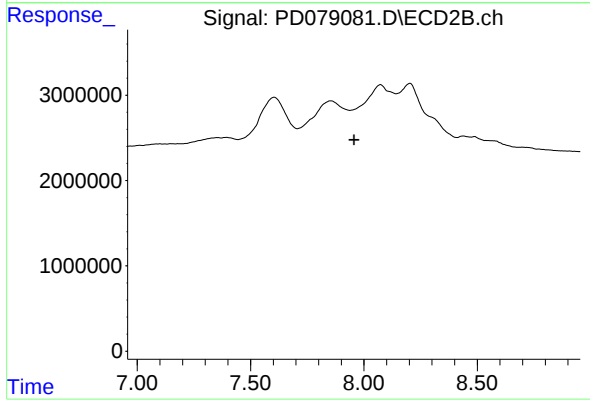

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.957 min
Response: 0
Conc: N.D.