

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
 Data File : PD079085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 11:03
 Operator : AR\AJ
 Sample : 01978-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:18:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.799	0	251681	N.D.	0.116
Target Compounds							
16)	A 4,4'-DDD	0.000	5.862f	0	138865	N.D.	<MDL
19)	B Endosulfa...	0.000	6.438f	0	135024	N.D.	<MDL
20)	A Methoxychlor	0.000	6.651	0	440265	N.D.	0.361
24)	Toxaphene-3	0.000	6.651	0	440265	N.D.	8.413
25)	Toxaphene-4	0.000	6.785	0	233360	N.D.	3.249


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 11:03
Operator : AR\AJ
Sample : 01978-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:18:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

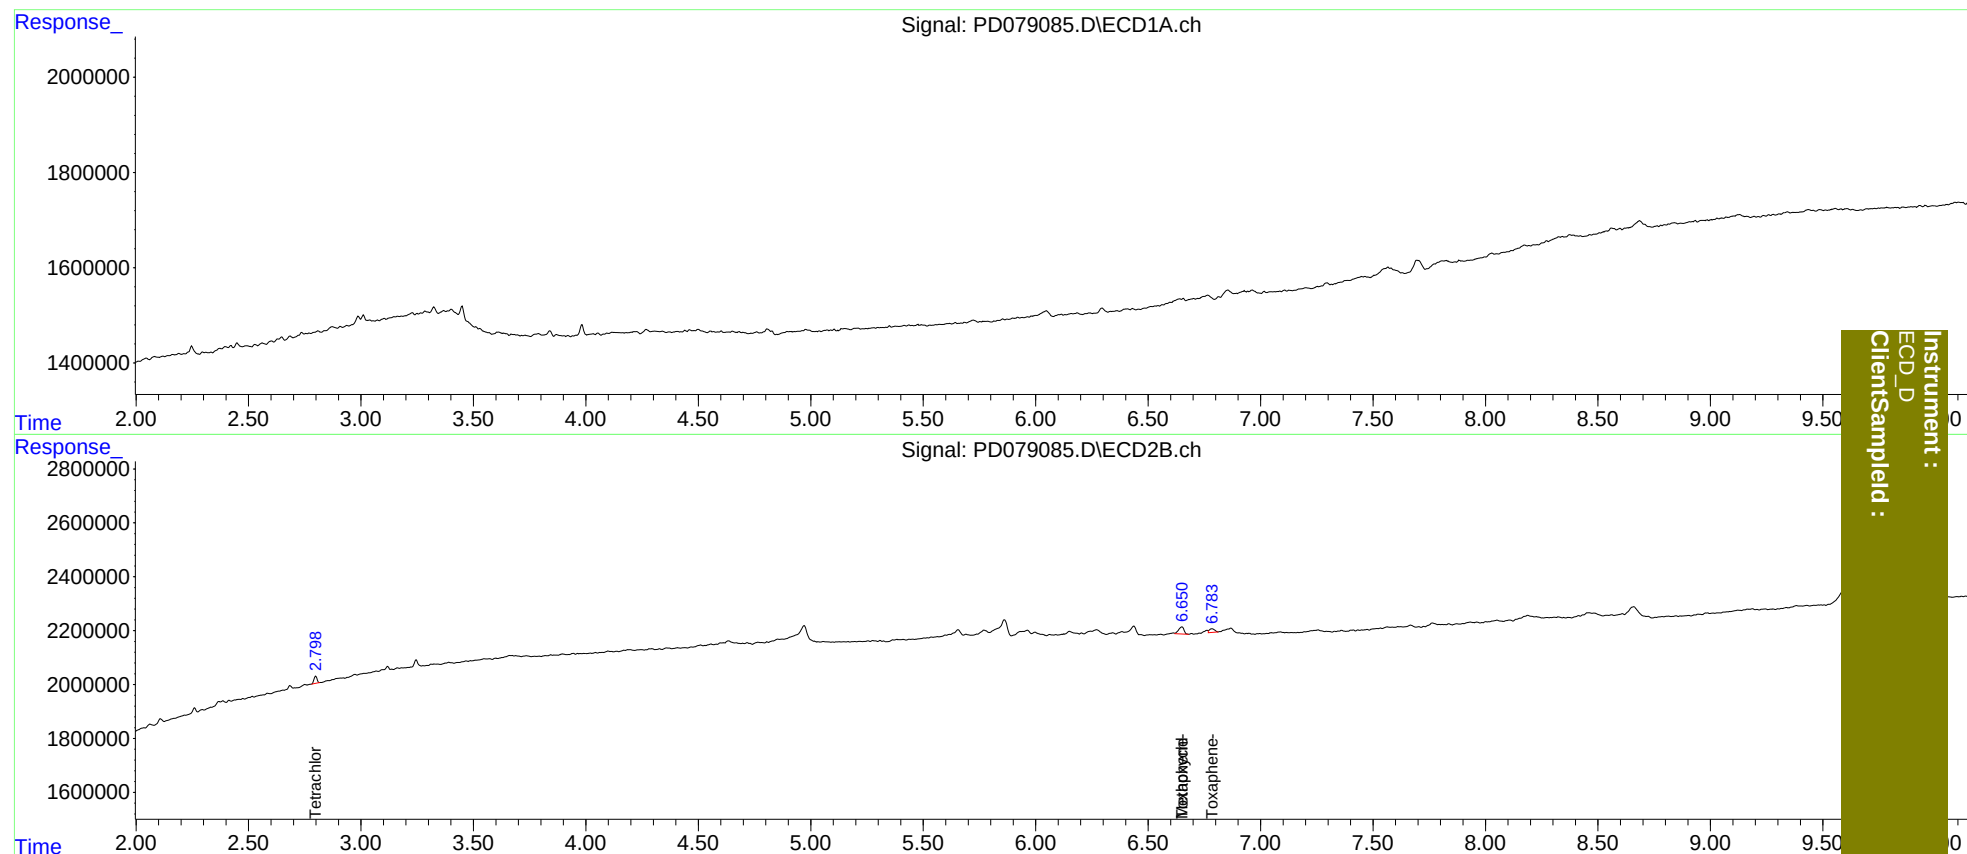


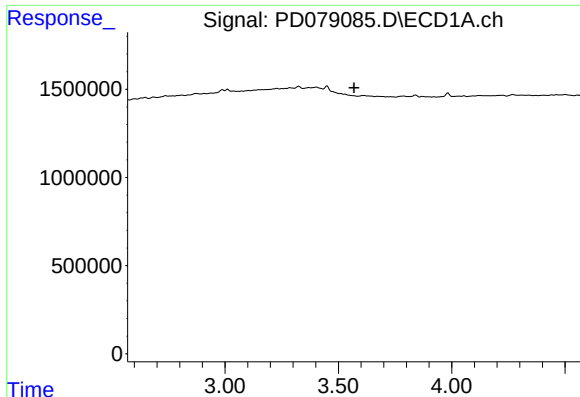

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

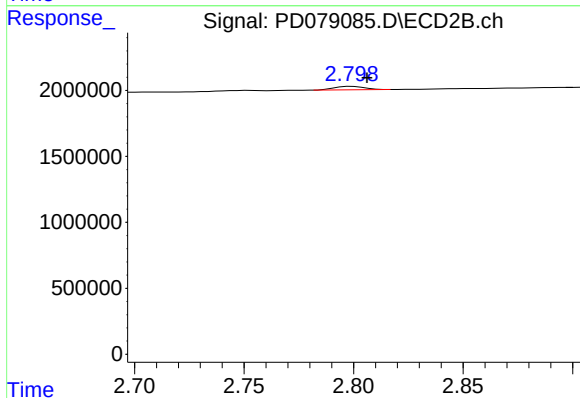


#1 Tetrachloro-m-xylene

R.T.: 2.799 min
Delta R.T.: -0.007 min
Response: 251681
Conc: 0.12 ng/ml

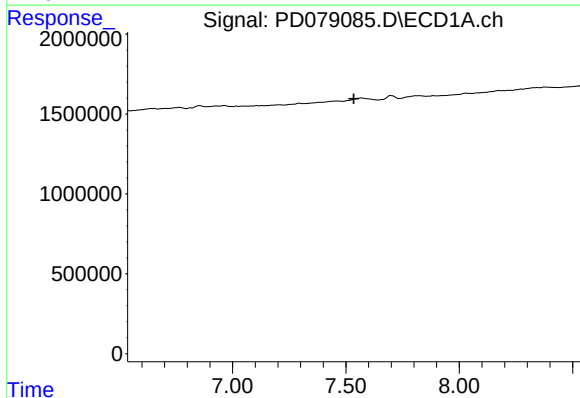


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.535 min
Response: 0
Conc: N.D.

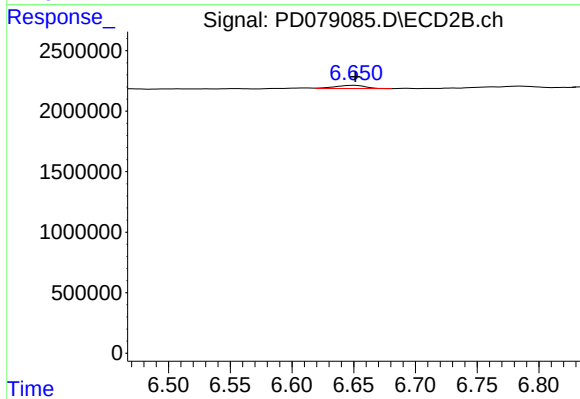

#20 Methoxychlor


R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 440265
Conc: 0.36 ng/ml

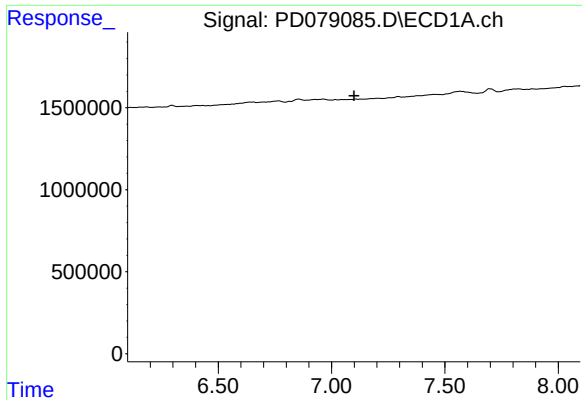

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

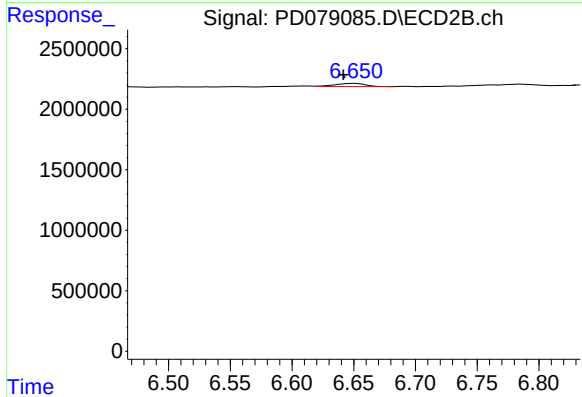


#24 Toxaphene-3

R.T.: 6.651 min
Delta R.T.: 0.009 min
Response: 440265
Conc: 8.41 ng/ml

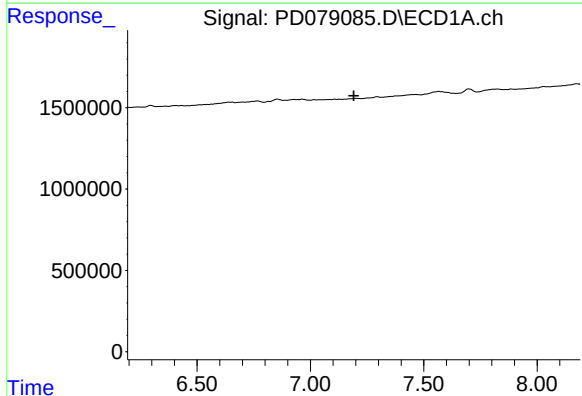


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.191 min
Response: 0
Conc: N.D.

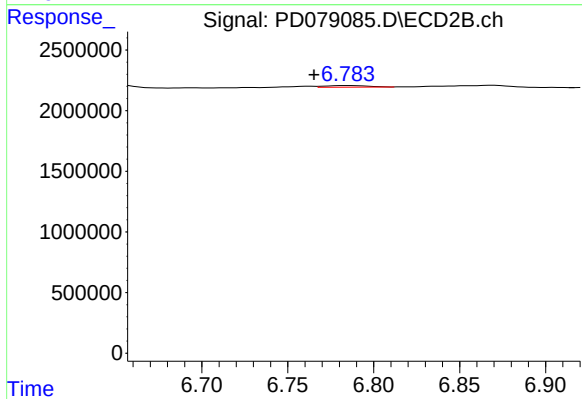

#25 Toxaphene-4


R.T.: 6.785 min
Delta R.T.: 0.019 min
Response: 233360
Conc: 3.25 ng/ml

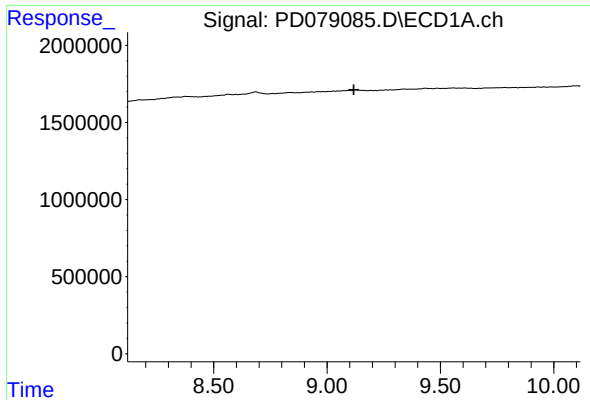

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

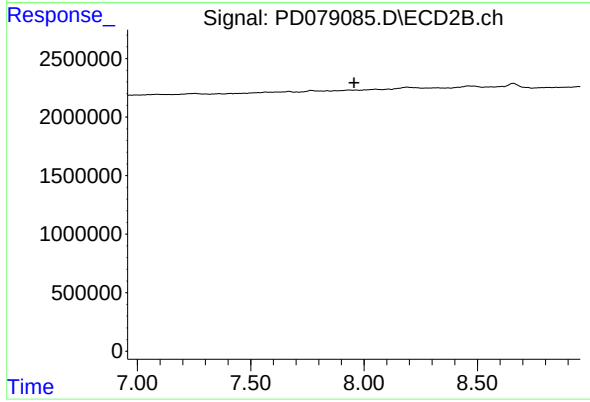

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.957 min
Response: 0
Conc: N.D.