

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 13:30
Operator : AR\AJ
Sample : 04996-05
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
A4935

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:20:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

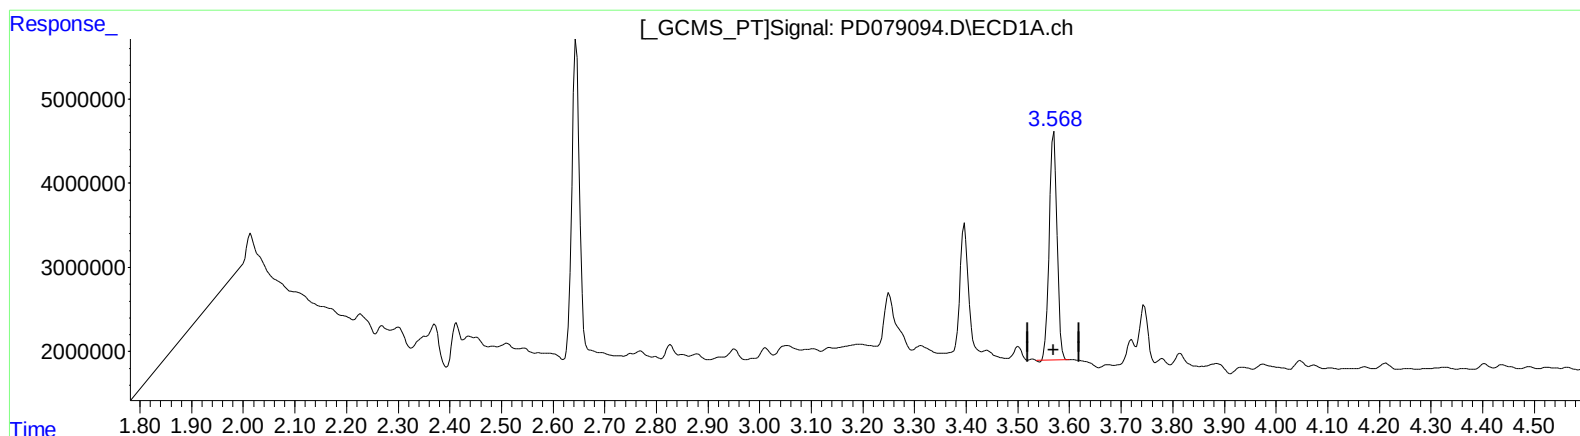

(1) Tetrachloro-m-xylene (SA)

3.570min 18.660 ng/ml

response 28617973

(1) Tetrachloro-m-xylene #2 (SA)

2.806min 20.505 ng/ml

response 44465361

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 13:30
Operator : AR\AJ
Sample : 04996-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
A4935

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:20:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

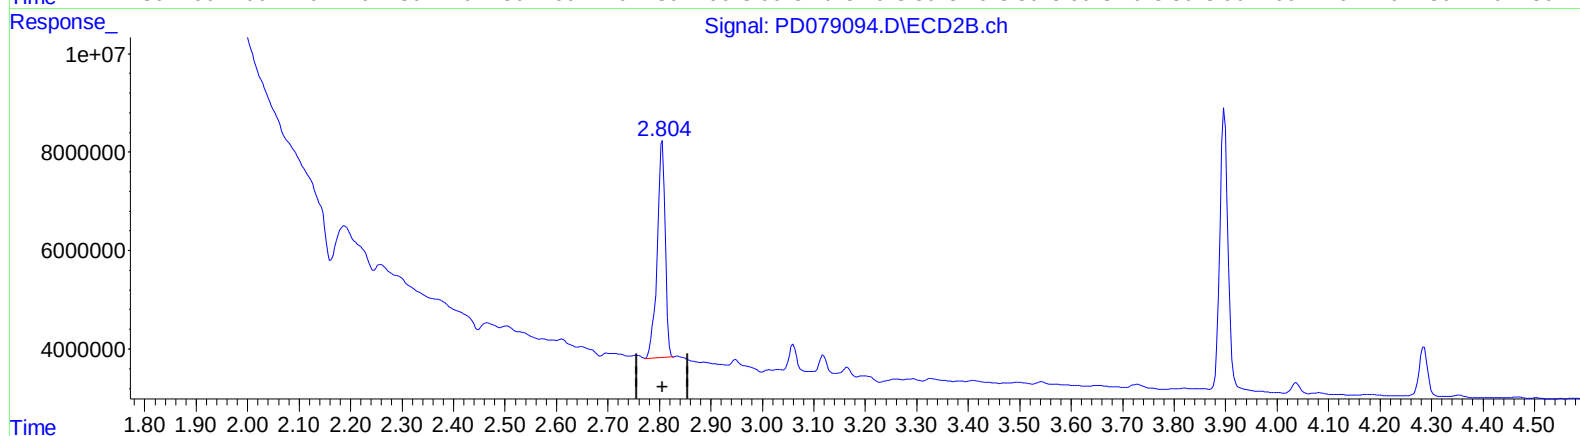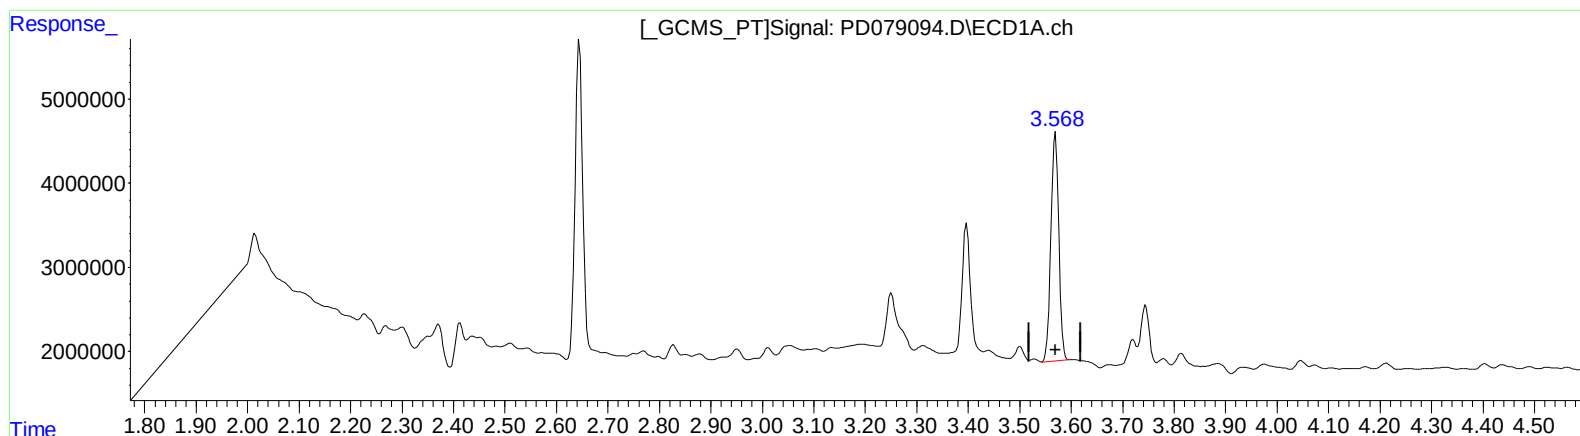

QEdit

(1) Tetrachloro-m-xylene (SA)

3.568min 18.917 ng/ml m

response 29012192

(1) Tetrachloro-m-xylene #2 (SA)

2.804min 21.899 ng/ml m

response 47488628

(+) = Expected Retention Time