

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
 Data File : PD079108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 16:49
 Operator : AR\AJ
 Sample : INDA312
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3162

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:22:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.574	2.802	28438501	39486541	18.543	18.209
27)	SA Decachlor...	9.119	7.953	65206981	84503742	34.380	36.232
Target Compounds							
2)	A alpha-BHC	4.031	3.306	48847799	62432336	18.748	18.309
3)	MA gamma-BHC...	4.365	3.636	46723783	59351465	18.773	18.363
4)	MA Heptachlor	4.958	3.980	48873570	56883577	18.345	18.706
9)	A Endosulfan I	6.113	5.133	38112185	47800821	17.791	18.823
13)	MA Dieldrin	6.389	5.398	80436314	107.0E6	35.407	36.343
14)	MA Endrin	6.619	5.673	64928937	91642760	34.295	36.317
16)	A 4,4'-DDD	6.750	5.821	59809743	82084290	35.583	37.163
17)	MA 4,4'-DDT	7.064	6.073	61683449	81866977	34.450	36.337
20)	A Methoxychlor	7.538	6.648	164.8E6	221.1E6	171.785	181.355

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 16:49
Operator : AR\AJ
Sample : INDA312
Misc :
ALS Vial : 99 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:22:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

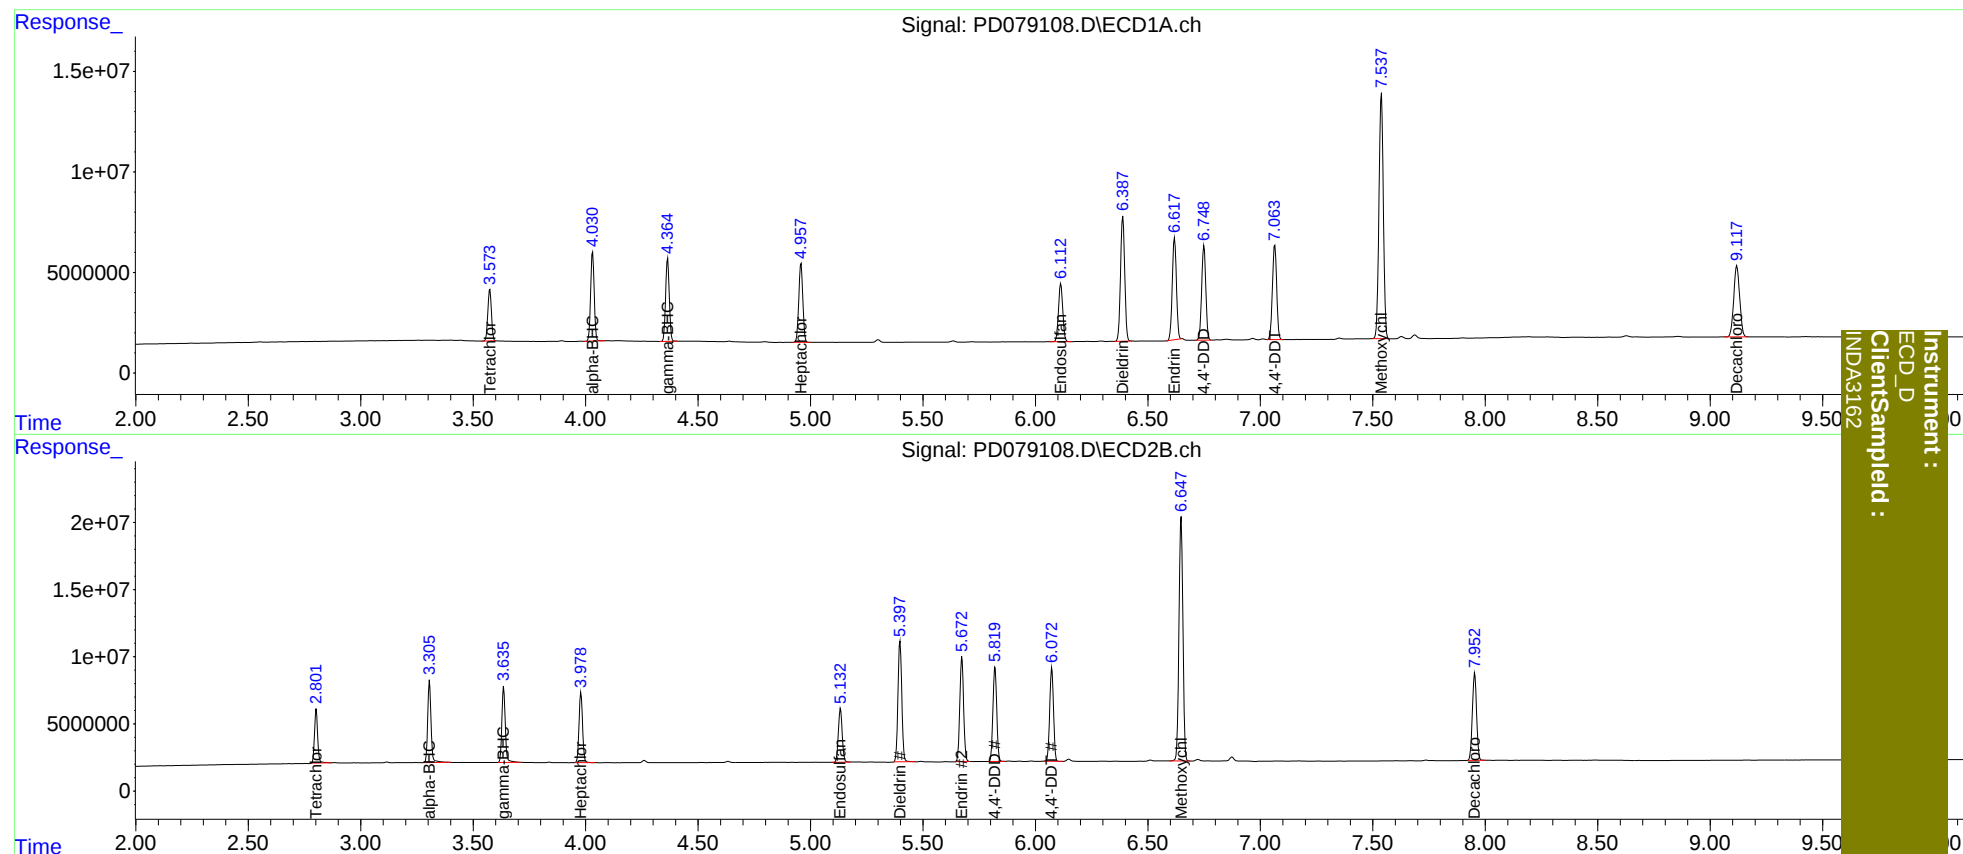

Instrument :
ECD_D
ClientSampled :
INDA3162