

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
 Data File : PD079122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 20:10
 Operator : AR\AJ
 Sample : 04922-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAQ9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2023
 Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:24:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.578	2.821	13332486	15146651	8.693m	6.985m
2)	SA Decachlor...	9.120	7.965	20203115	84890547	10.652m	36.398m#
Target Compounds							
5)	MB Aldrin	5.300	4.286	158.6E6	87394778	64.142m	28.367m#
8)	B Heptachlo...	5.727	4.772	57449377	330.0E6	23.922m	114.336m#
13)	MA Dieldrin	6.366	5.411	298.7E6	186.0E6	131.468m	63.150m#
15)	B Endosulfa...	6.817	5.980	643.6E6	311.8E6	324.590	131.026m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 20:10
Operator : AR\AJ
Sample : 04922-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:24:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

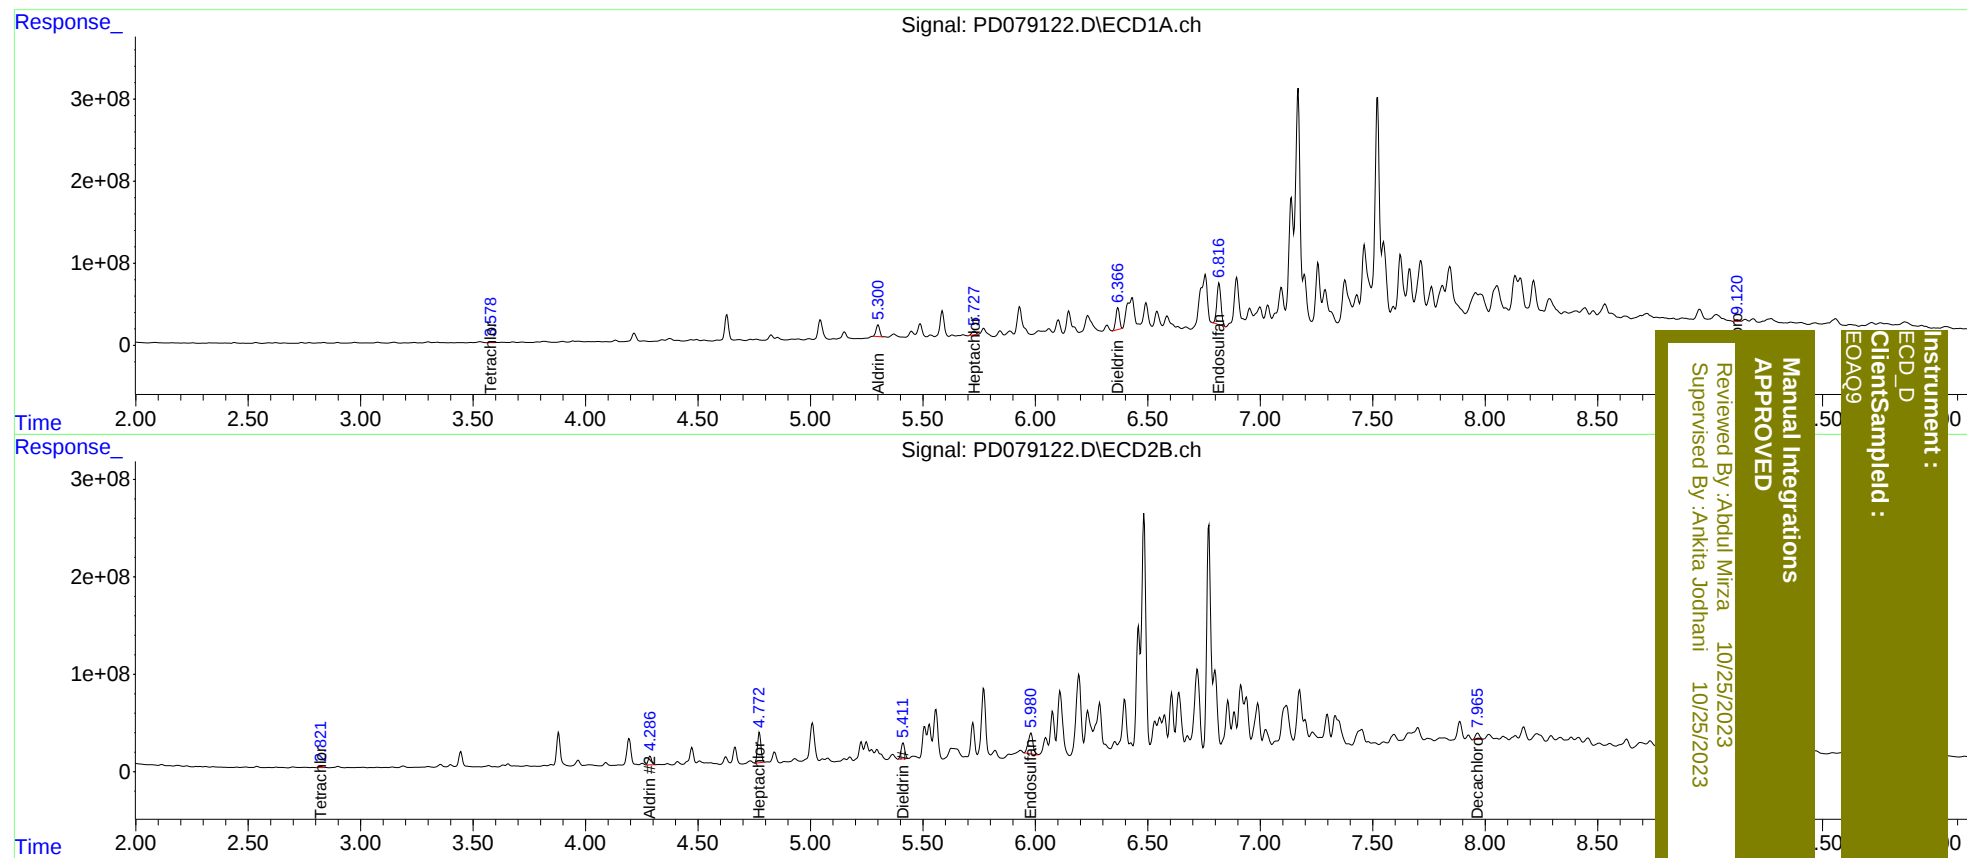

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 10/25/2023
Supervised By: Ankita Jodhani 10/25/2023

Instrument :
ECD_D
Client Sampled :
EOAQ9