

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
 Data File : PD079129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 21:44
 Operator : AR\AJ
 Sample : 04922-12
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EOAT1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2023
 Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:25:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.807	13399010	19242973	8.736	8.874
27) SA Decachlor...	9.107	7.951	8724223	13212124	4.600m	5.665
Target Compounds						
12) B 4,4'-DDE	6.226	5.269	82158822	128.9E6	39.884	49.289
14) MA Endrin	6.644	5.686	13193979	17416151	6.969m	6.902
16) A 4,4'-DDD	6.742	5.822	32422679	48001304	19.289	21.732
17) MA 4,4'-DDT	7.058	6.074	255.3E6	366.1E6	142.602	162.489

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102423\
Data File : PD079129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 21:44
Operator : AR\AJ
Sample : 04922-12
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:25:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

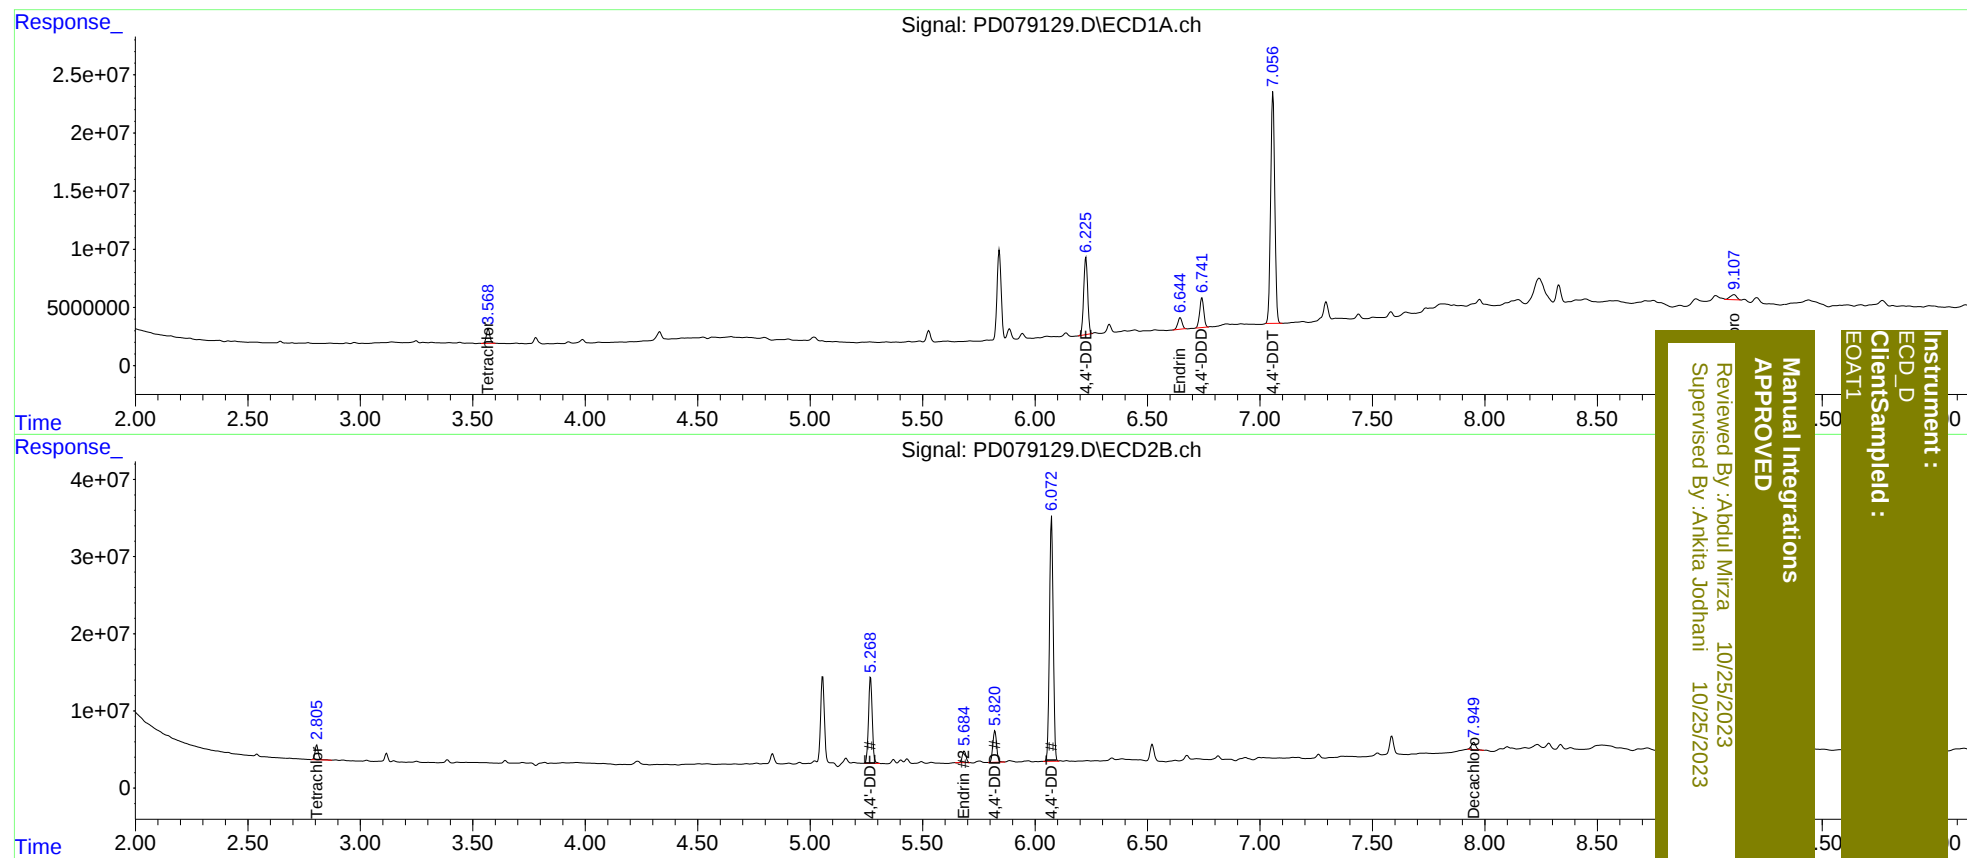

Instrument :
ECD_D
ClientSampled :
EOAT1

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 10/25/2023
Supervised By: Ankita Jodhani 10/25/2023