

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102522\
 Data File : PD072612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 10:28
 Operator : AR\AJ
 Sample : N5234-06 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LSP-SS-06-00-20

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/07/2022
 Supervised By : Ankita Jodhani 11/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 21:45:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 04:17:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.706	3.464	5849751	70841917	2.348	2.130m
28) SA Decachlor...	7.839	8.920	4087242	20721706	1.816	2.303 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102522\
Data File : PD072612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 10:28
Operator : AR\AJ
Sample : N5234-06 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
LSP-SS-06-00-20


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/07/2022
Supervised By : Ankita Jodhani 11/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 21:45:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102022.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 04:17:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

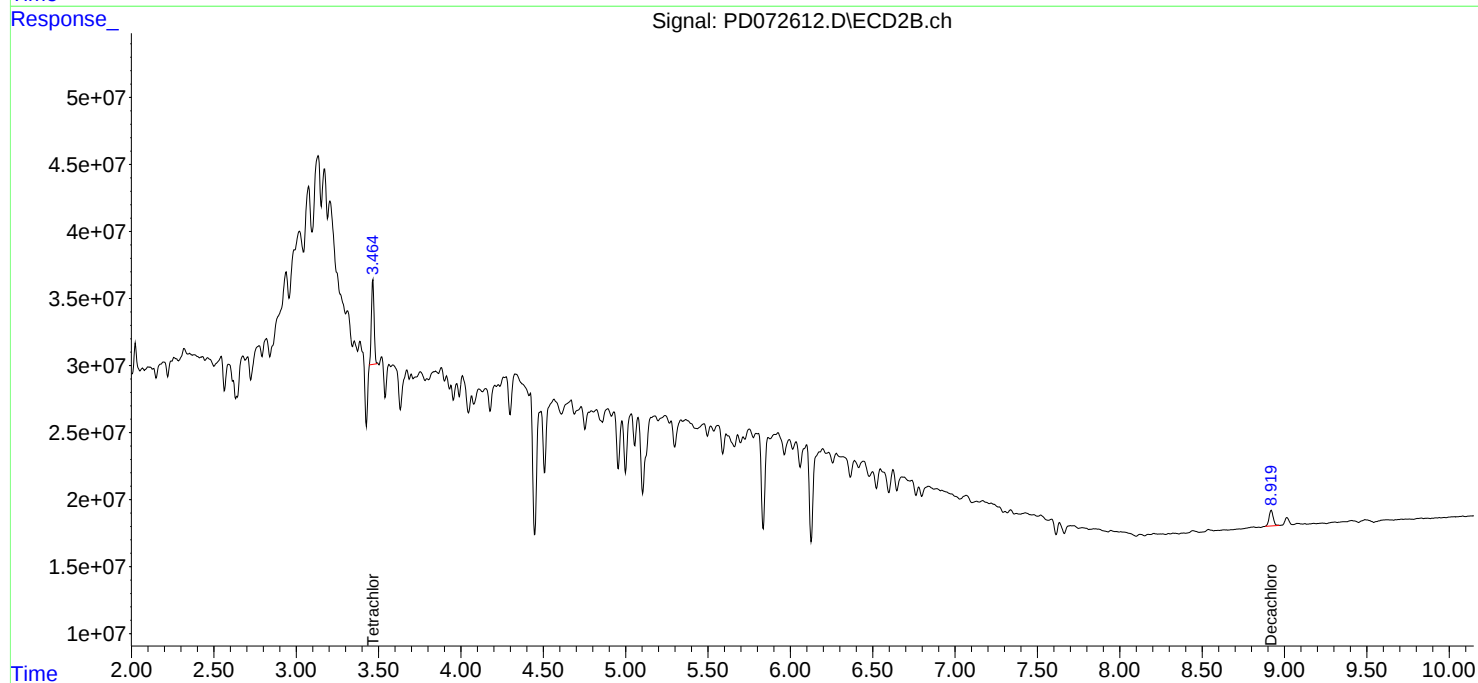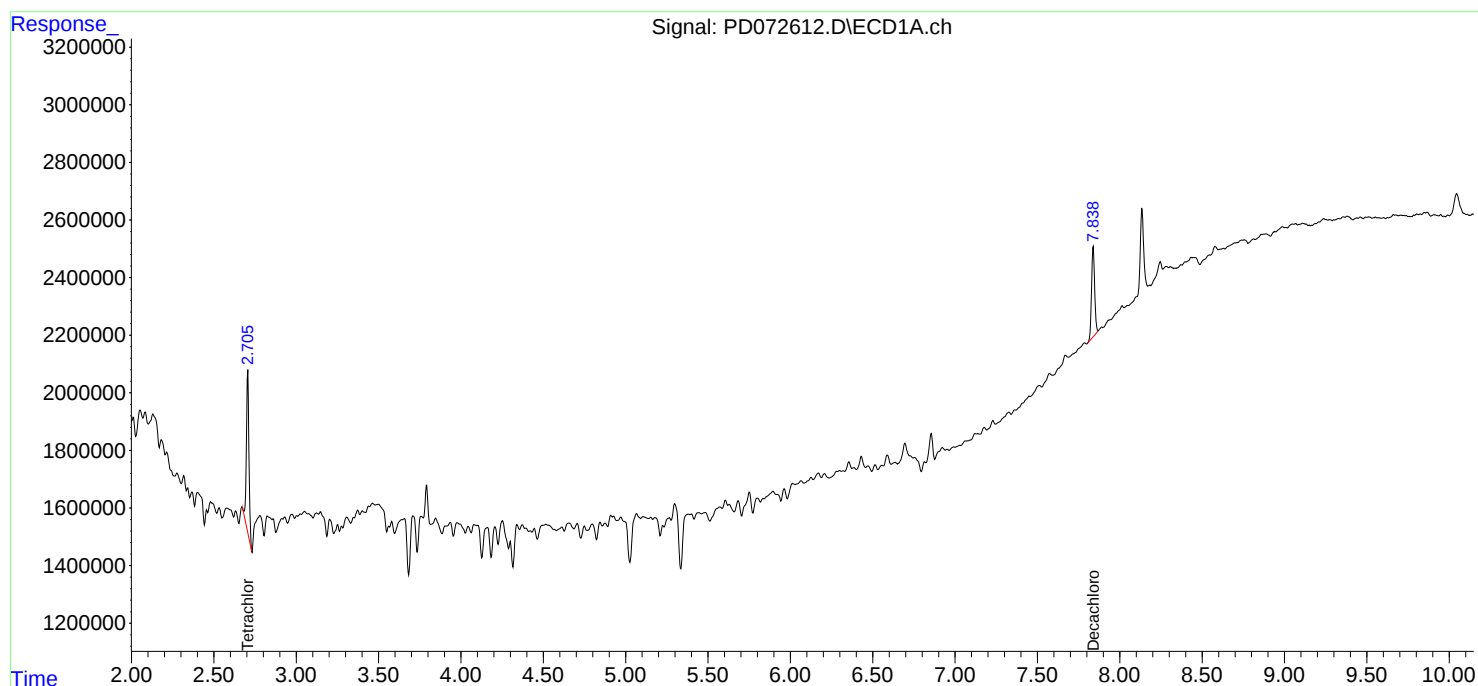

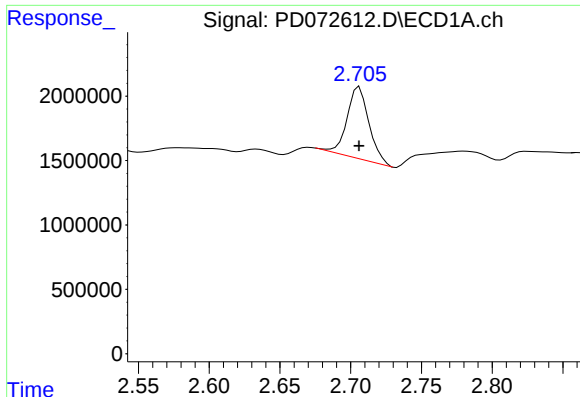


#1 Tetrachloro-m-xylene

R.T.: 2.706 min
Delta R.T.: 0.000 min
Response: 5849751
Conc: 2.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
LSP-SS-06-00-20


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/07/2022
Supervised By :Ankita Jodhani 11/09/2022

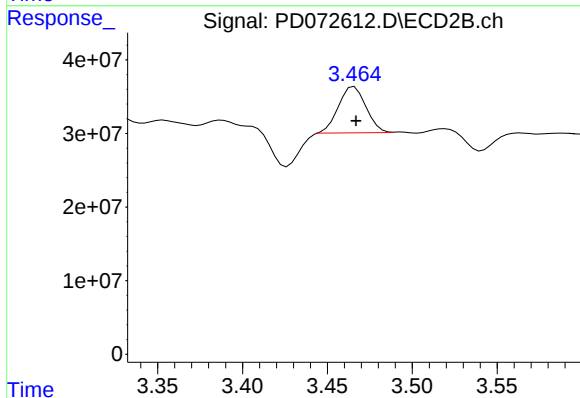


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.003 min
Response: 70841917
Conc: 2.13 ng/ml m

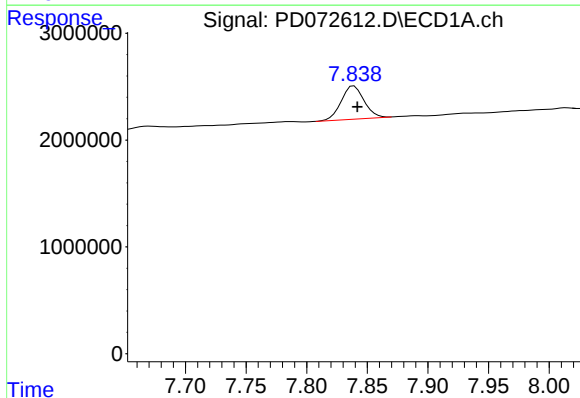

#28 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: -0.003 min
Response: 4087242
Conc: 1.82 ng/ml

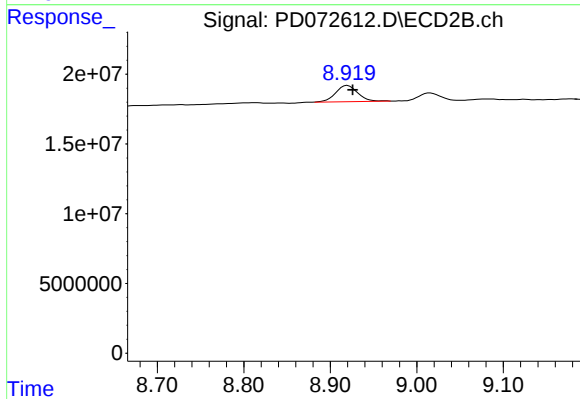

#28 Decachlorobiphenyl

R.T.: 8.920 min
Delta R.T.: -0.006 min
Response: 20721706
Conc: 2.30 ng/ml