

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102523\
 Data File : PD079163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 19:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 01:40:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.805	73196247	131.8E6	45.334	56.905 #
28)	SA Decachlor...	9.111	7.952	88665806	117.7E6	44.200	48.306
Target Compounds							
23)	Chlordane-1	4.736	3.808	38987254	44116111	501.454	507.928
24)	Chlordane-2	5.266	4.384	38834389	45282385	486.476	498.381
25)	Chlordane-3	5.976	5.015	156.4E6	139.3E6	504.565	522.164
26)	Chlordane-4	6.059	5.079	187.6E6	130.9E6	504.918	533.475
27)	Chlordane-5	6.910	5.974	34108076	52482770	485.418	526.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102523\
Data File : PD079163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 19:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 01:40:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

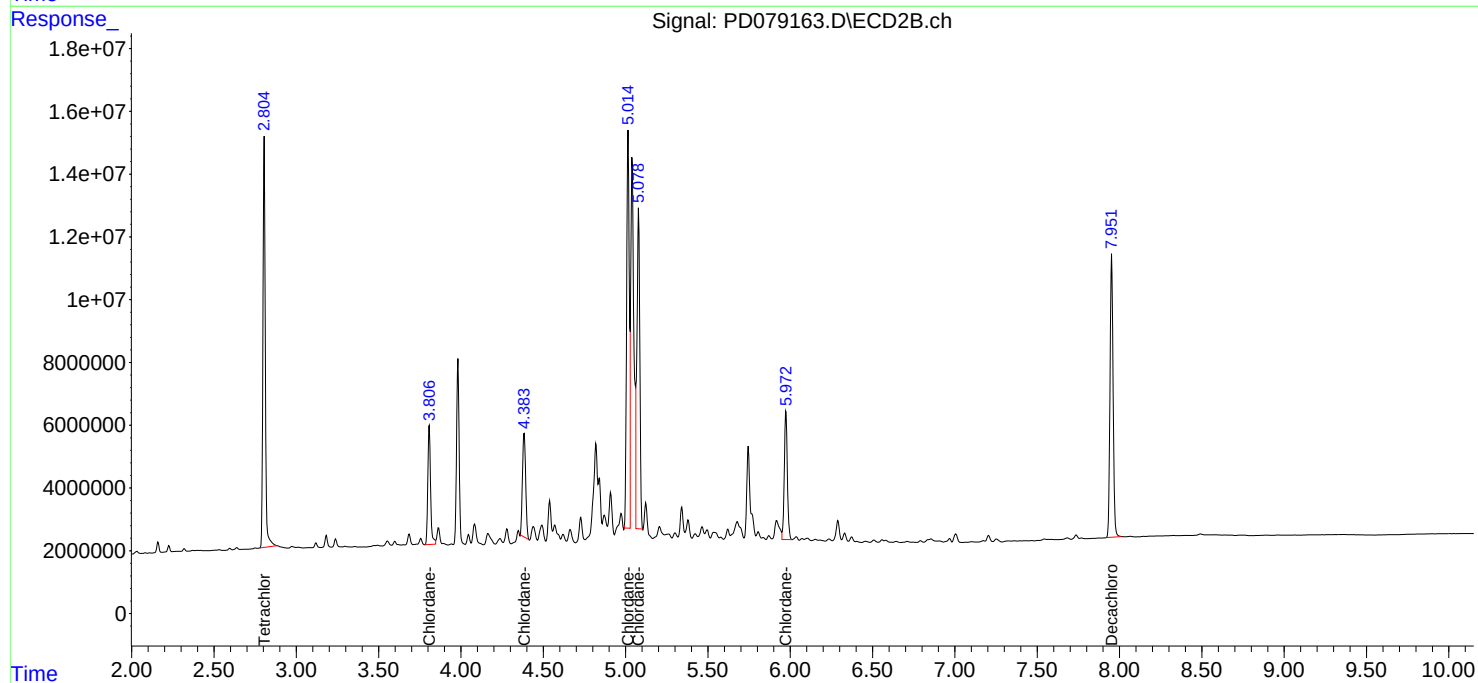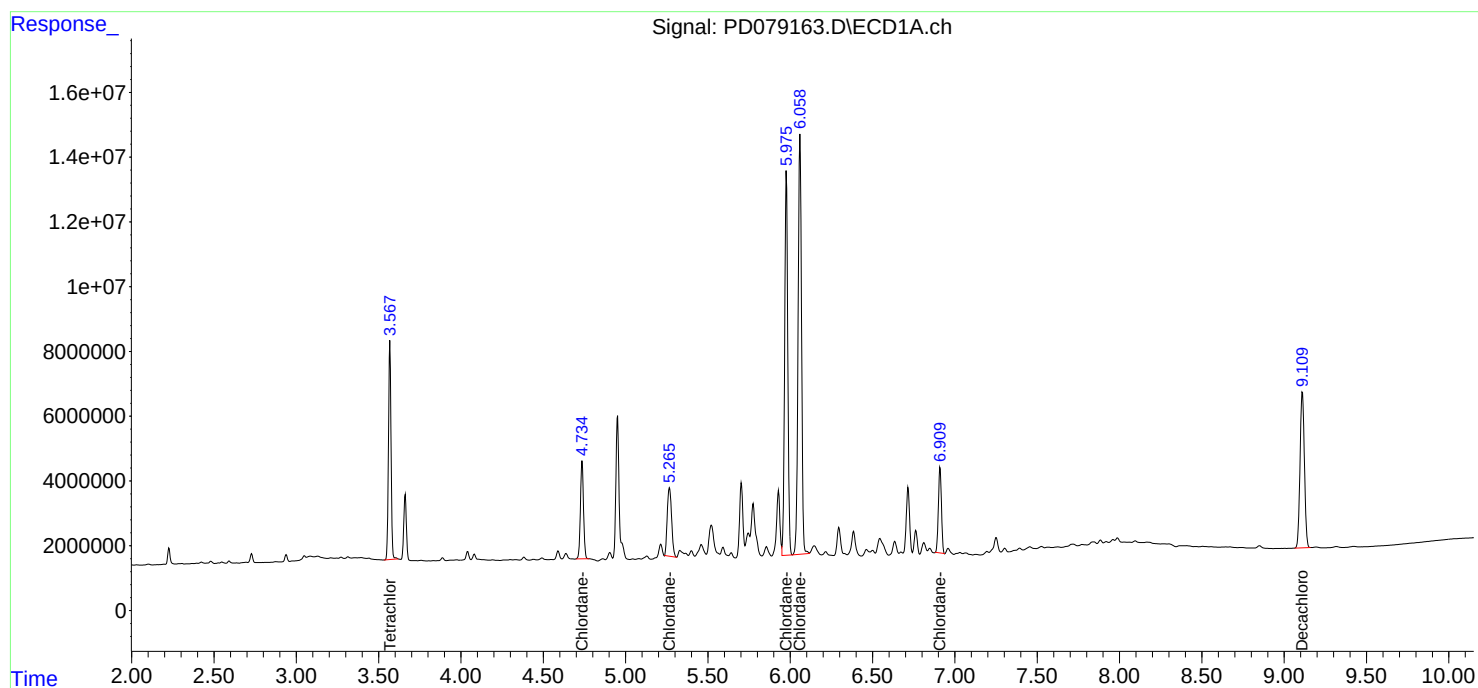


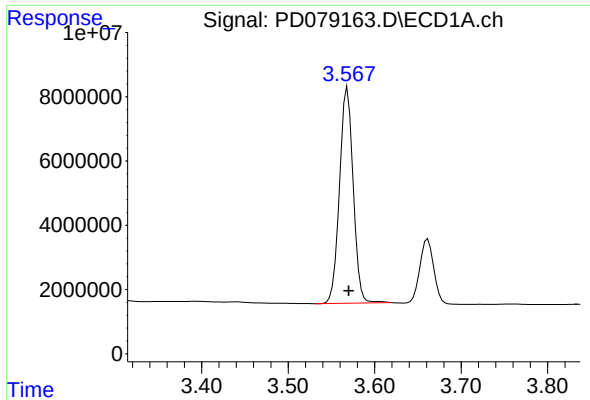

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: -0.001 min
Response: 73196247
Conc: 45.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

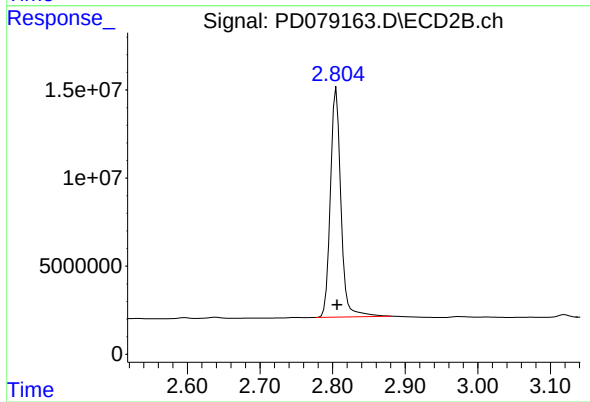


#1 Tetrachloro-m-xylene

R.T.: 2.805 min
Delta R.T.: -0.001 min
Response: 131751478
Conc: 56.91 ng/ml

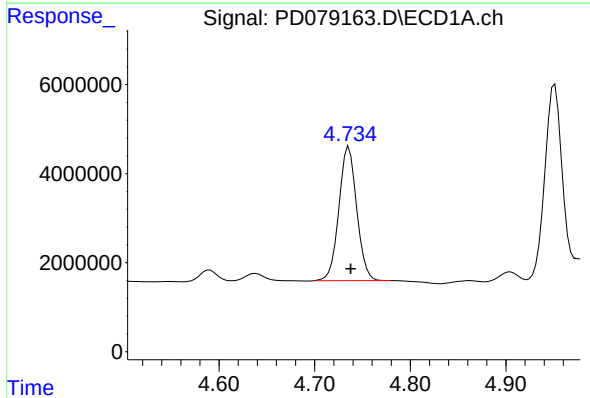


#23 Chlordane-1

R.T.: 4.736 min
Delta R.T.: -0.002 min
Response: 38987254
Conc: 501.45 ng/ml

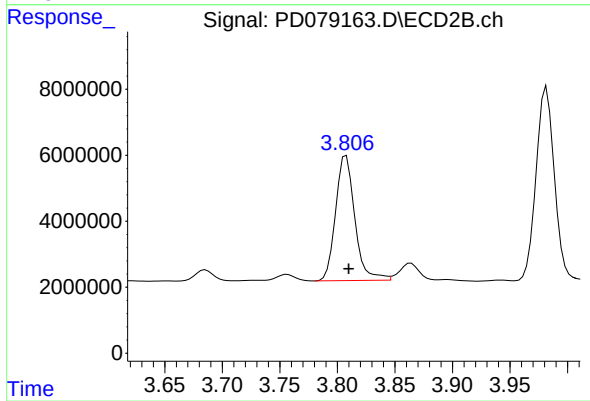

#23 Chlordane-1


R.T.: 3.808 min
Delta R.T.: -0.002 min
Response: 44116111
Conc: 507.93 ng/ml

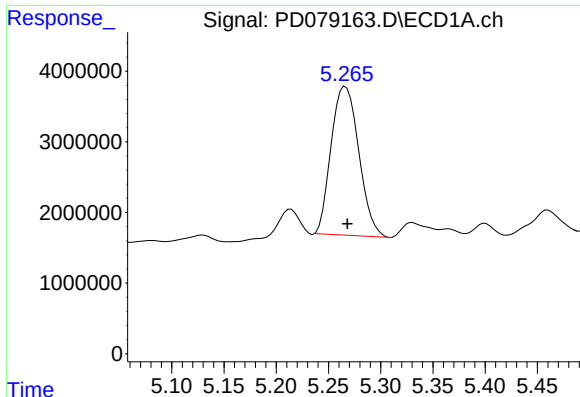

#24 Chlordane-2


R.T.: 5.266 min
Delta R.T.: -0.002 min
Response: 38834389
Conc: 486.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

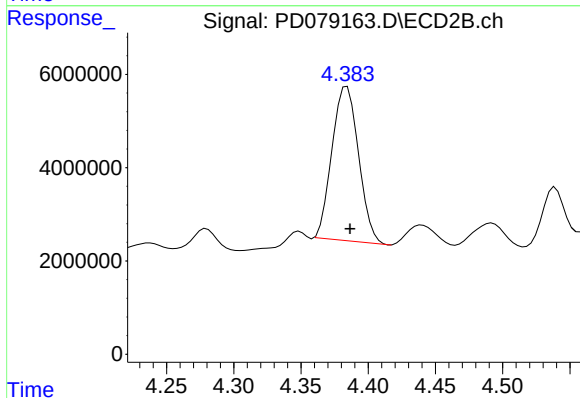


#24 Chlordane-2

R.T.: 4.384 min
Delta R.T.: -0.002 min
Response: 45282385
Conc: 498.38 ng/ml

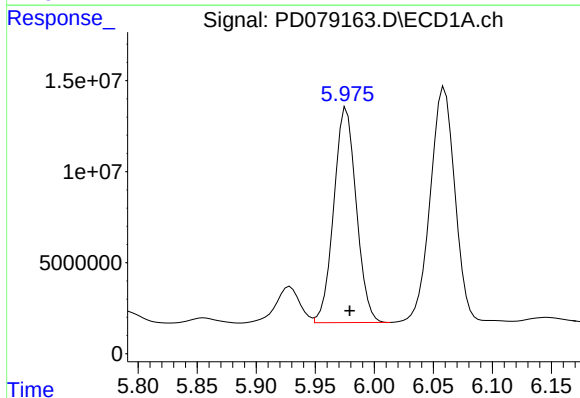


#25 Chlordane-3

R.T.: 5.976 min
Delta R.T.: -0.003 min
Response: 156417461
Conc: 504.56 ng/ml

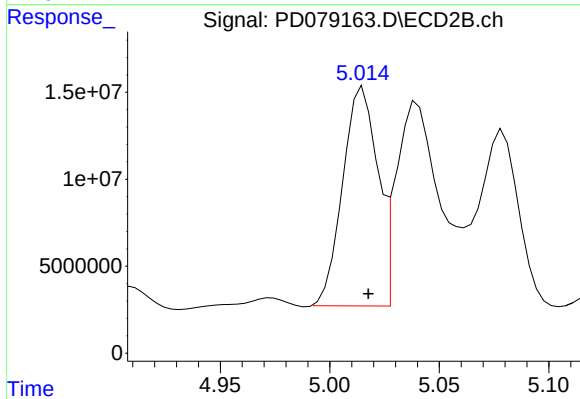

#25 Chlordane-3


R.T.: 5.015 min
Delta R.T.: -0.003 min
Response: 139277882
Conc: 522.16 ng/ml

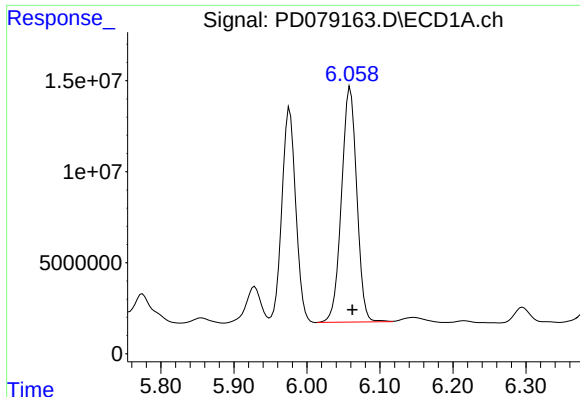

#26 Chlordane-4


R.T.: 6.059 min
Delta R.T.: -0.003 min
Response: 187589207
Conc: 504.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

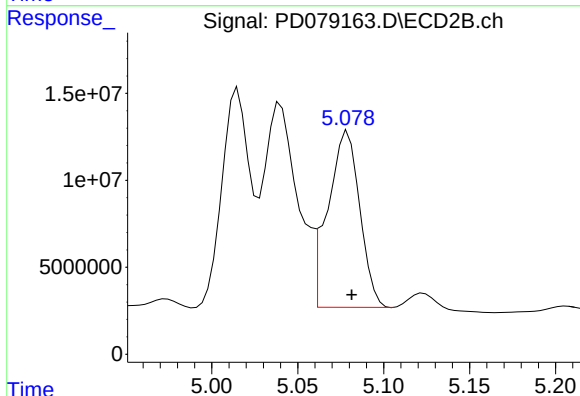


#26 Chlordane-4

R.T.: 5.079 min
Delta R.T.: -0.002 min
Response: 130903524
Conc: 533.47 ng/ml

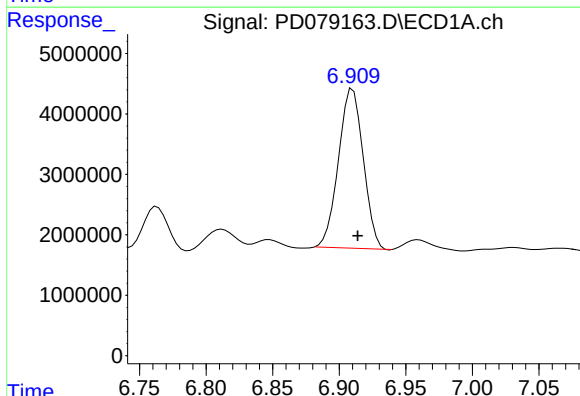


#27 Chlordane-5

R.T.: 6.910 min
Delta R.T.: -0.004 min
Response: 34108076
Conc: 485.42 ng/ml

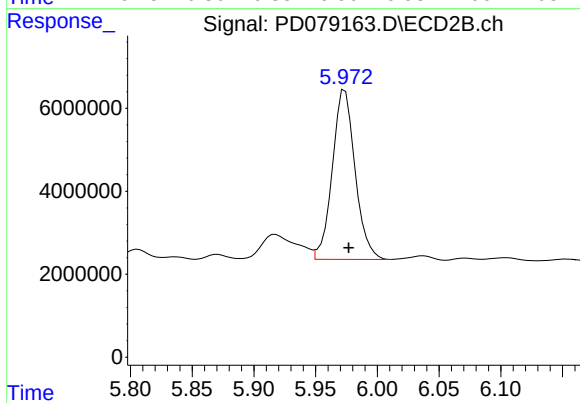

#27 Chlordane-5


R.T.: 5.974 min
Delta R.T.: -0.003 min
Response: 52482770
Conc: 526.60 ng/ml

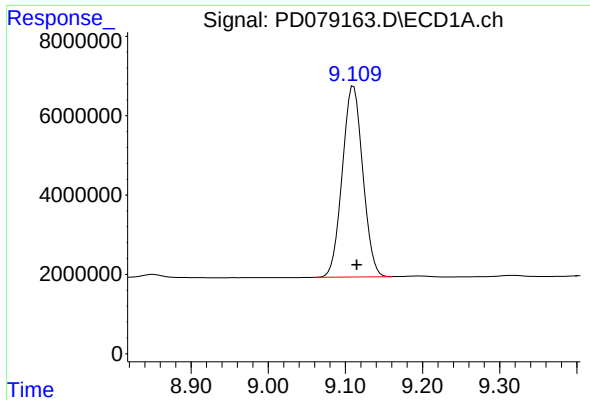

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.004 min
Response: 88665806
Conc: 44.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

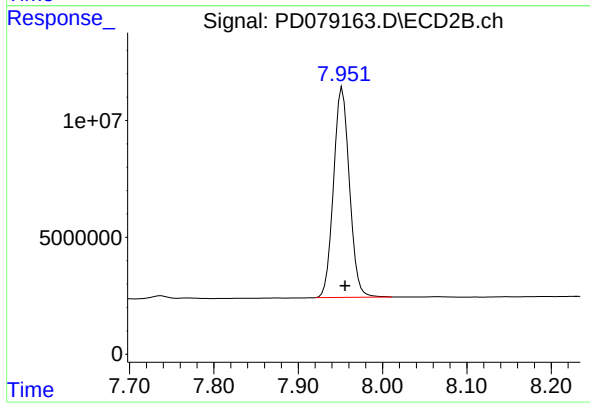

#28 Decachlorobiphenyl

R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 117744551
Conc: 48.31 ng/ml