

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 12:22
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:11:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.465	12395989	221.9E6	5.463	5.640
27)	SA Decachlor...	7.838	8.922	22288258	104.6E6	11.616	11.281
Target Compounds							
2)	A alpha-BHC	3.208	3.930	16947790	297.1E6	4.967	5.739
3)	MA gamma-BHC...	3.539	4.263	15669958	246.7E6	5.056	5.931
4)	MA Heptachlor	3.872	4.830	16784797	176.5E6	5.313	6.070
9)	A Endosulfan I	5.025	5.987	13591819	98890677	5.506	5.801
13)	MA Dieldrin	5.291	6.263	27931816	199.6E6	10.359	11.372
14)	MA Endrin	5.569	6.495	24684003	164.3E6	10.347	11.402
16)	A 4,4'-DDD	5.715	6.629	21486732	147.4E6	10.274	11.071
17)	MA 4,4'-DDT	5.965	6.938	21694029	147.9E6	10.205	11.084
20)	A Methoxychlor	6.549	7.416	62874553	339.7E6	54.856	56.816


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 12:22
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:11:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

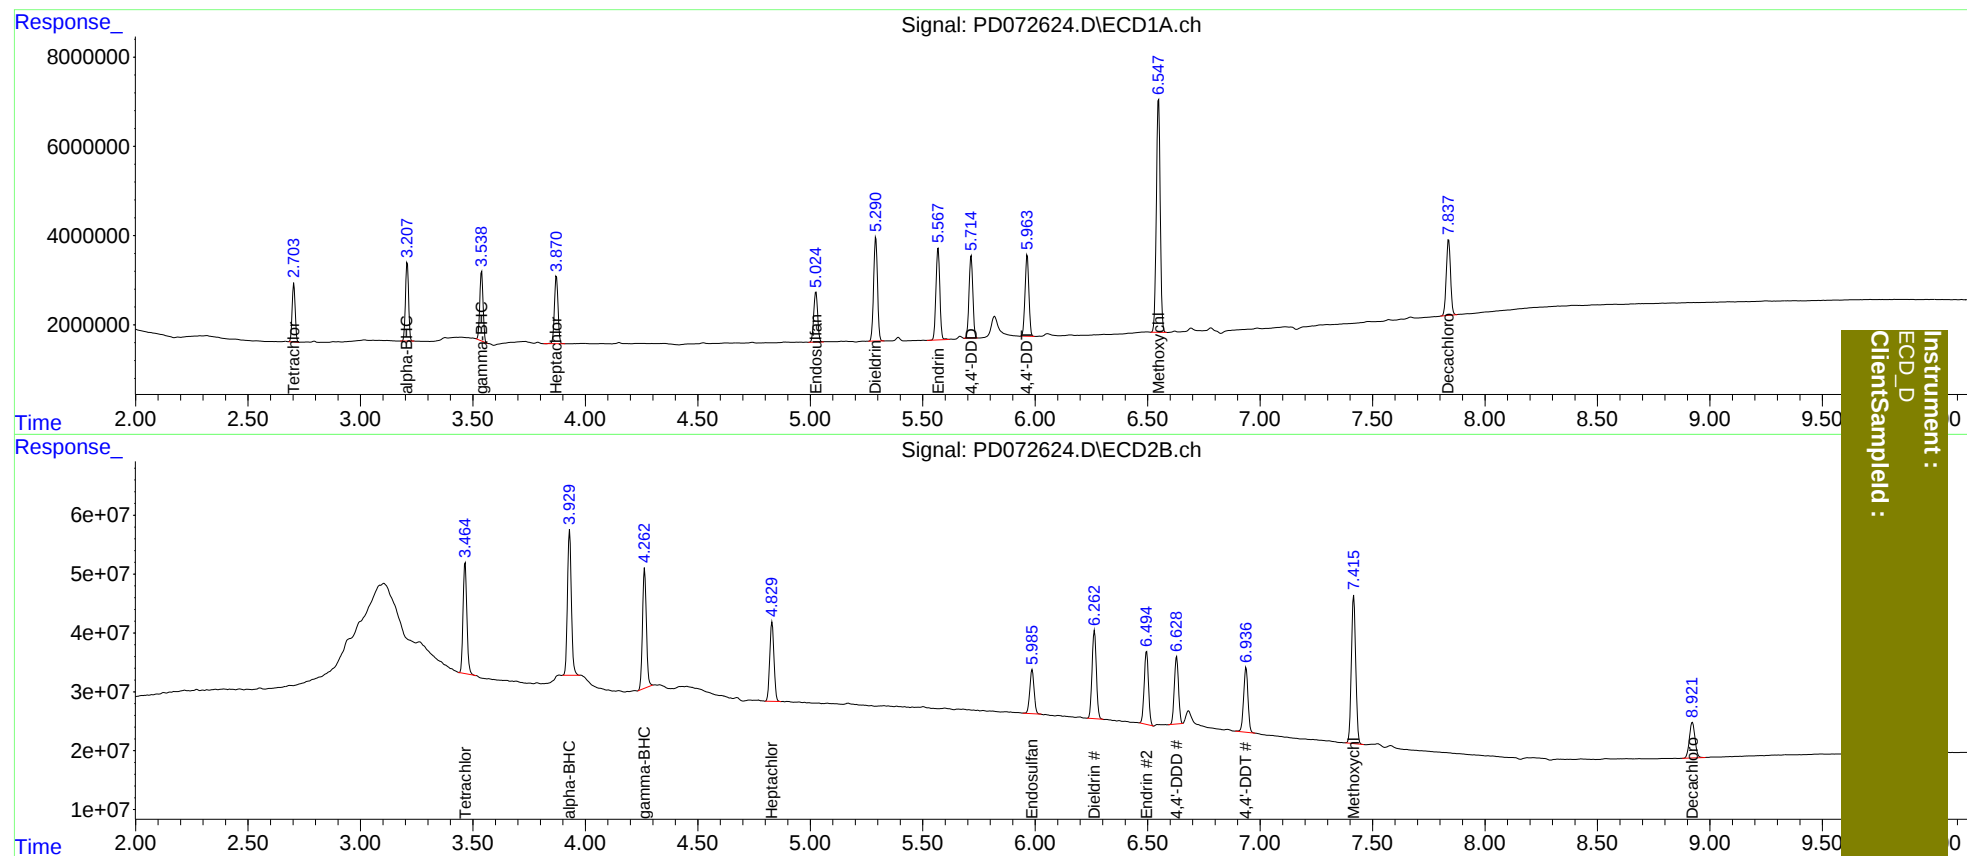


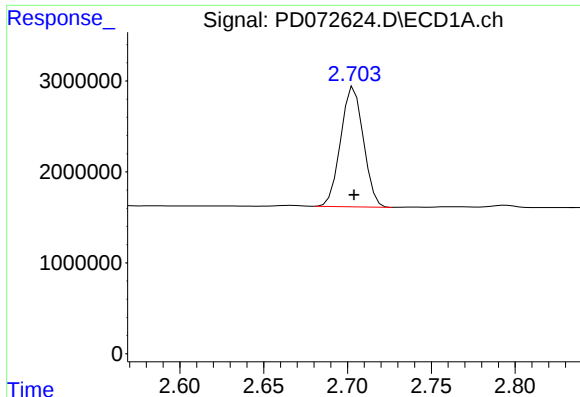

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 12395989
Conc: 5.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

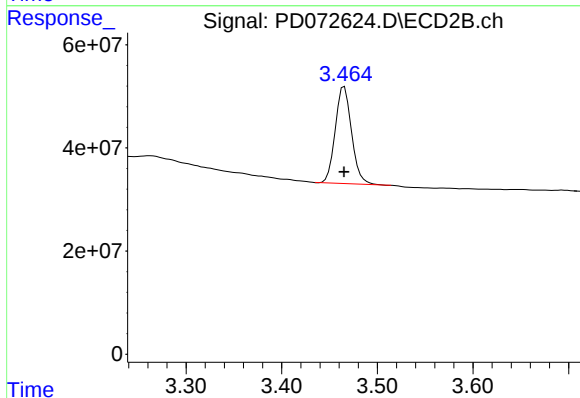


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 221932756
Conc: 5.64 ng/ml

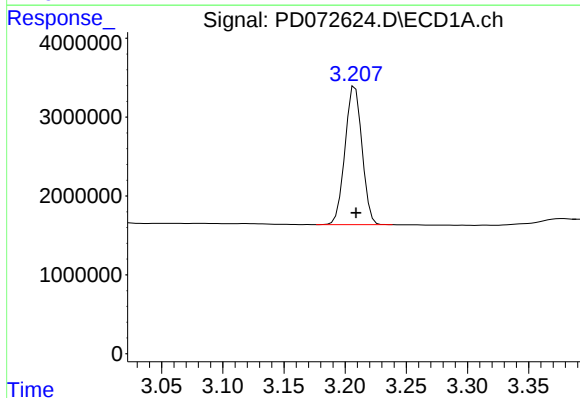


#2 alpha-BHC

R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 16947790
Conc: 4.97 ng/ml

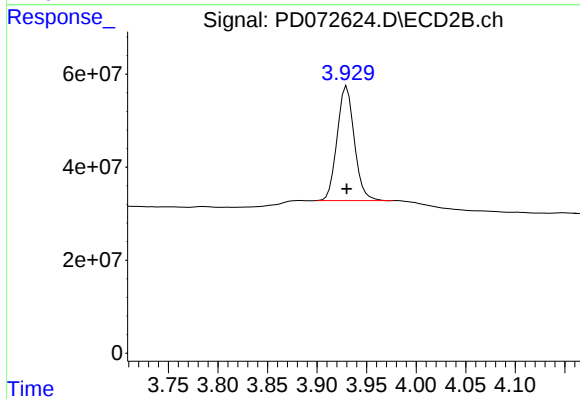

#2 alpha-BHC


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 297127807
Conc: 5.74 ng/ml

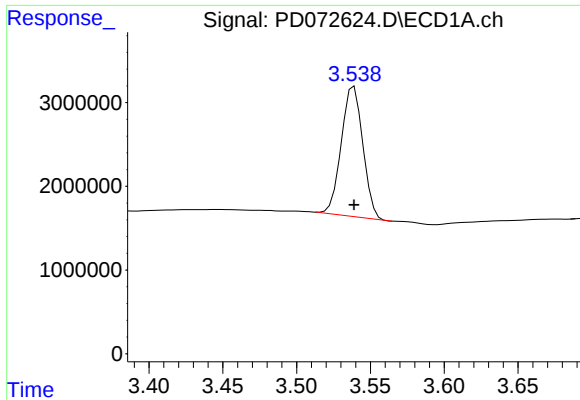

#3 gamma-BHC (Lindane)


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 15669958
Conc: 5.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

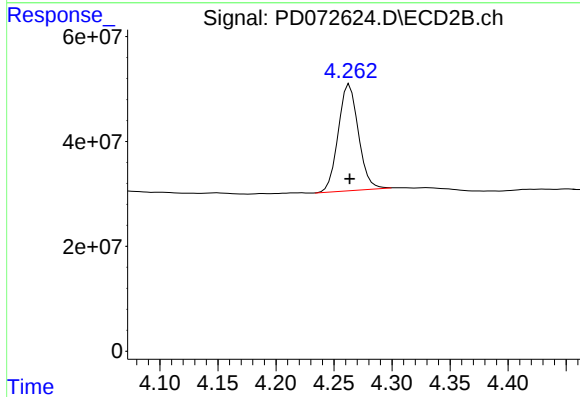


#3 gamma-BHC (Lindane)

R.T.: 4.263 min
Delta R.T.: 0.000 min
Response: 246733155
Conc: 5.93 ng/ml

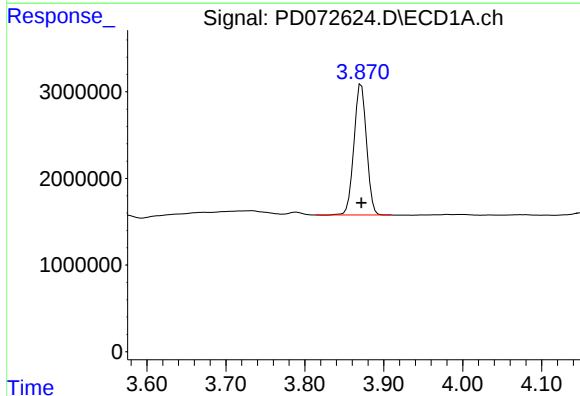


#4 Heptachlor

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 16784797
Conc: 5.31 ng/ml

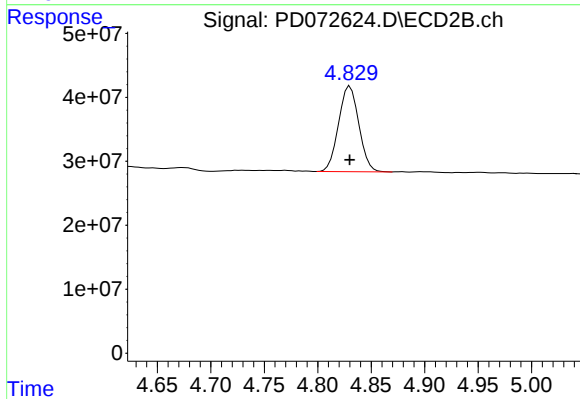

#4 Heptachlor


R.T.: 4.830 min
Delta R.T.: 0.000 min
Response: 176508339
Conc: 6.07 ng/ml

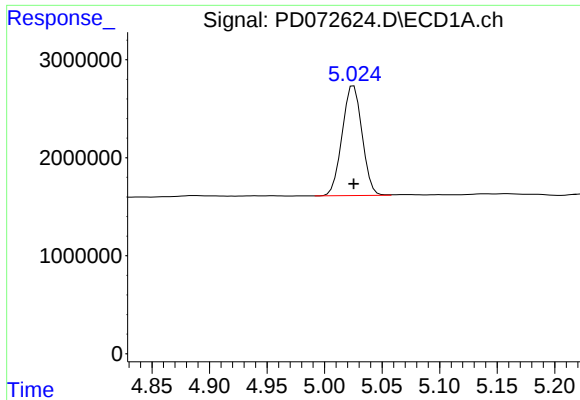

#9 Endosulfan I


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 13591819
Conc: 5.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

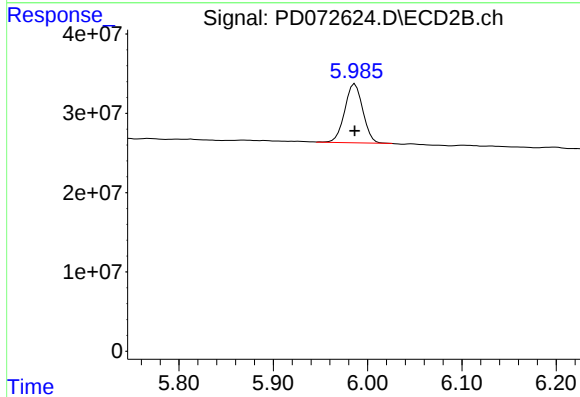


#9 Endosulfan I

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 98890677
Conc: 5.80 ng/ml

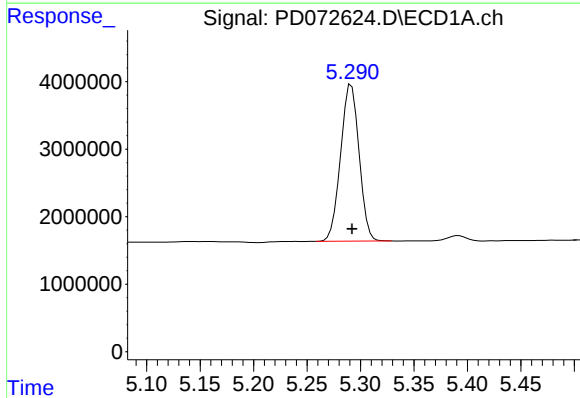


#13 Dieldrin

R.T.: 5.291 min
Delta R.T.: 0.000 min
Response: 27931816
Conc: 10.36 ng/ml

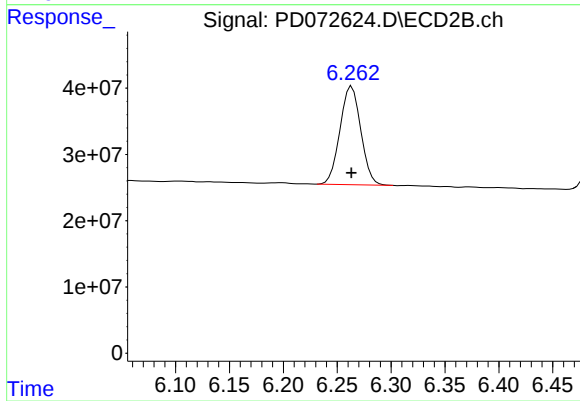

#13 Dieldrin


R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 199585381
Conc: 11.37 ng/ml

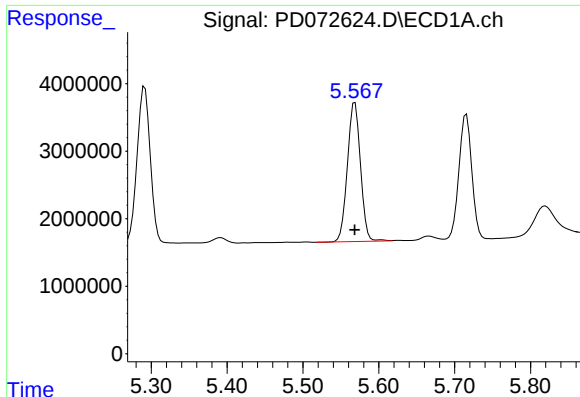

#14 Endrin


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 24684003
Conc: 10.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

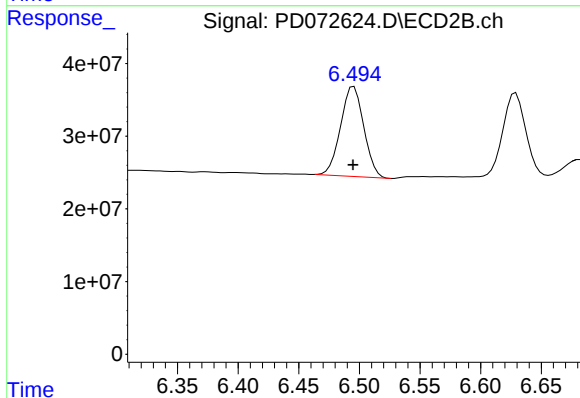


#14 Endrin

R.T.: 6.495 min
Delta R.T.: 0.000 min
Response: 164280761
Conc: 11.40 ng/ml

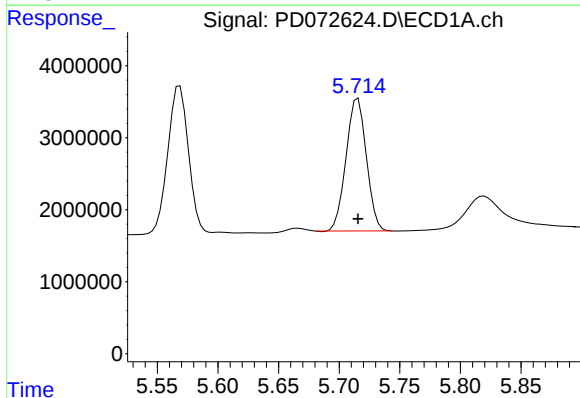


#16 4,4'-DDD

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 21486732
Conc: 10.27 ng/ml

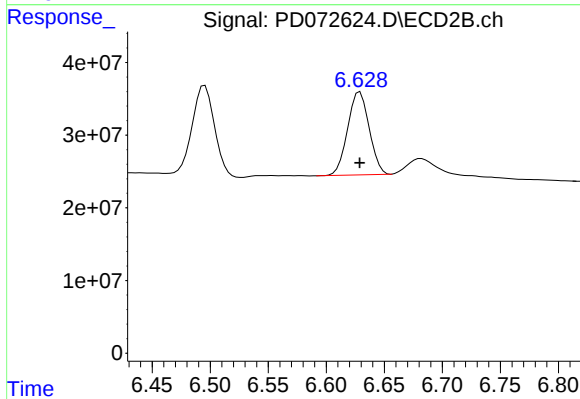

#16 4,4'-DDD


R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 147410153
Conc: 11.07 ng/ml

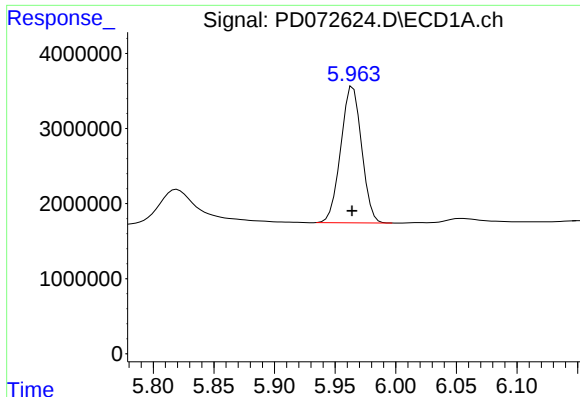

#17 4,4'-DDT


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 21694029
Conc: 10.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

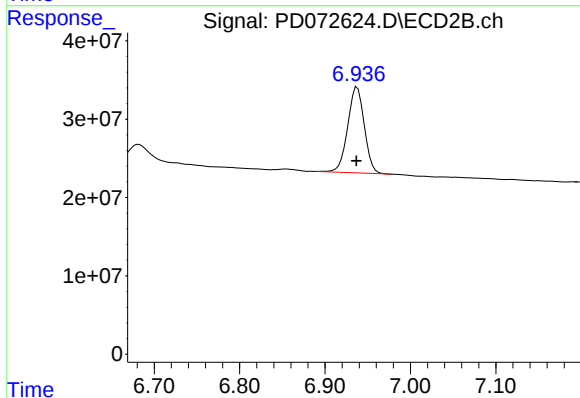


#17 4,4'-DDT

R.T.: 6.938 min
Delta R.T.: 0.001 min
Response: 147866673
Conc: 11.08 ng/ml

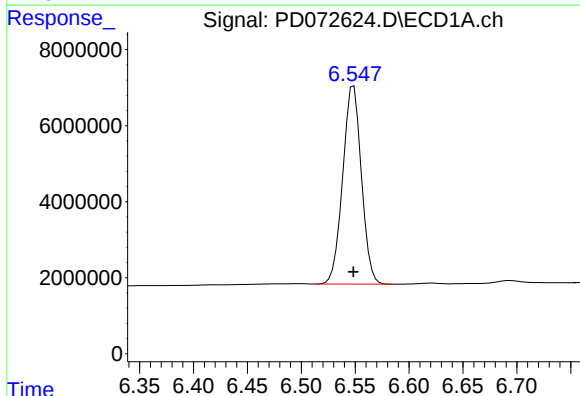


#20 Methoxychlor

R.T.: 6.549 min
Delta R.T.: 0.000 min
Response: 62874553
Conc: 54.86 ng/ml

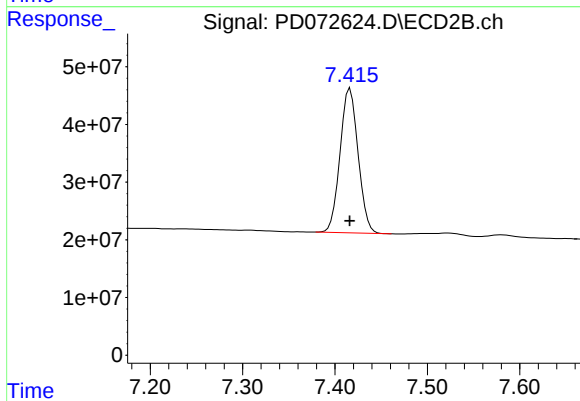

#20 Methoxychlor


R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 339676972
Conc: 56.82 ng/ml

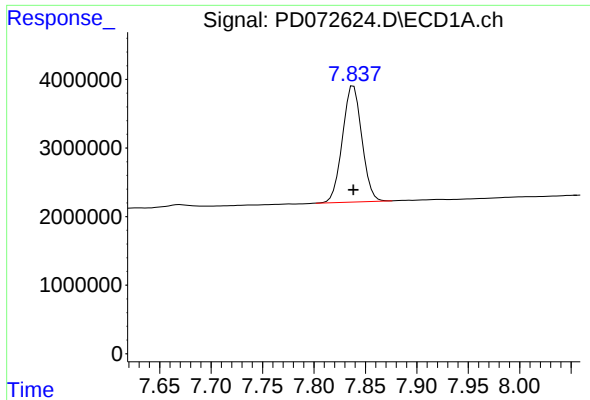

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 22288258
Conc: 11.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

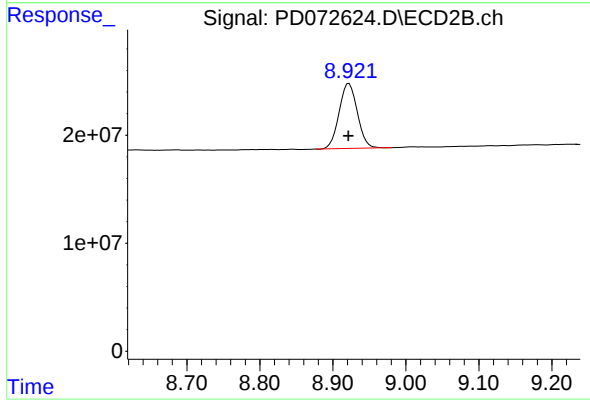

#27 Decachlorobiphenyl

R.T.: 8.922 min
Delta R.T.: 0.001 min
Response: 104550714
Conc: 11.28 ng/ml