

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 12:49
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:11:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.465	23927819	430.4E6	10.545	10.938
27)	SA Decachlor...	7.839	8.923	41266762	198.1E6	21.508	21.375
Target Compounds							
2)	A alpha-BHC	3.208	3.930	34059694	568.2E6	9.983	10.975
3)	MA gamma-BHC...	3.539	4.264	31236884	452.2E6	10.079	10.870
4)	MA Heptachlor	3.872	4.831	32486477	321.6E6	10.283	11.060
9)	A Endosulfan I	5.026	5.987	25877049	184.5E6	10.482	10.822
13)	MA Dieldrin	5.292	6.264	54508640	374.6E6	20.216	21.343
14)	MA Endrin	5.569	6.496	47946252	309.7E6	20.097	21.491
16)	A 4,4'-DDD	5.716	6.630	42366946	282.7E6	20.258	21.230
17)	MA 4,4'-DDT	5.965	6.937	42598463	279.9E6	20.039	20.979
20)	A Methoxychlor	6.549	7.418	118.9E6	639.2E6	103.747	106.914


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 12:49
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:11:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

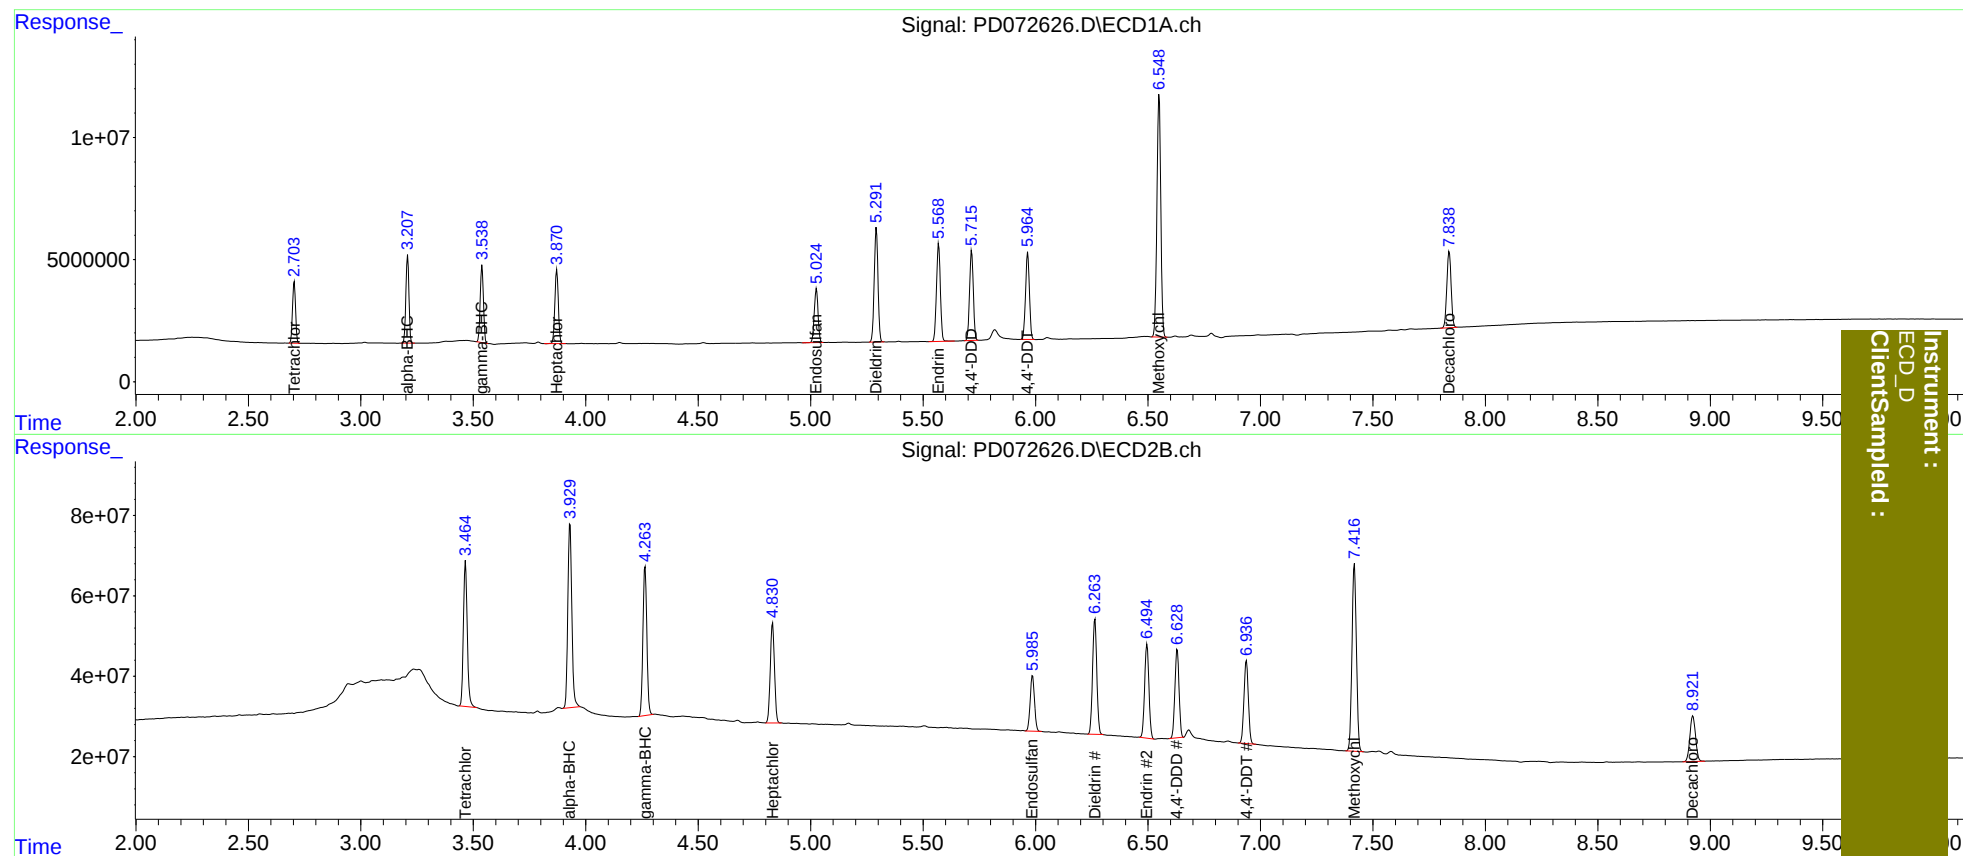


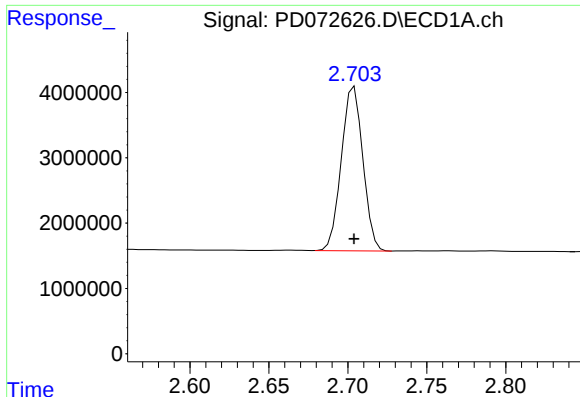

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 23927819
Conc: 10.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

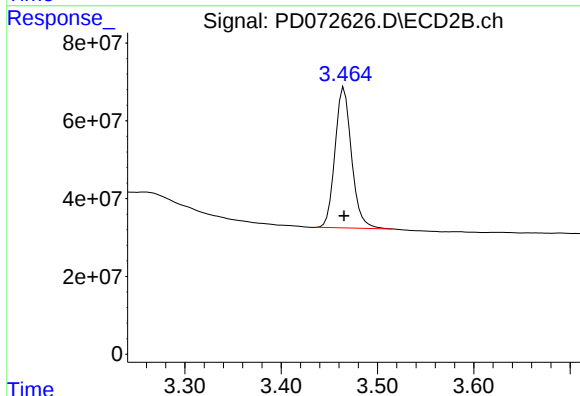


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 430375275
Conc: 10.94 ng/ml

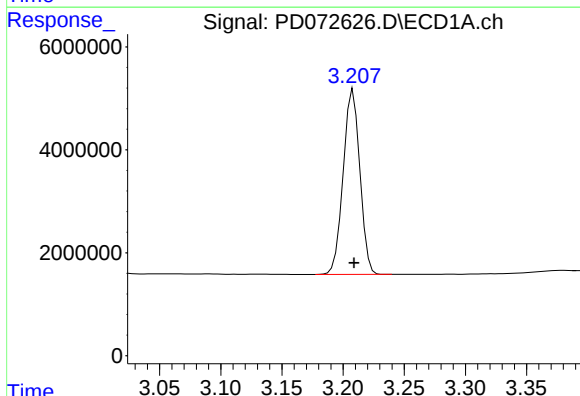


#2 alpha-BHC

R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 34059694
Conc: 9.98 ng/ml

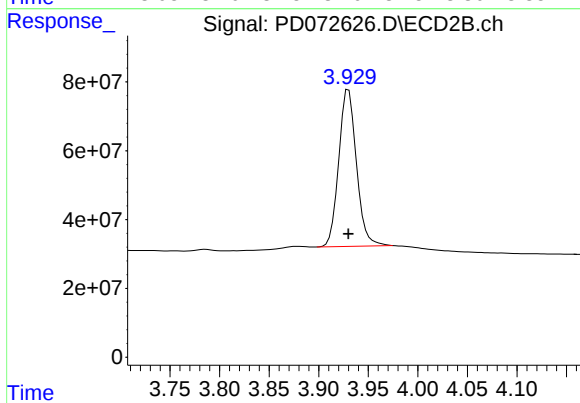

#2 alpha-BHC


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 568178873
Conc: 10.97 ng/ml

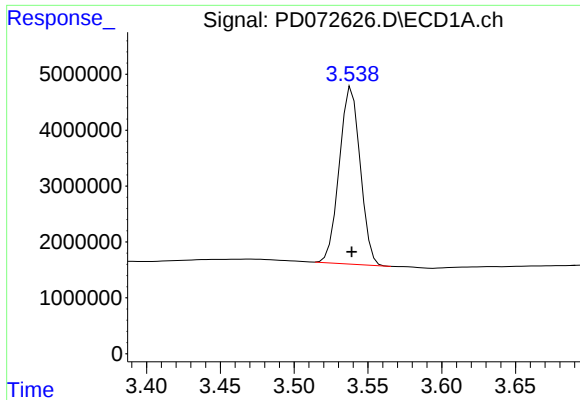

#3 gamma-BHC (Lindane)


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 31236884
Conc: 10.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

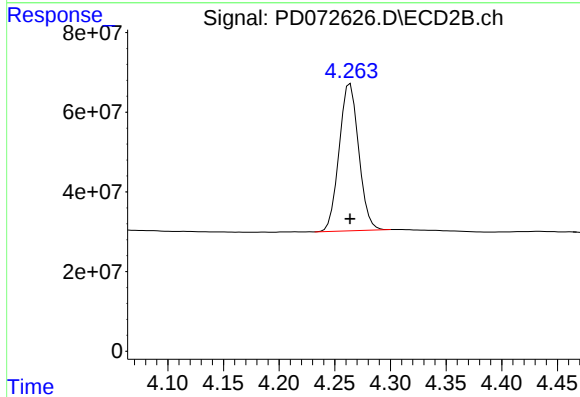


#3 gamma-BHC (Lindane)

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 452208681
Conc: 10.87 ng/ml

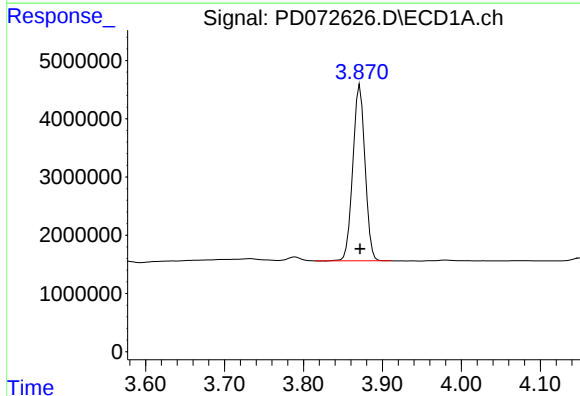


#4 Heptachlor

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 32486477
Conc: 10.28 ng/ml

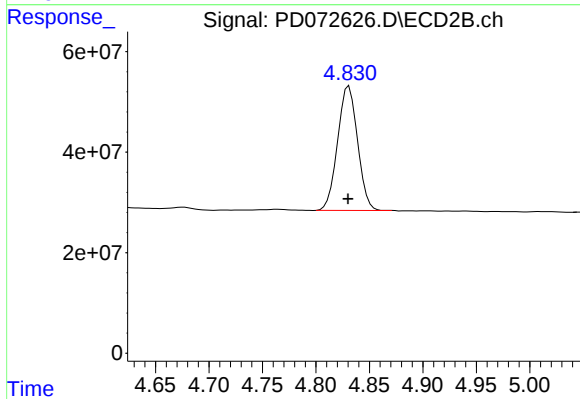

#4 Heptachlor


R.T.: 4.831 min
Delta R.T.: 0.000 min
Response: 321601938
Conc: 11.06 ng/ml

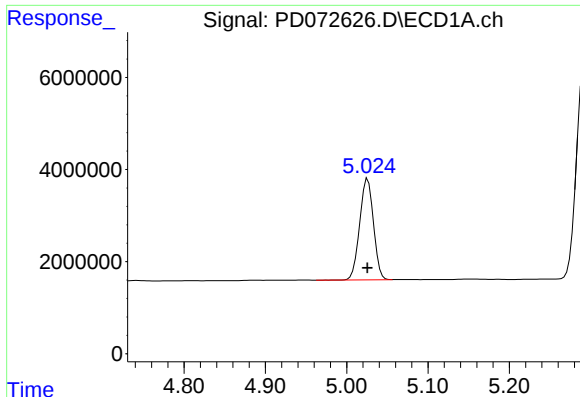

#9 Endosulfan I


R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 25877049
Conc: 10.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

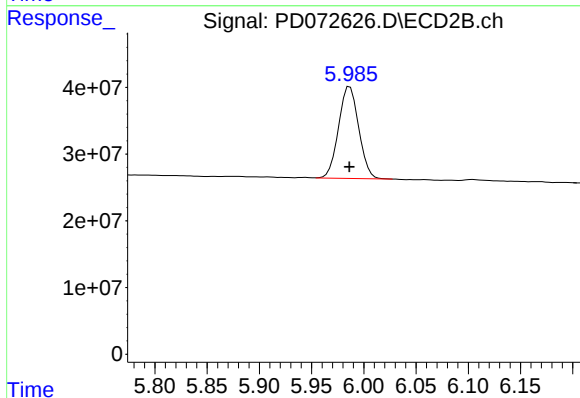


#9 Endosulfan I

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 184495567
Conc: 10.82 ng/ml

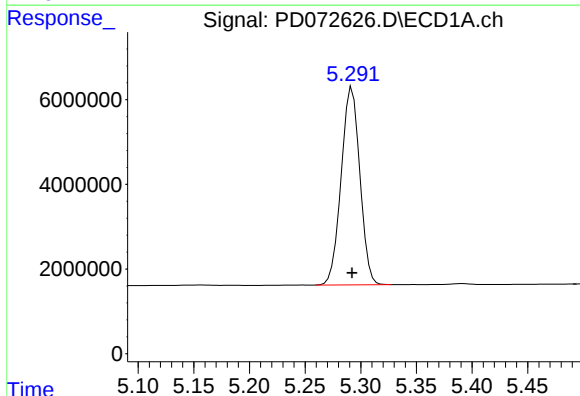


#13 Dieldrin

R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 54508640
Conc: 20.22 ng/ml

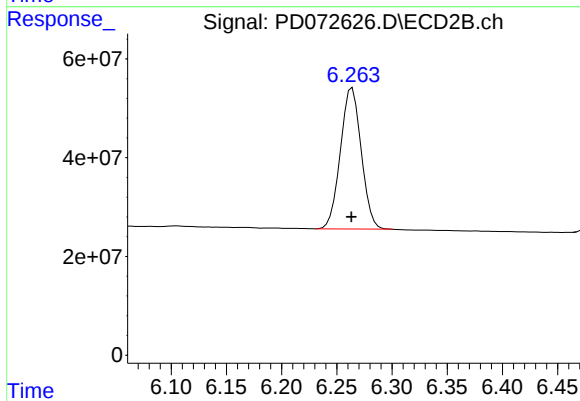

#13 Dieldrin


R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 374571506
Conc: 21.34 ng/ml

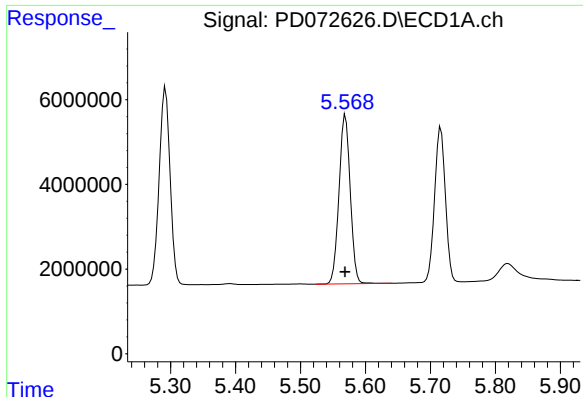

#14 Endrin


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 47946252
Conc: 20.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

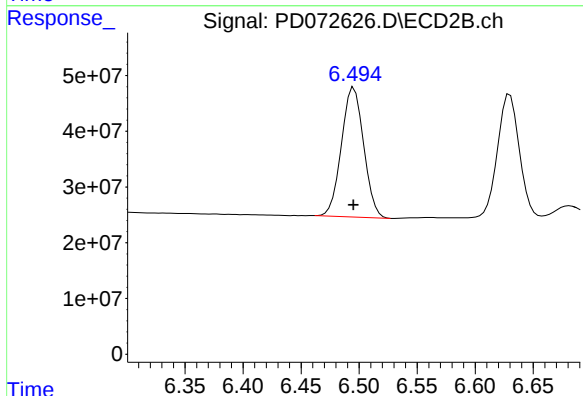


#14 Endrin

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 309656609
Conc: 21.49 ng/ml

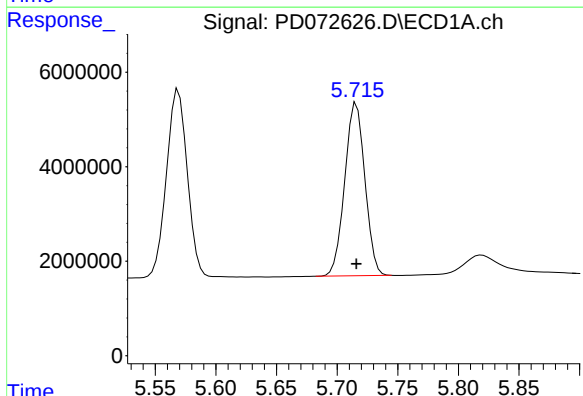


#16 4,4'-DDD

R.T.: 5.716 min
Delta R.T.: 0.000 min
Response: 42366946
Conc: 20.26 ng/ml

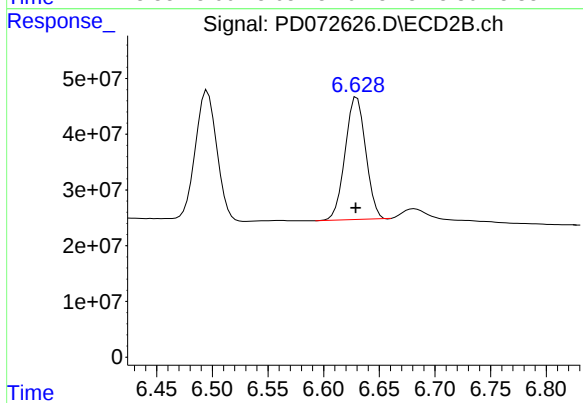

#16 4,4'-DDD


R.T.: 6.630 min
Delta R.T.: 0.001 min
Response: 282684775
Conc: 21.23 ng/ml

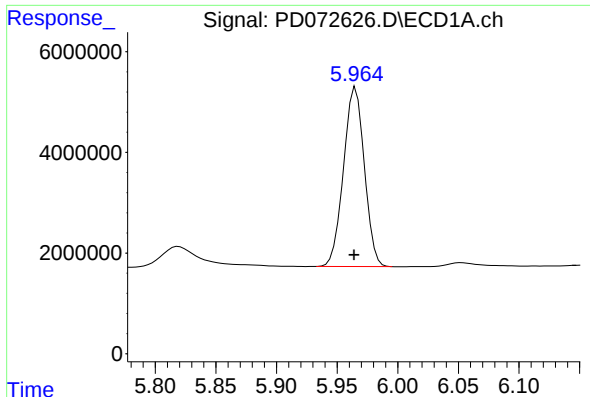

#17 4,4'-DDT


R.T.: 5.965 min
Delta R.T.: 0.001 min
Response: 42598463
Conc: 20.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

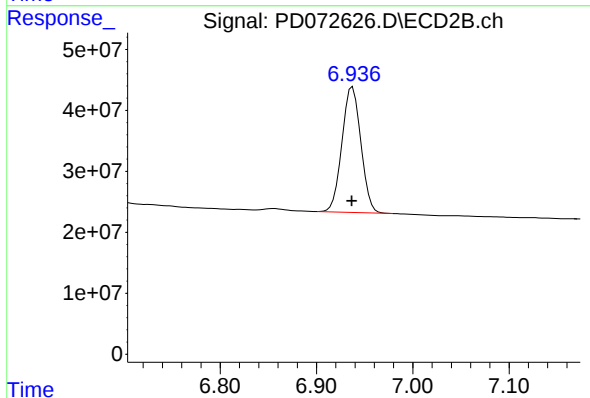


#17 4,4'-DDT

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 279882846
Conc: 20.98 ng/ml

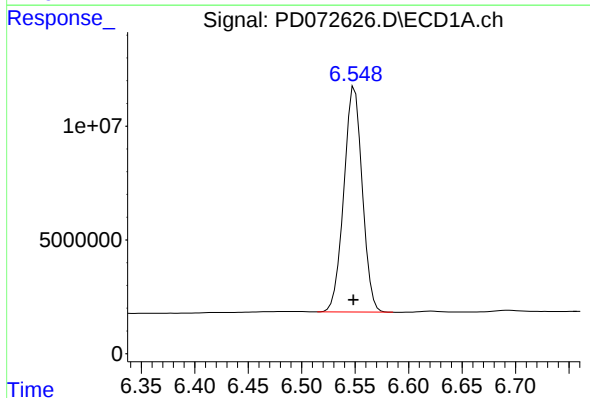


#20 Methoxychlor

R.T.: 6.549 min
Delta R.T.: 0.001 min
Response: 118912074
Conc: 103.75 ng/ml

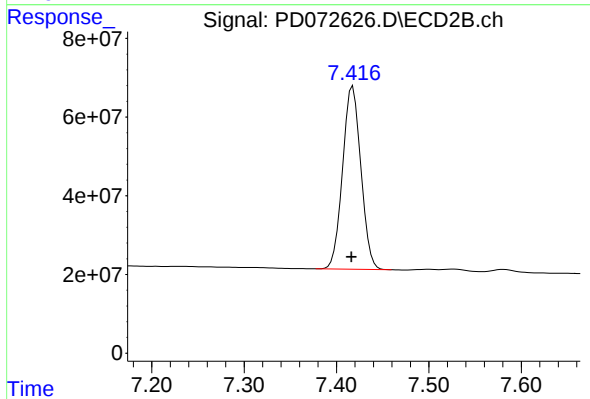

#20 Methoxychlor

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 639195371
Conc: 106.91 ng/ml

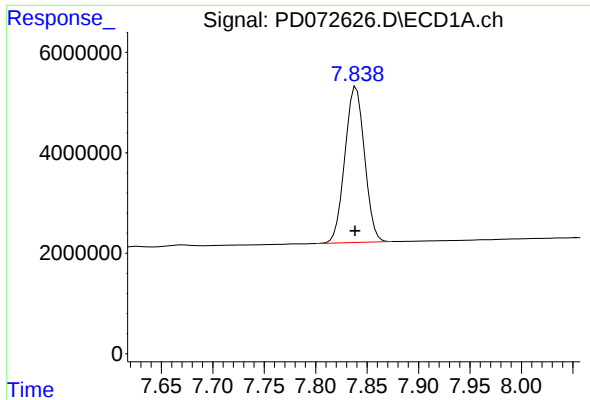

#27 Decachlorobiphenyl


R.T.: 7.839 min

Delta R.T.: 0.000 min

Response: 41266762

Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

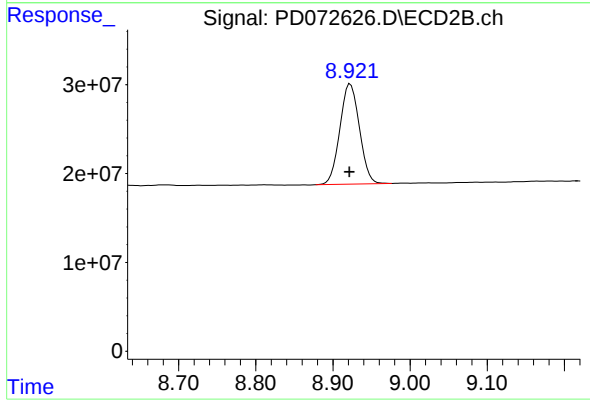

#27 Decachlorobiphenyl

R.T.: 8.923 min

Delta R.T.: 0.002 min

Response: 198110763

Conc: 21.38 ng/ml