

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 13:15
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.465	45381680	786.9E6	20.000	20.000
27)	SA Decachlor...	7.838	8.921	76747975	370.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.209	3.930	68235030	1035.4E6	20.000	20.000
3)	MA gamma-BHC...	3.539	4.264	61982484	832.0E6	20.000	20.000
4)	MA Heptachlor	3.872	4.830	63184118	581.5E6	20.000	20.000
9)	A Endosulfan I	5.025	5.986	49371910	341.0E6	20.000	20.000
13)	MA Dieldrin	5.292	6.263	107.9E6	702.0E6	40.000	40.000
14)	MA Endrin	5.568	6.495	95428278	576.3E6	40.000	40.000
16)	A 4,4'-DDD	5.716	6.629	83654598	532.6E6	40.000	40.000
17)	MA 4,4'-DDT	5.964	6.937	85029029	533.6E6	40.000	40.000
20)	A Methoxychlor	6.548	7.416	229.2E6	1195.7E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 13:15
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

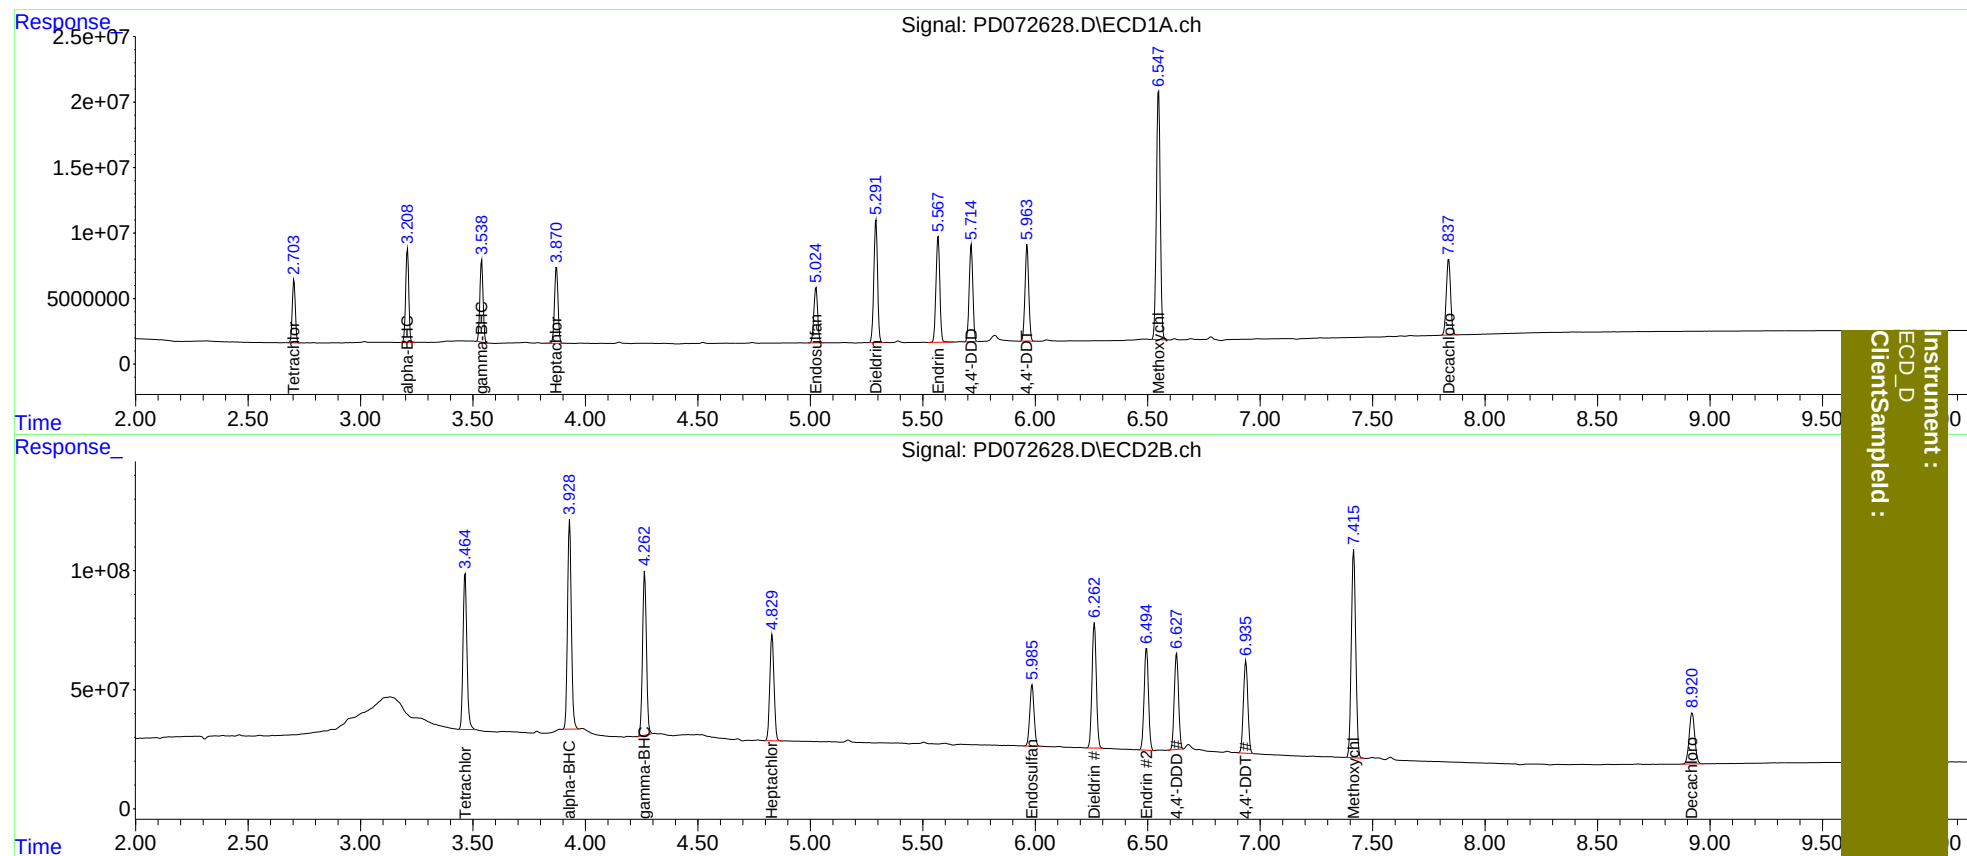


Instrument :
ECD_D
ClientSampled :
0

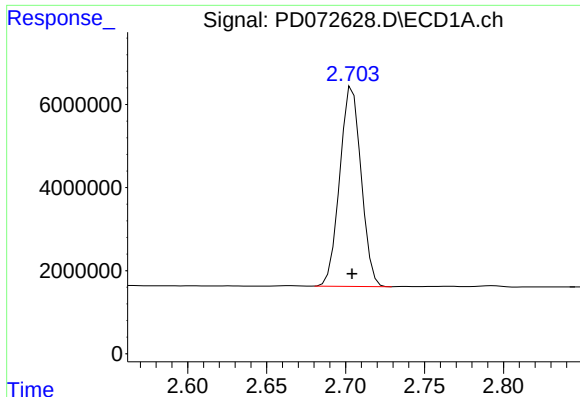

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 45381680
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

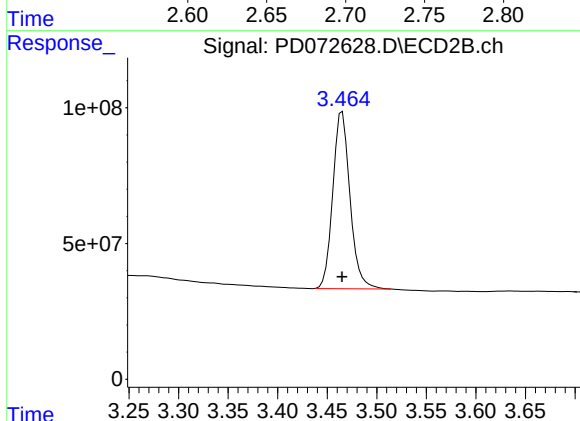


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 786933101
Conc: 20.00 ng/ml

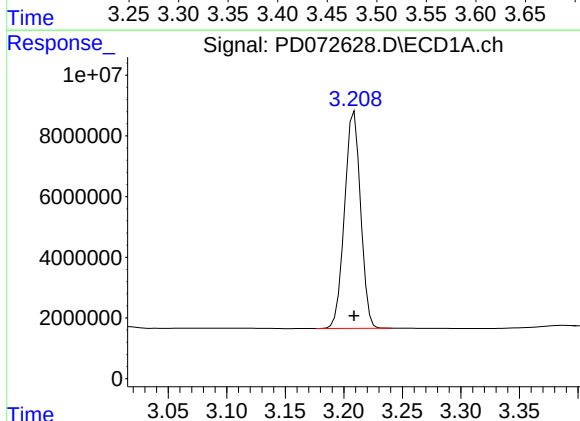


#2 alpha-BHC

R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 68235030
Conc: 20.00 ng/ml

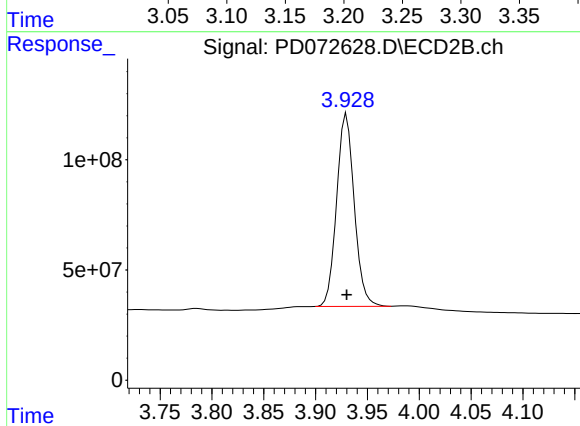

#2 alpha-BHC


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 1035448983
Conc: 20.00 ng/ml

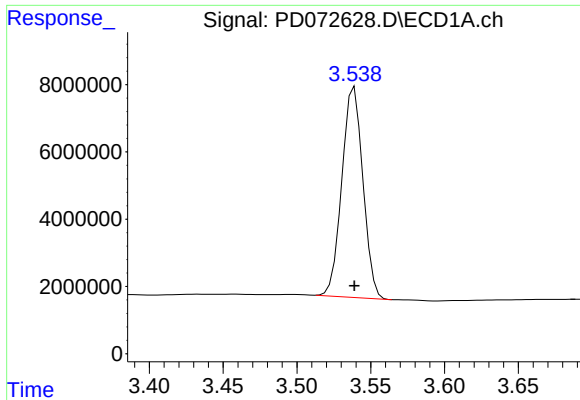

#3 gamma-BHC (Lindane)


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 61982484
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

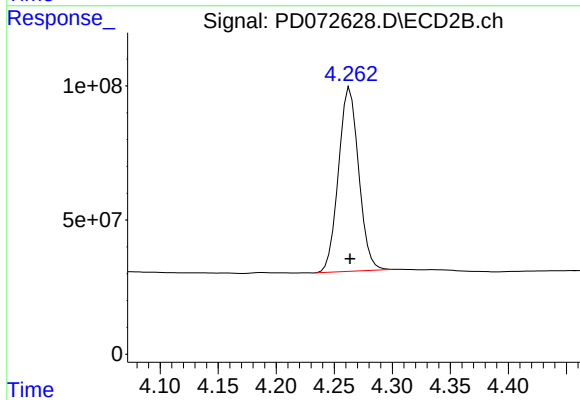


#3 gamma-BHC (Lindane)

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 832018768
Conc: 20.00 ng/ml

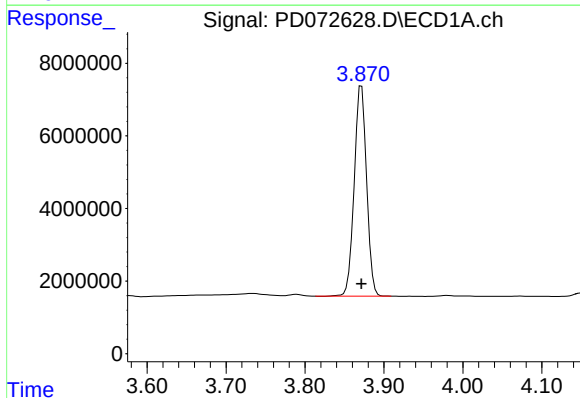


#4 Heptachlor

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 63184118
Conc: 20.00 ng/ml

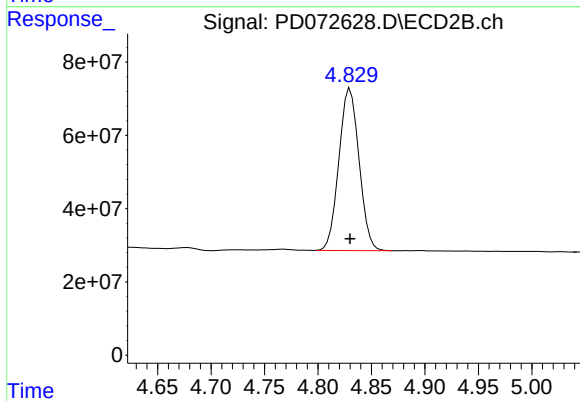

#4 Heptachlor


R.T.: 4.830 min
Delta R.T.: 0.000 min
Response: 581538747
Conc: 20.00 ng/ml

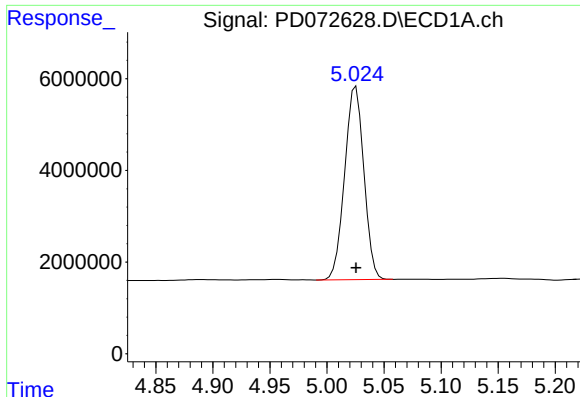

#9 Endosulfan I


R.T.: 5.025 min
Delta R.T.: 0.000 min
Response: 49371910
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

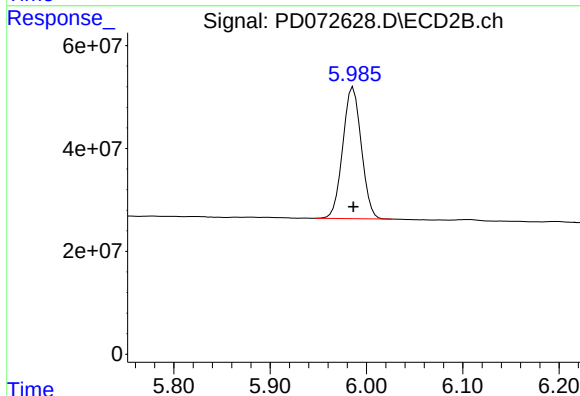


#9 Endosulfan I

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 340967031
Conc: 20.00 ng/ml

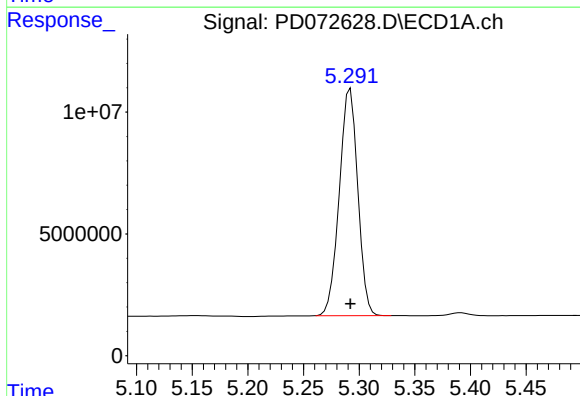


#13 Dieldrin

R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 107852586
Conc: 40.00 ng/ml

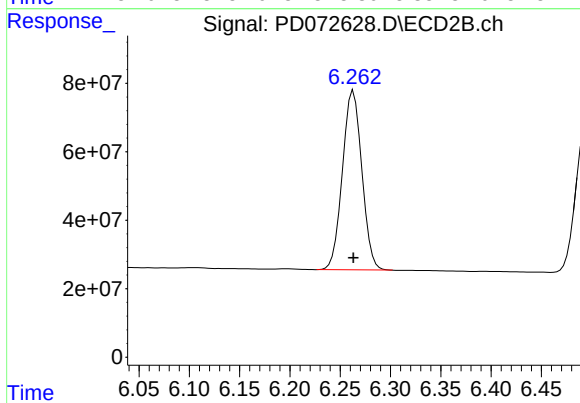

#13 Dieldrin


R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 702001703
Conc: 40.00 ng/ml

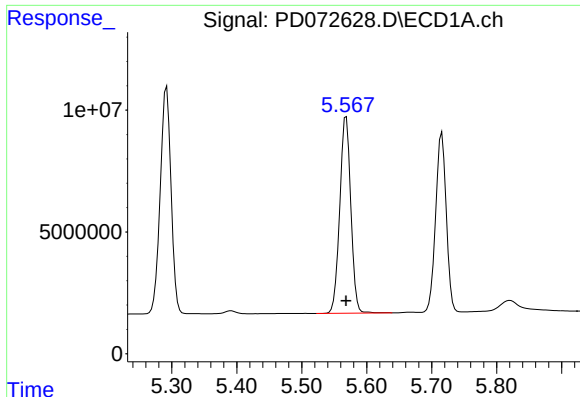

#14 Endrin


R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 95428278
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

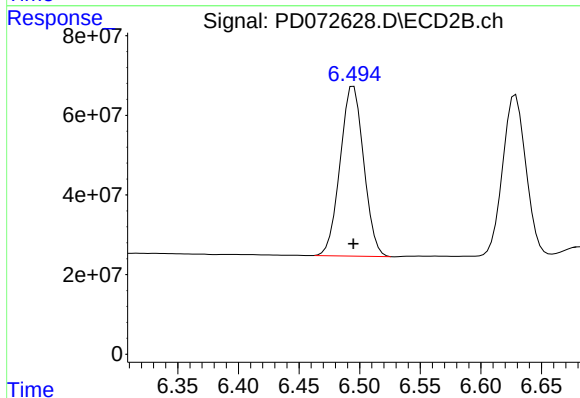


#14 Endrin

R.T.: 6.495 min
Delta R.T.: 0.000 min
Response: 576346086
Conc: 40.00 ng/ml

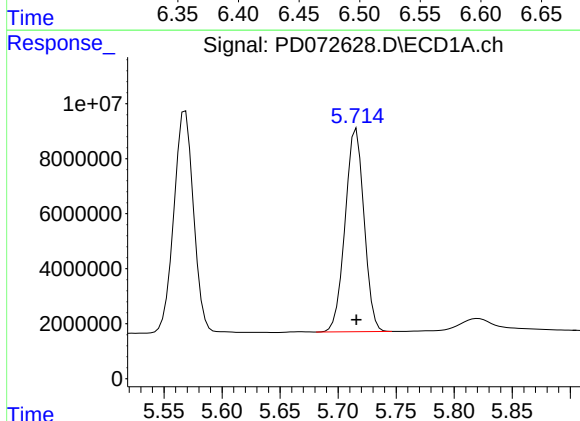


#16 4,4'-DDD

R.T.: 5.716 min
Delta R.T.: 0.000 min
Response: 83654598
Conc: 40.00 ng/ml

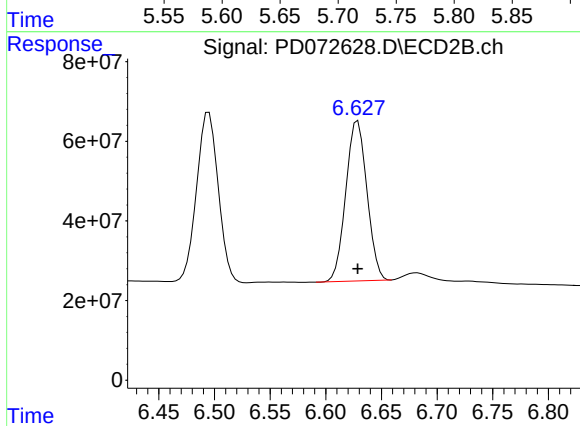

#16 4,4'-DDD


R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 532603596
Conc: 40.00 ng/ml

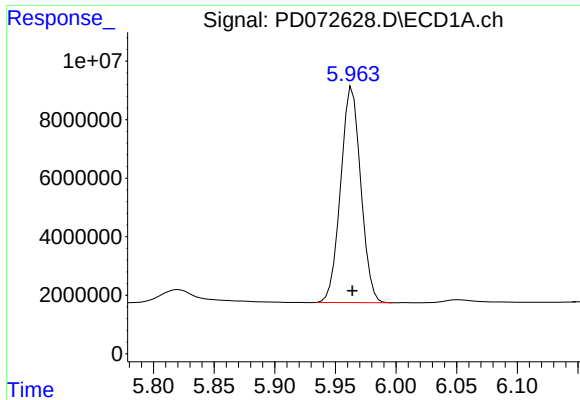

#17 4,4'-DDT


R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 85029029
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

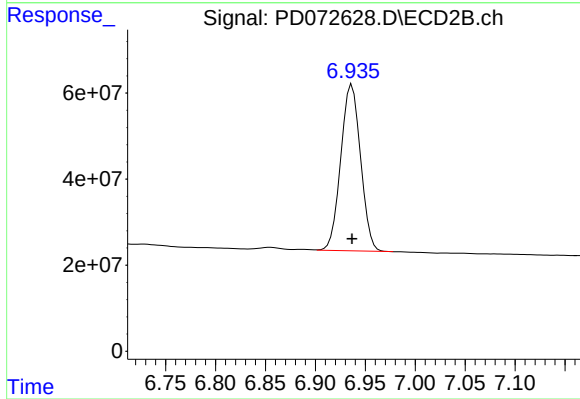


#17 4,4'-DDT

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 533637566
Conc: 40.00 ng/ml

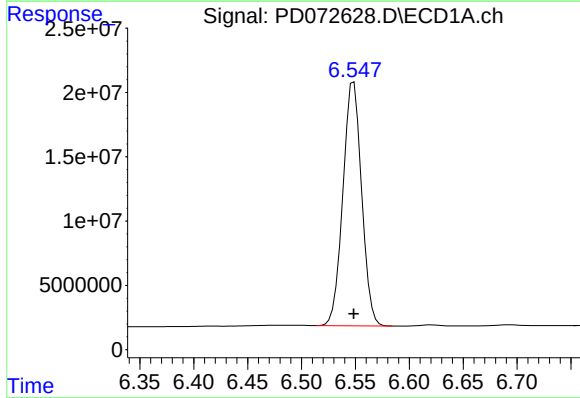


#20 Methoxychlor

R.T.: 6.548 min
Delta R.T.: 0.000 min
Response: 229234635
Conc: 200.00 ng/ml

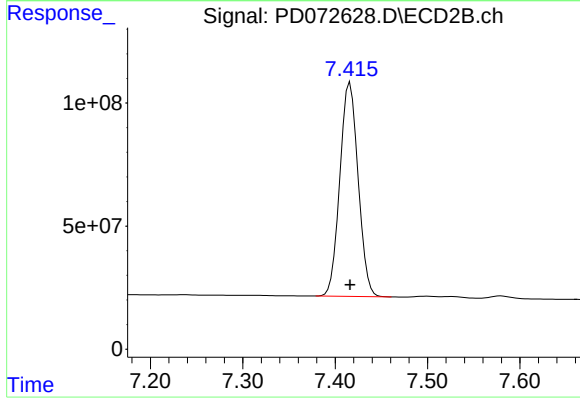

#20 Methoxychlor


R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1195719208
Conc: 200.00 ng/ml

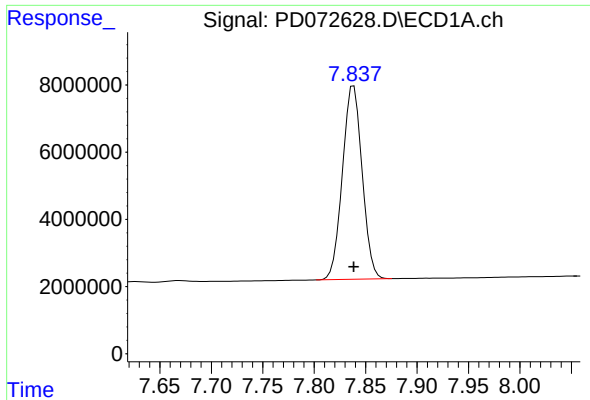

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 76747975
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

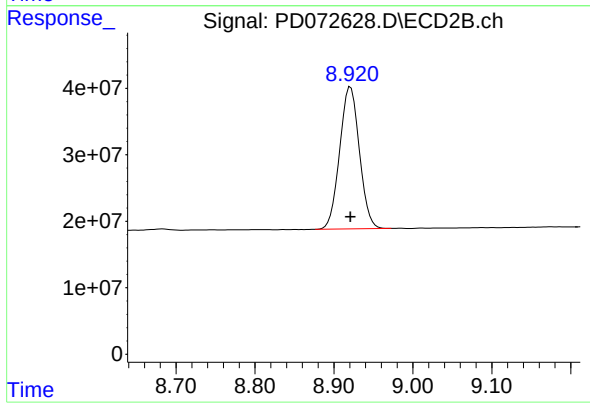

#27 Decachlorobiphenyl

R.T.: 8.921 min
Delta R.T.: 0.000 min
Response: 370728180
Conc: 40.00 ng/ml