

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 13:42
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.466	90658657	1522.4E6	39.954	38.691
27)	SA Decachlor...	7.838	8.921	148.4E6	722.8E6	77.334	77.989
Target Compounds							
2)	A alpha-BHC	3.208	3.930	144.3E6	2004.0E6	42.282	38.708
3)	MA gamma-BHC...	3.539	4.264	129.7E6	1582.5E6	41.836	38.040
4)	MA Heptachlor	3.872	4.831	129.9E6	1094.0E6	41.113	37.625
9)	A Endosulfan I	5.026	5.987	99463917	655.2E6	40.292	38.434
13)	MA Dieldrin	5.292	6.264	224.1E6	1362.1E6	83.115	77.610
14)	MA Endrin	5.569	6.496	197.3E6	1111.8E6	82.695	77.162
16)	A 4,4'-DDD	5.716	6.630	172.6E6	1047.6E6	82.516	78.679
17)	MA 4,4'-DDT	5.965	6.937	177.4E6	1050.0E6	83.458	78.702
20)	A Methoxychlor	6.549	7.416	454.5E6	2315.7E6	396.578	387.336


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 13:42
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

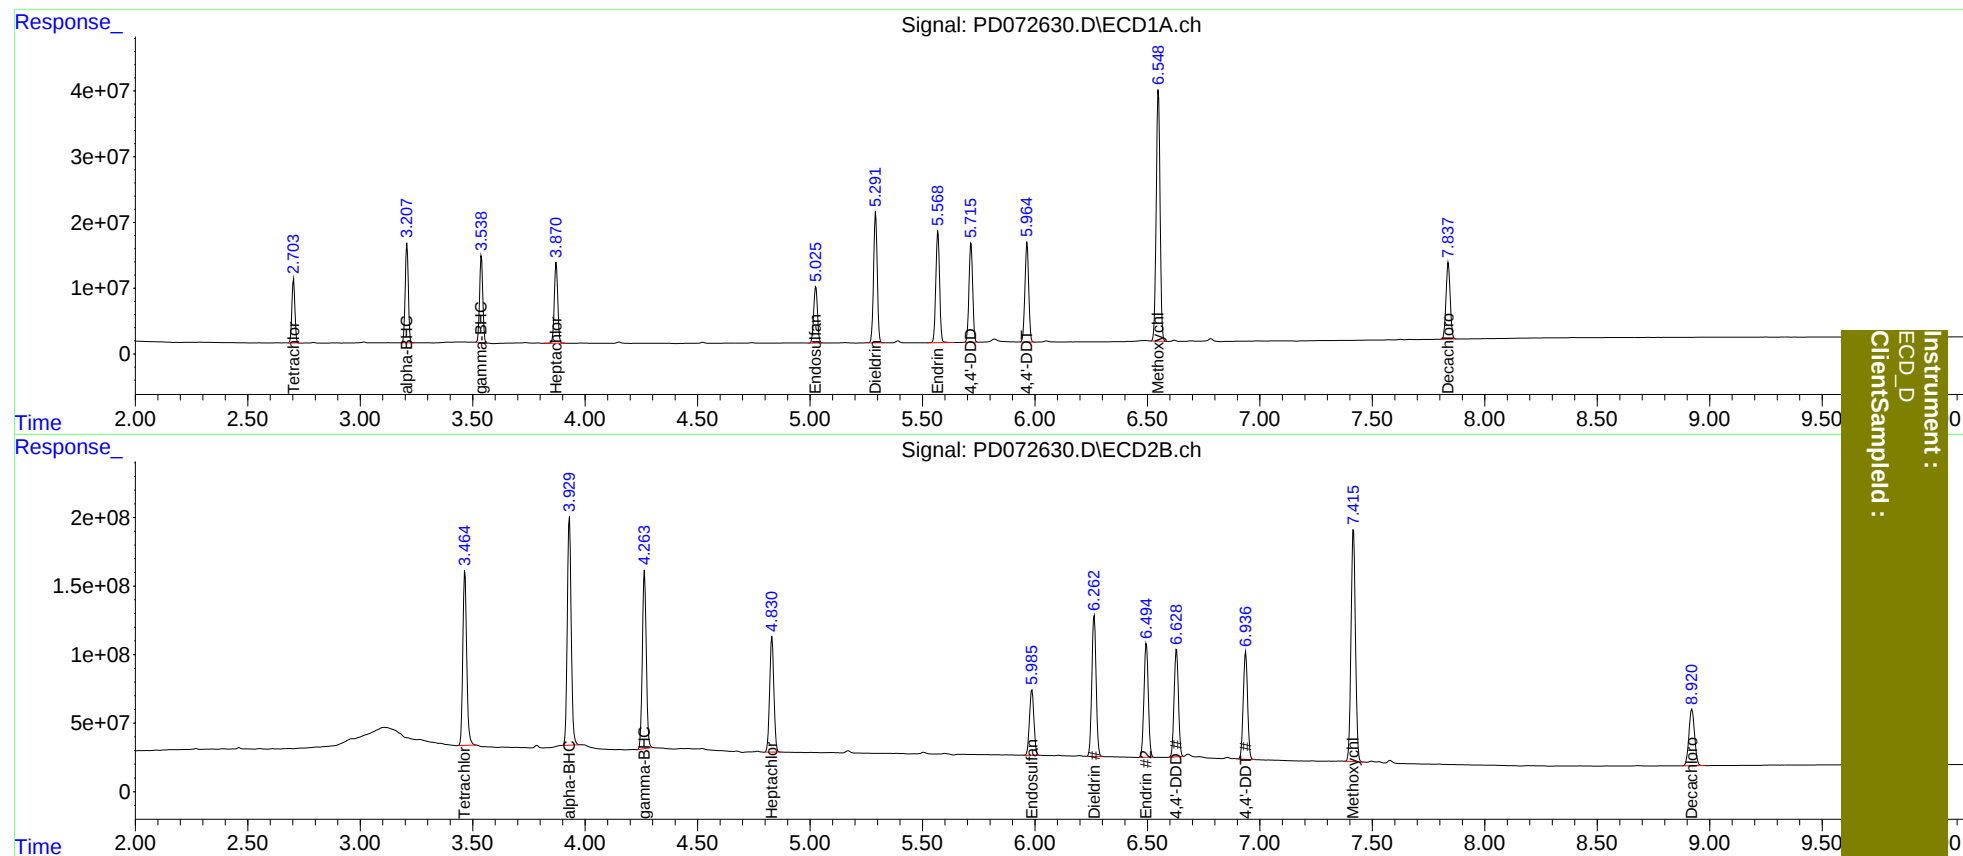


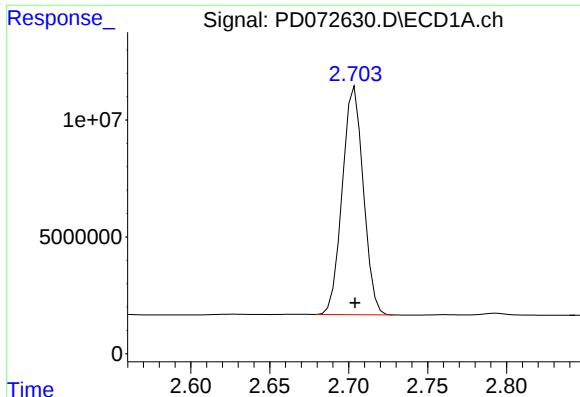

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 90658657
Conc: 39.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

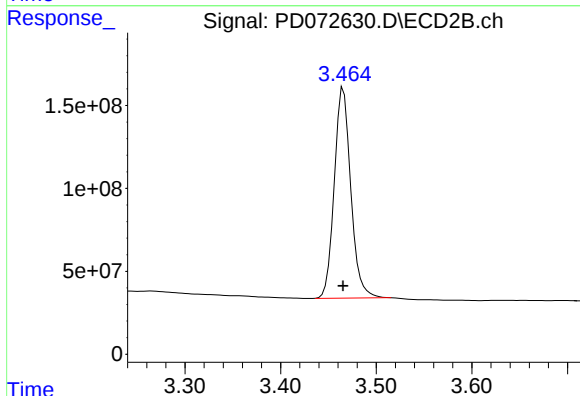


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 1522374477
Conc: 38.69 ng/ml

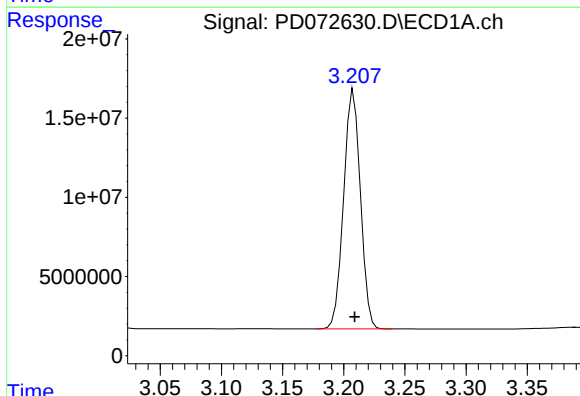


#2 alpha-BHC

R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 144255622
Conc: 42.28 ng/ml

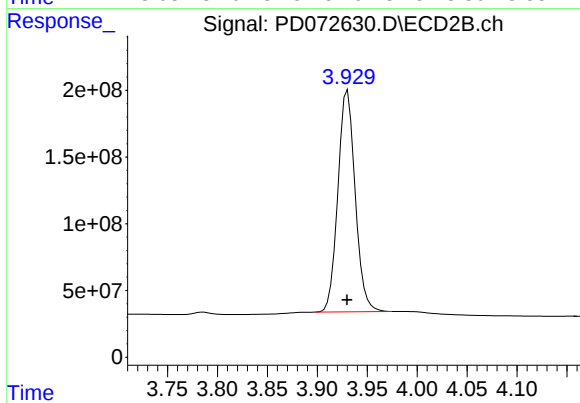

#2 alpha-BHC


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 2004015438
Conc: 38.71 ng/ml

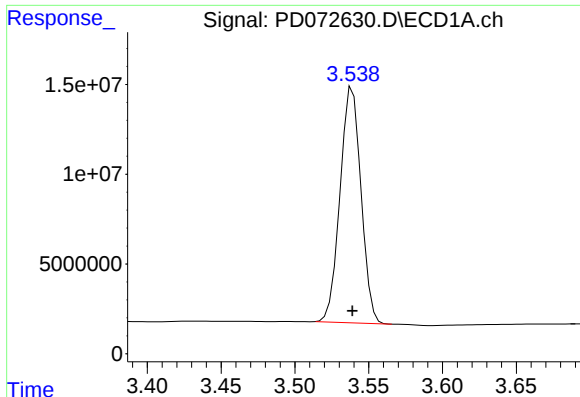

#3 gamma-BHC (Lindane)


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 129655998
Conc: 41.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

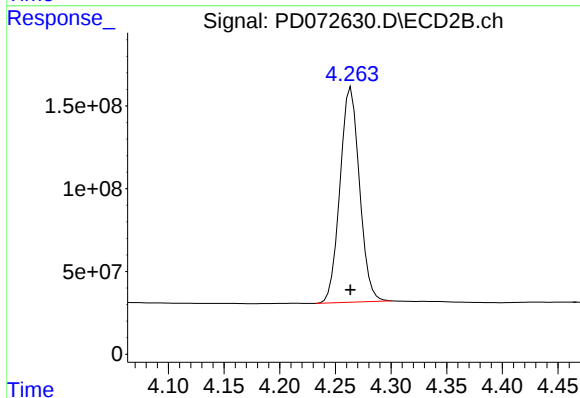


#3 gamma-BHC (Lindane)

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 1582487919
Conc: 38.04 ng/ml

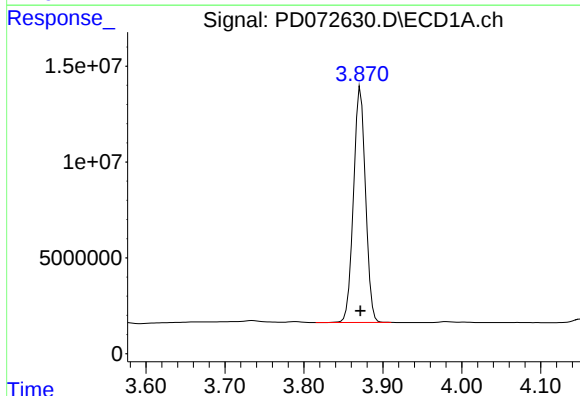


#4 Heptachlor

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 129883249
Conc: 41.11 ng/ml

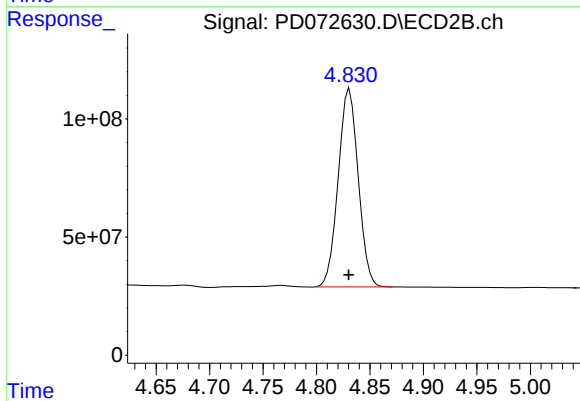

#4 Heptachlor


R.T.: 4.831 min
Delta R.T.: 0.000 min
Response: 1094022161
Conc: 37.63 ng/ml

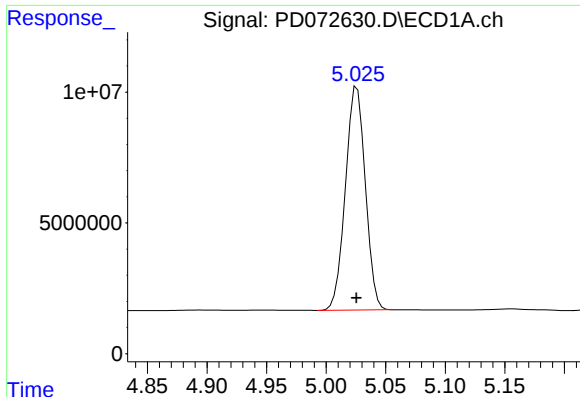

#9 Endosulfan I


R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 99463917
Conc: 40.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

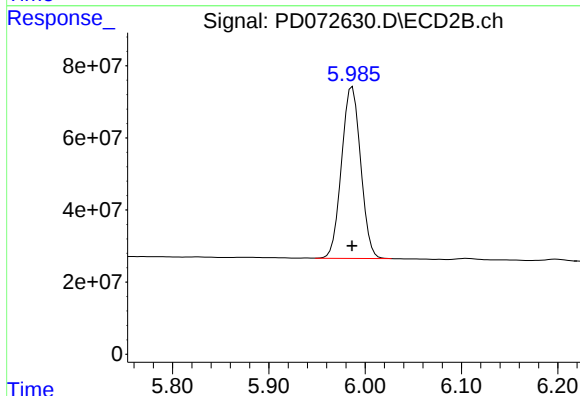


#9 Endosulfan I

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 655232325
Conc: 38.43 ng/ml

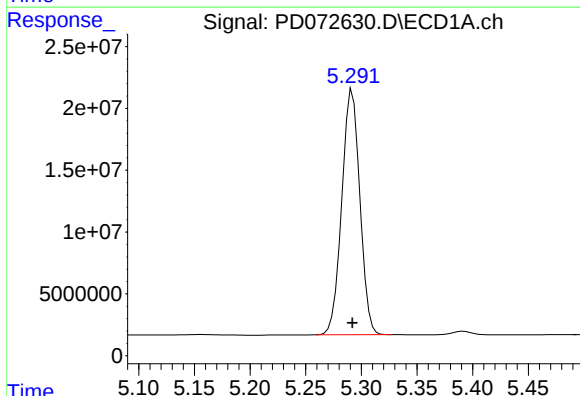


#13 Dieldrin

R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 224104223
Conc: 83.12 ng/ml

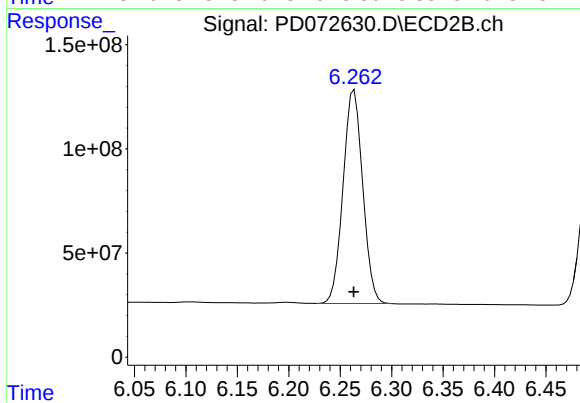

#13 Dieldrin


R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 1362060422
Conc: 77.61 ng/ml

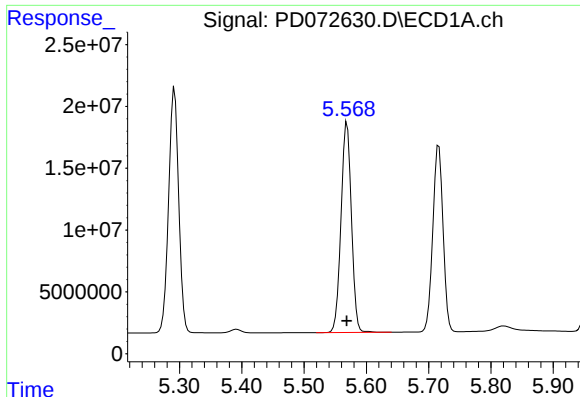

#14 Endrin


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 197286339
Conc: 82.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

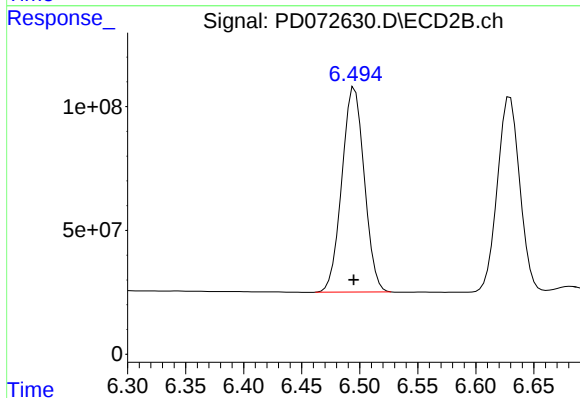


#14 Endrin

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 1111793222
Conc: 77.16 ng/ml

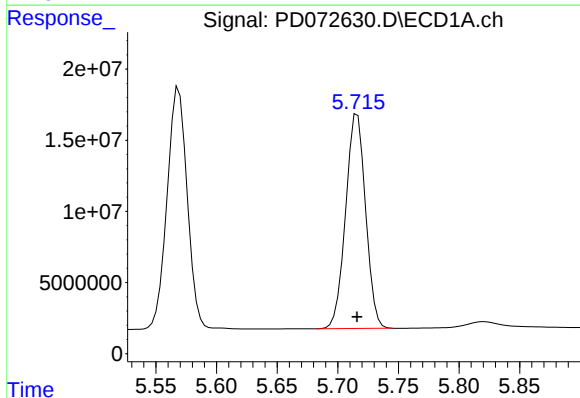


#16 4,4'-DDD

R.T.: 5.716 min
Delta R.T.: 0.000 min
Response: 172571474
Conc: 82.52 ng/ml

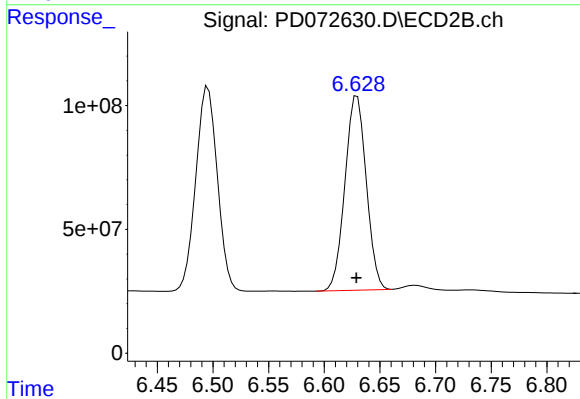

#16 4,4'-DDD


R.T.: 6.630 min
Delta R.T.: 0.000 min
Response: 1047623876
Conc: 78.68 ng/ml

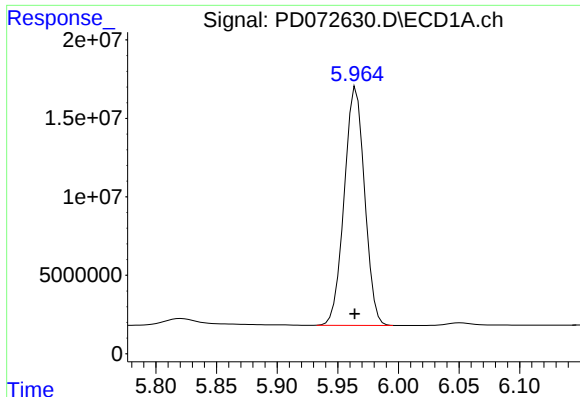

#17 4,4'-DDT


R.T.: 5.965 min
Delta R.T.: 0.001 min
Response: 177408312
Conc: 83.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

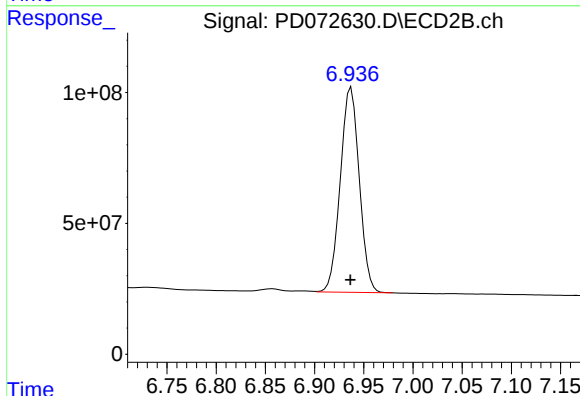


#17 4,4'-DDT

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 1049963109
Conc: 78.70 ng/ml

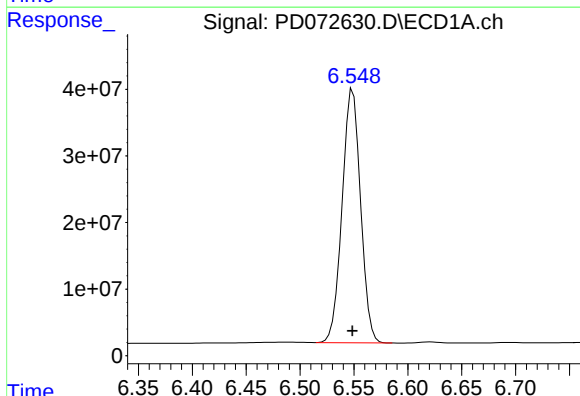


#20 Methoxychlor

R.T.: 6.549 min
Delta R.T.: 0.000 min
Response: 454546971
Conc: 396.58 ng/ml

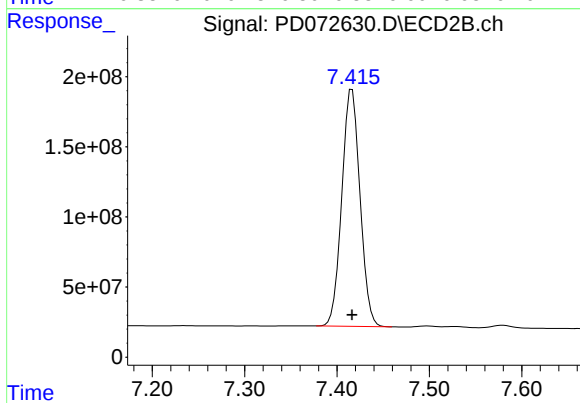

#20 Methoxychlor


R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 2315728144
Conc: 387.34 ng/ml

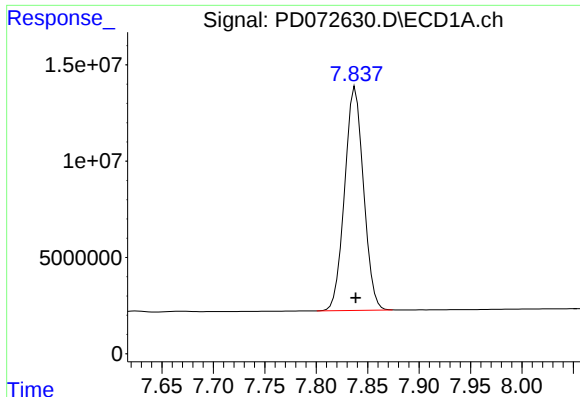

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 148380664
Conc: 77.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

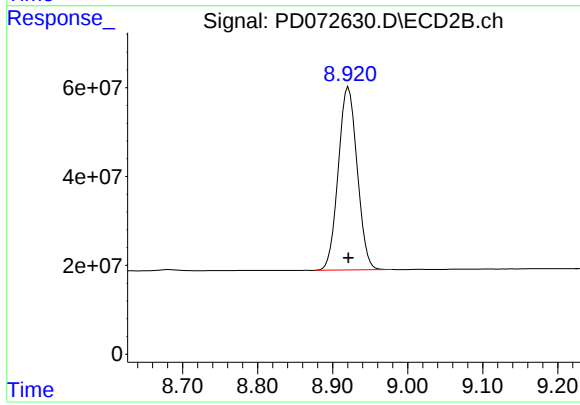

#27 Decachlorobiphenyl

R.T.: 8.921 min
Delta R.T.: 0.000 min
Response: 722822566
Conc: 77.99 ng/ml