

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 14:08
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.466	177.4E6	2842.6E6	78.168	72.245
27)	SA Decachlor...	7.838	8.921	279.8E6	1336.8E6	145.852	144.238
Target Compounds							
2)	A alpha-BHC	3.208	3.930	291.6E6	3769.8E6	85.482	72.814
3)	MA gamma-BHC...	3.539	4.264	260.0E6	2940.3E6	83.880	70.678
4)	MA Heptachlor	3.872	4.831	257.0E6	1982.2E6	81.343	68.172
9)	A Endosulfan I	5.026	5.986	193.9E6	1197.6E6	78.527	70.248
13)	MA Dieldrin	5.292	6.263	441.6E6	2533.0E6	163.795	144.330
14)	MA Endrin	5.569	6.496	384.0E6	2068.7E6	160.968	143.573
16)	A 4,4'-DDD	5.716	6.629	341.0E6	1951.2E6	163.041	146.537
17)	MA 4,4'-DDT	5.965	6.937	350.4E6	1973.6E6	164.841	147.937
20)	A Methoxychlor	6.549	7.417	860.1E6	4232.4E6	750.430	707.926


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 14:08
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

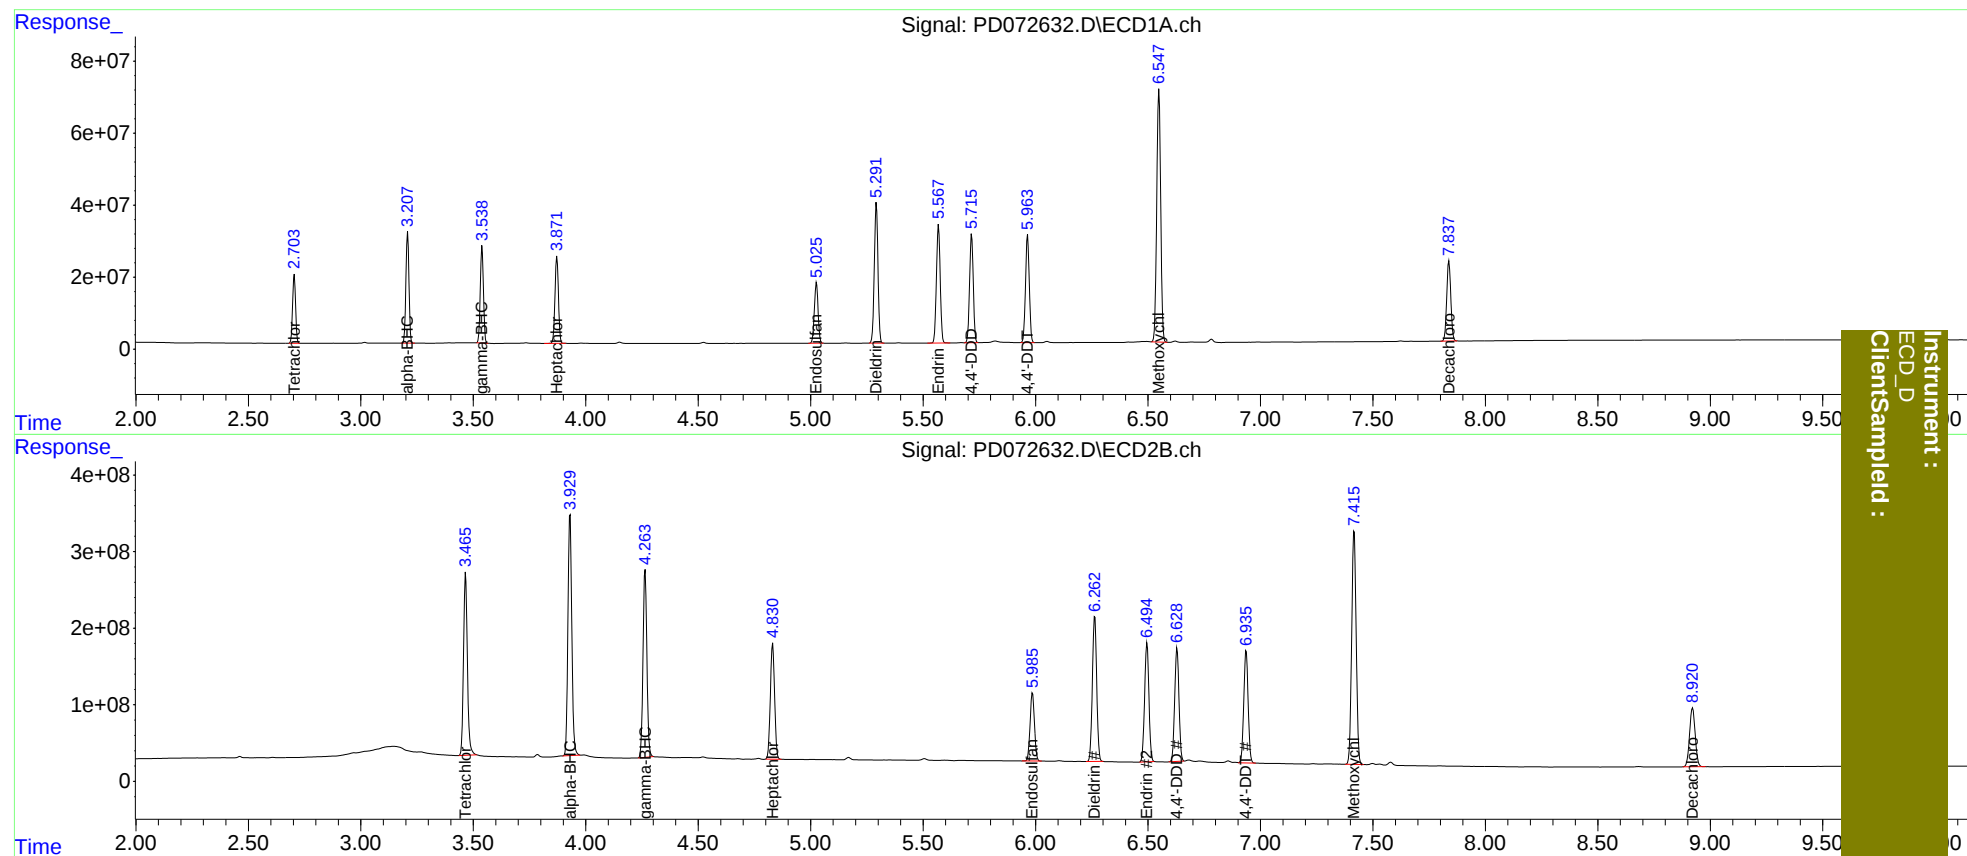


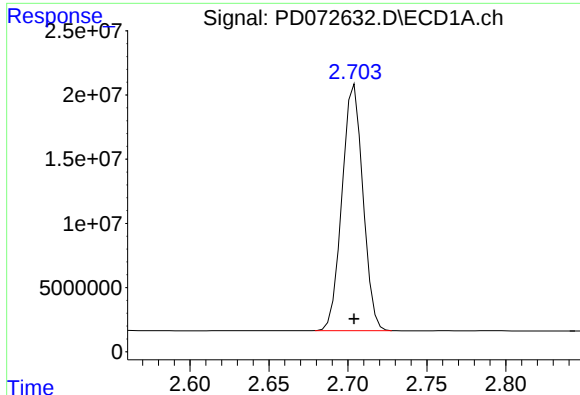

#1 Tetrachloro-m-xylene


R.T.: 2.704 min
Delta R.T.: 0.000 min
Response: 177369356
Conc: 78.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

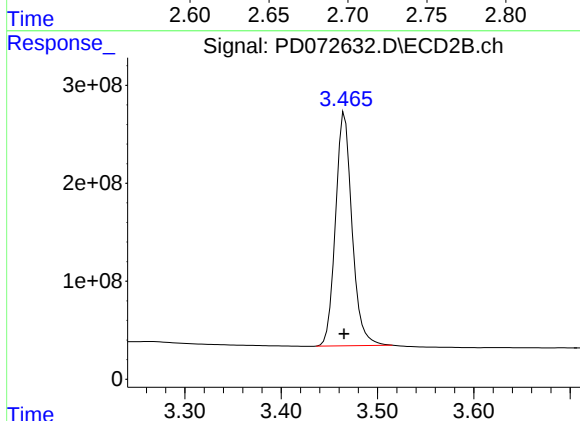


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 2842609540
Conc: 72.25 ng/ml

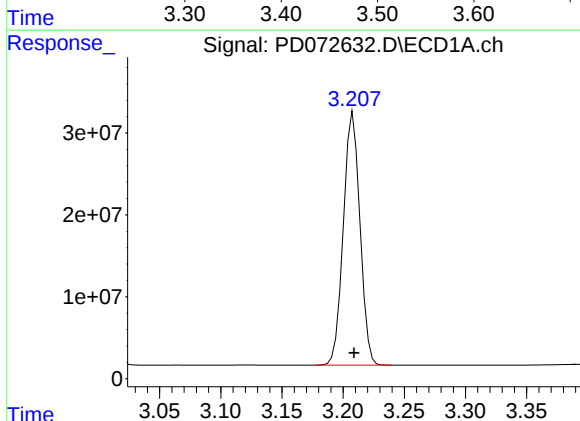


#2 alpha-BHC

R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 291642293
Conc: 85.48 ng/ml

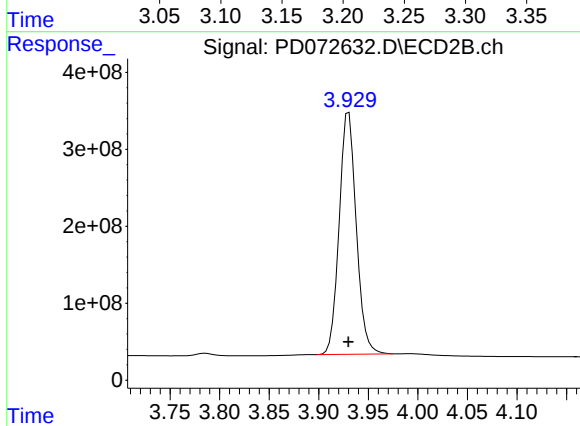

#2 alpha-BHC


R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 3769765878
Conc: 72.81 ng/ml

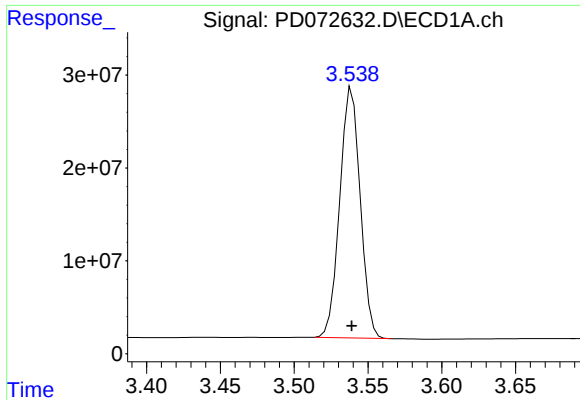

#3 gamma-BHC (Lindane)


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 259953710
Conc: 83.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

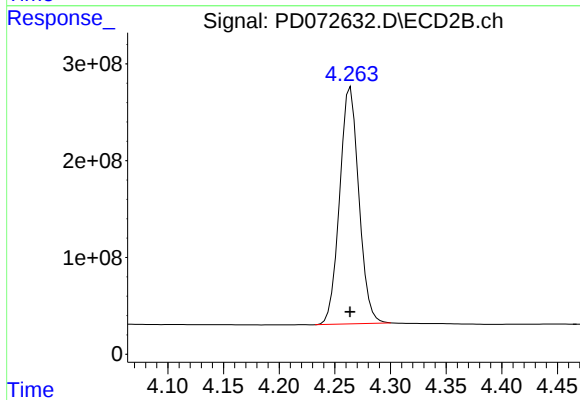


#3 gamma-BHC (Lindane)

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 2940253422
Conc: 70.68 ng/ml

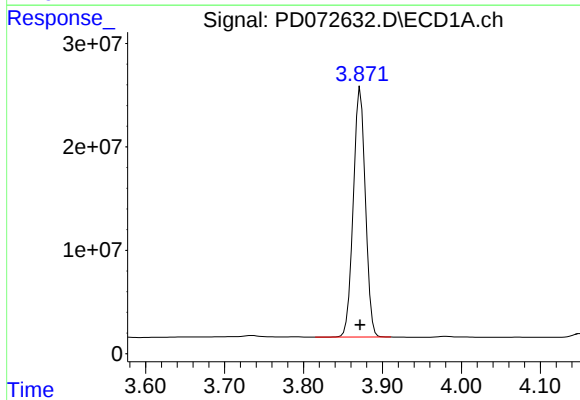


#4 Heptachlor

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 256980301
Conc: 81.34 ng/ml

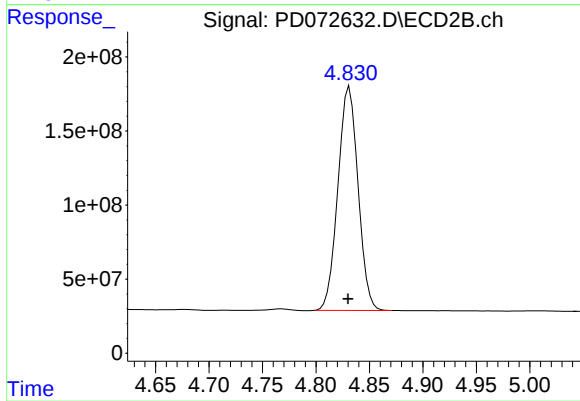

#4 Heptachlor


R.T.: 4.831 min
Delta R.T.: 0.001 min
Response: 1982228903
Conc: 68.17 ng/ml

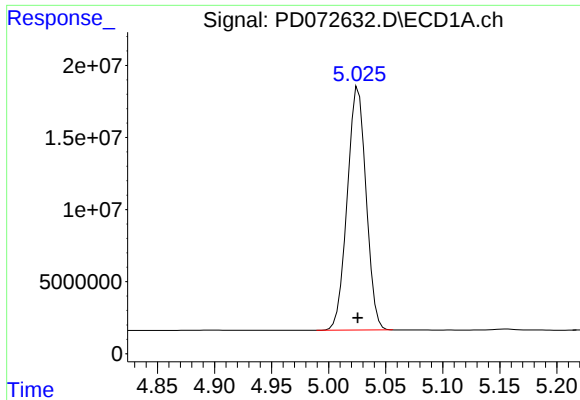

#9 Endosulfan I


R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 193850519
Conc: 78.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

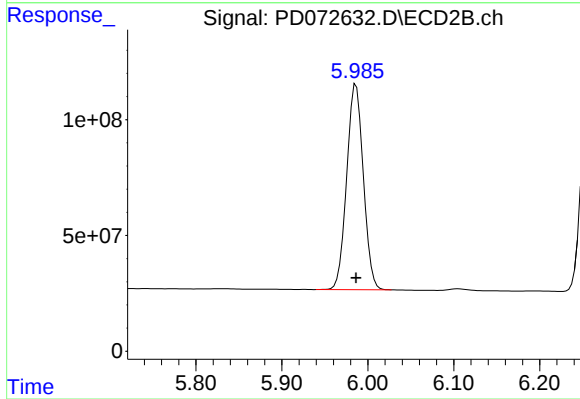


#9 Endosulfan I

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 1197605837
Conc: 70.25 ng/ml

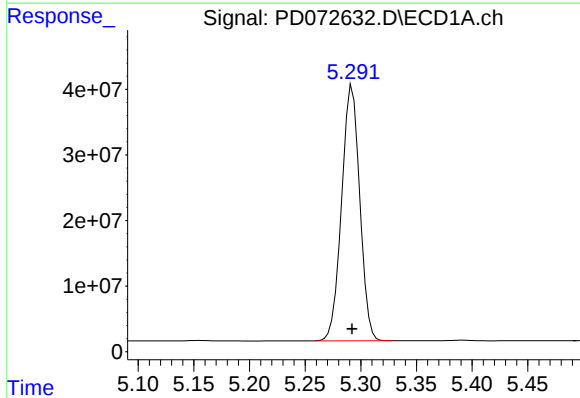


#13 Dieldrin

R.T.: 5.292 min
Delta R.T.: 0.000 min
Response: 441643061
Conc: 163.80 ng/ml

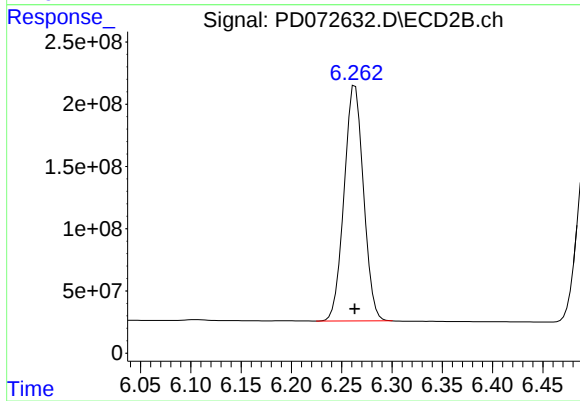

#13 Dieldrin


R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 2532993027
Conc: 144.33 ng/ml

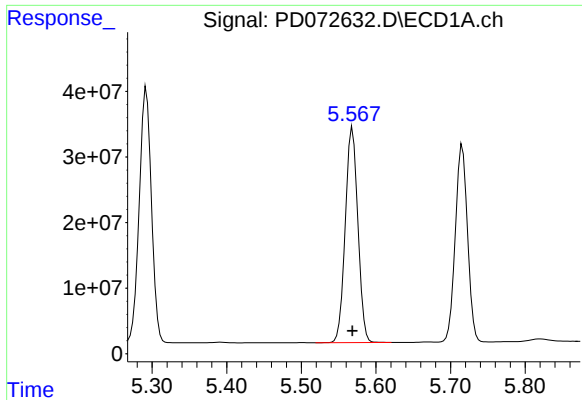

#14 Endrin


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 384021601
Conc: 160.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

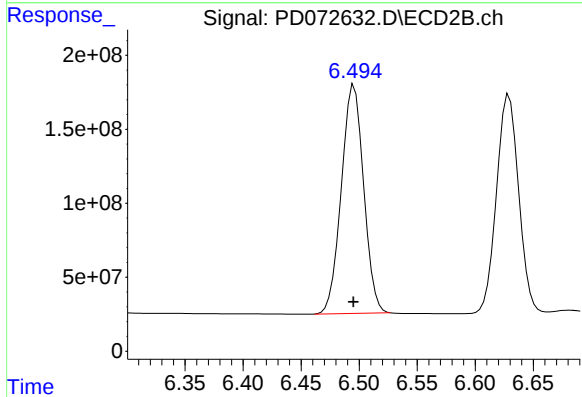


#14 Endrin

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 2068691332
Conc: 143.57 ng/ml

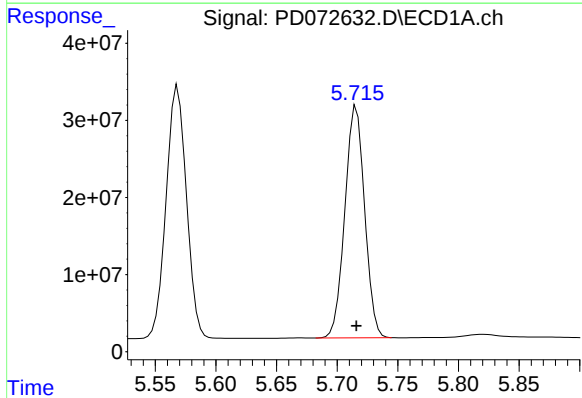


#16 4,4'-DDD

R.T.: 5.716 min
Delta R.T.: 0.000 min
Response: 340977466
Conc: 163.04 ng/ml

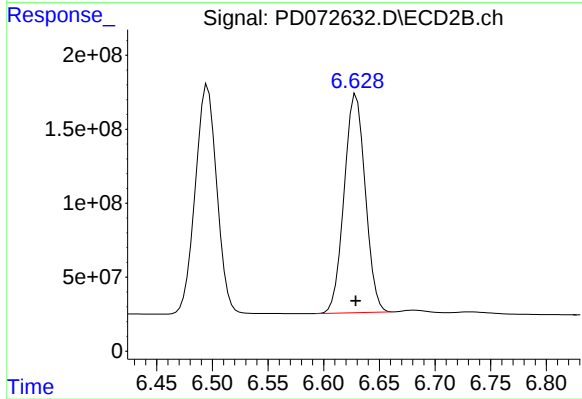

#16 4,4'-DDD


R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 1951156914
Conc: 146.54 ng/ml

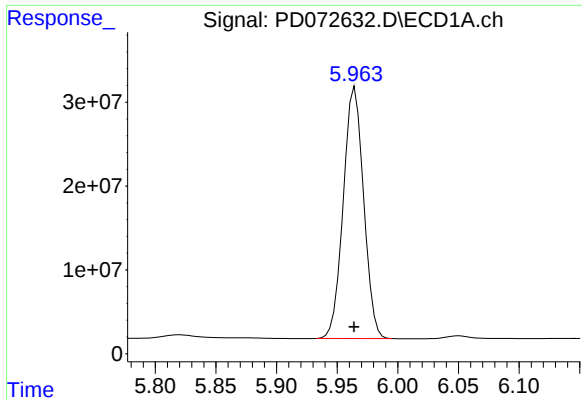

#17 4,4'-DDT


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 350406337
Conc: 164.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

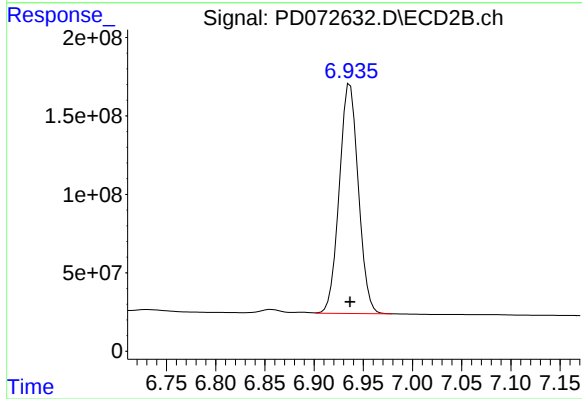


#17 4,4'-DDT

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 1973620749
Conc: 147.94 ng/ml

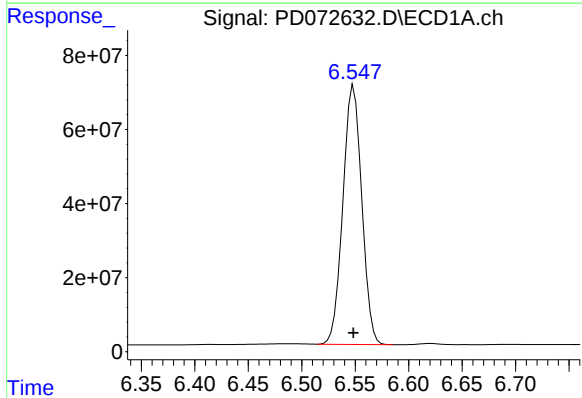


#20 Methoxychlor

R.T.: 6.549 min
Delta R.T.: 0.000 min
Response: 860122464
Conc: 750.43 ng/ml

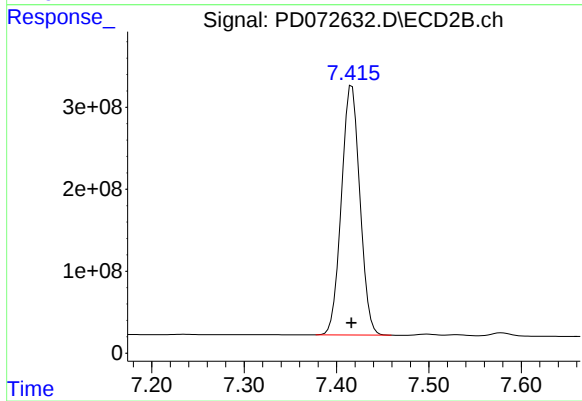

#20 Methoxychlor


R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 4232405320
Conc: 707.93 ng/ml

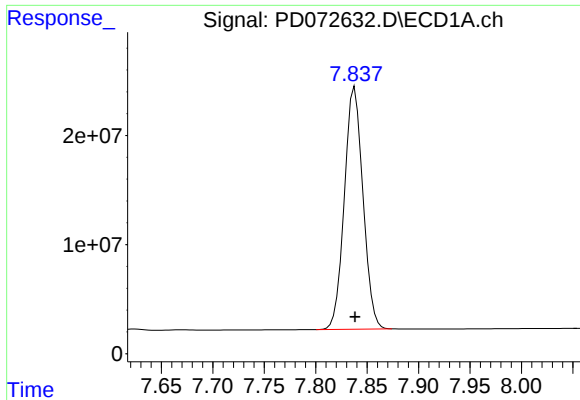

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 279845766
Conc: 145.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

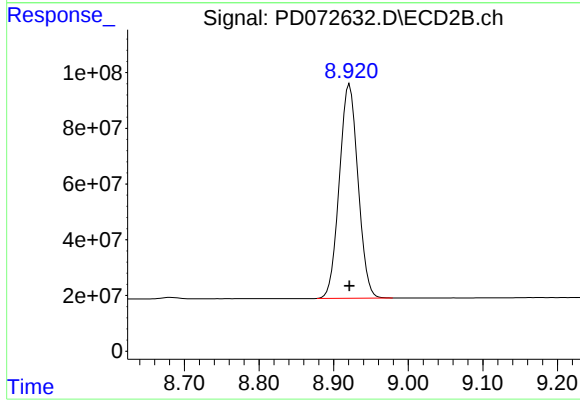

#27 Decachlorobiphenyl

R.T.: 8.921 min
Delta R.T.: 0.000 min
Response: 1336830052
Conc: 144.24 ng/ml