

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 13:15
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3061

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.465	45381680	786.9E6	20.000	20.000
27)	SA Decachlor...	7.838	8.921	76747975	370.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.209	3.930	68235030	1035.4E6	20.000	20.000
3)	MA gamma-BHC...	3.539	4.264	61982484	832.0E6	20.000	20.000
4)	MA Heptachlor	3.872	4.830	63184118	581.5E6	20.000	20.000
9)	A Endosulfan I	5.025	5.986	49371910	341.0E6	20.000	20.000
13)	MA Dieldrin	5.292	6.263	107.9E6	702.0E6	40.000	40.000
14)	MA Endrin	5.568	6.495	95428278	576.3E6	40.000	40.000
16)	A 4,4'-DDD	5.716	6.629	83654598	532.6E6	40.000	40.000
17)	MA 4,4'-DDT	5.964	6.937	85029029	533.6E6	40.000	40.000
20)	A Methoxychlor	6.548	7.416	229.2E6	1195.7E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 13:15
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

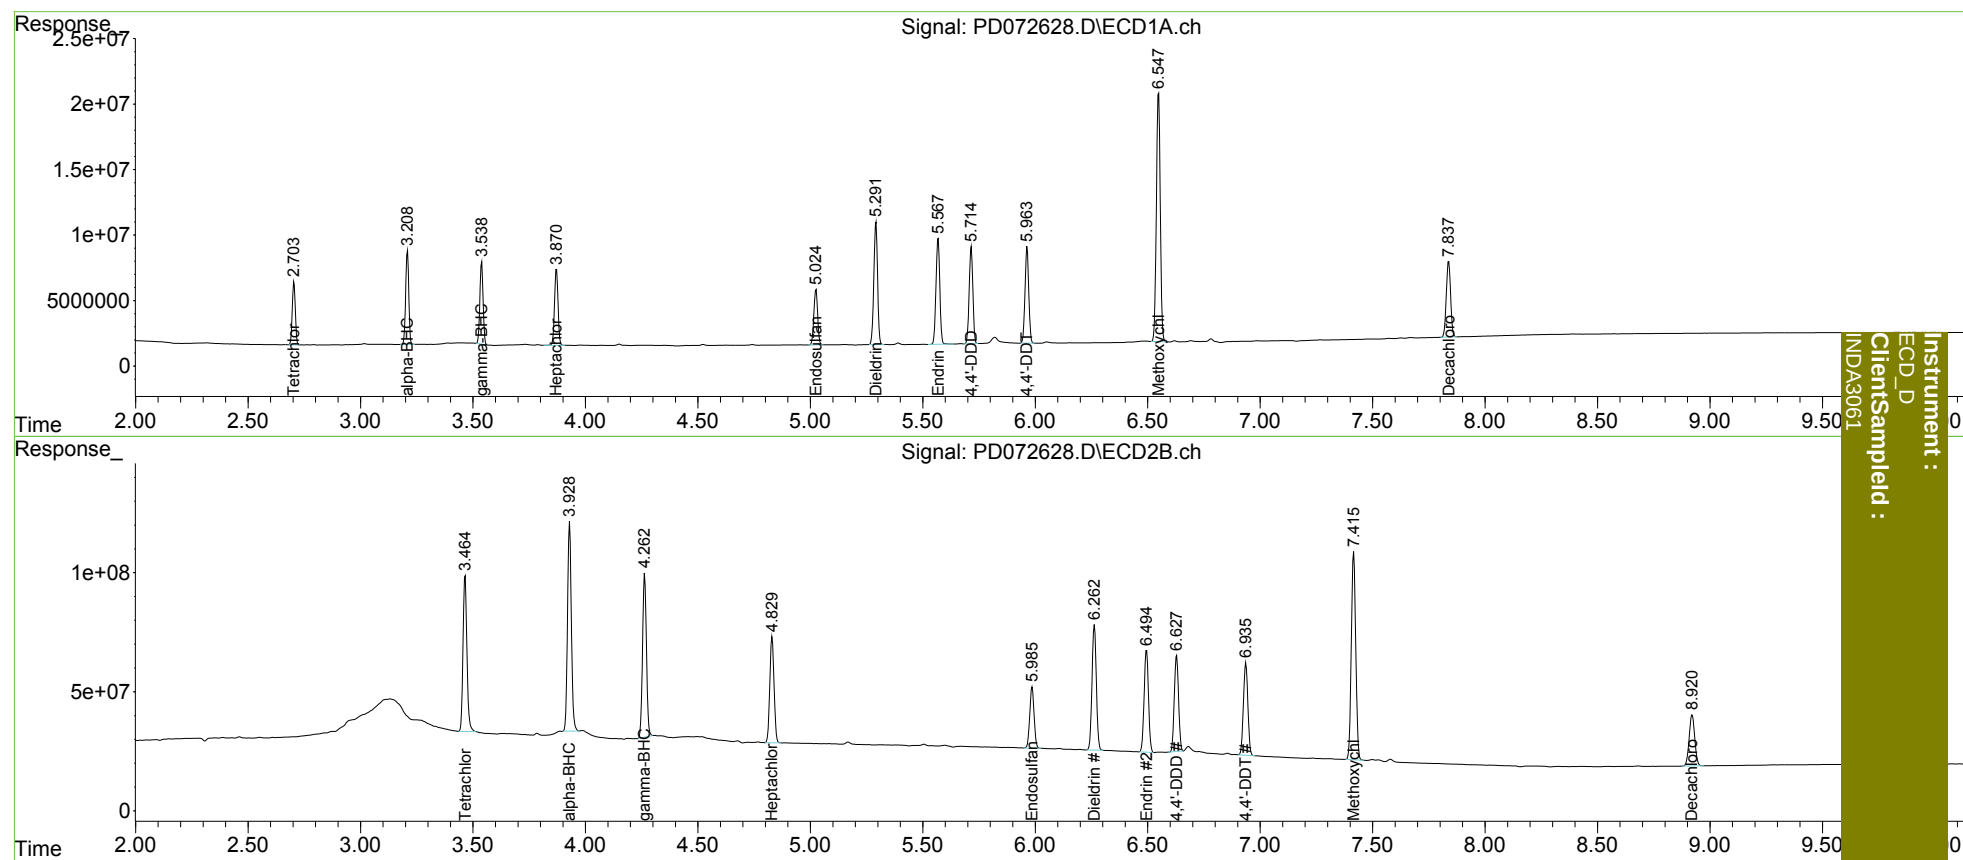

Instrument :
ECD_D
ClientSampled :
INDA3061