

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 14:08
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5065

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.466	177.4E6	2842.6E6	78.168	72.245
27)	SA Decachlor...	7.838	8.921	279.8E6	1336.8E6	145.852	144.238
Target Compounds							
2)	A alpha-BHC	3.208	3.930	291.6E6	3769.8E6	85.482	72.814
3)	MA gamma-BHC...	3.539	4.264	260.0E6	2940.3E6	83.880	70.678
4)	MA Heptachlor	3.872	4.831	257.0E6	1982.2E6	81.343	68.172
9)	A Endosulfan I	5.026	5.986	193.9E6	1197.6E6	78.527	70.248
13)	MA Dieldrin	5.292	6.263	441.6E6	2533.0E6	163.795	144.330
14)	MA Endrin	5.569	6.496	384.0E6	2068.7E6	160.968	143.573
16)	A 4,4'-DDD	5.716	6.629	341.0E6	1951.2E6	163.041	146.537
17)	MA 4,4'-DDT	5.965	6.937	350.4E6	1973.6E6	164.841	147.937
20)	A Methoxychlor	6.549	7.417	860.1E6	4232.4E6	750.430	707.926

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 14:08
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

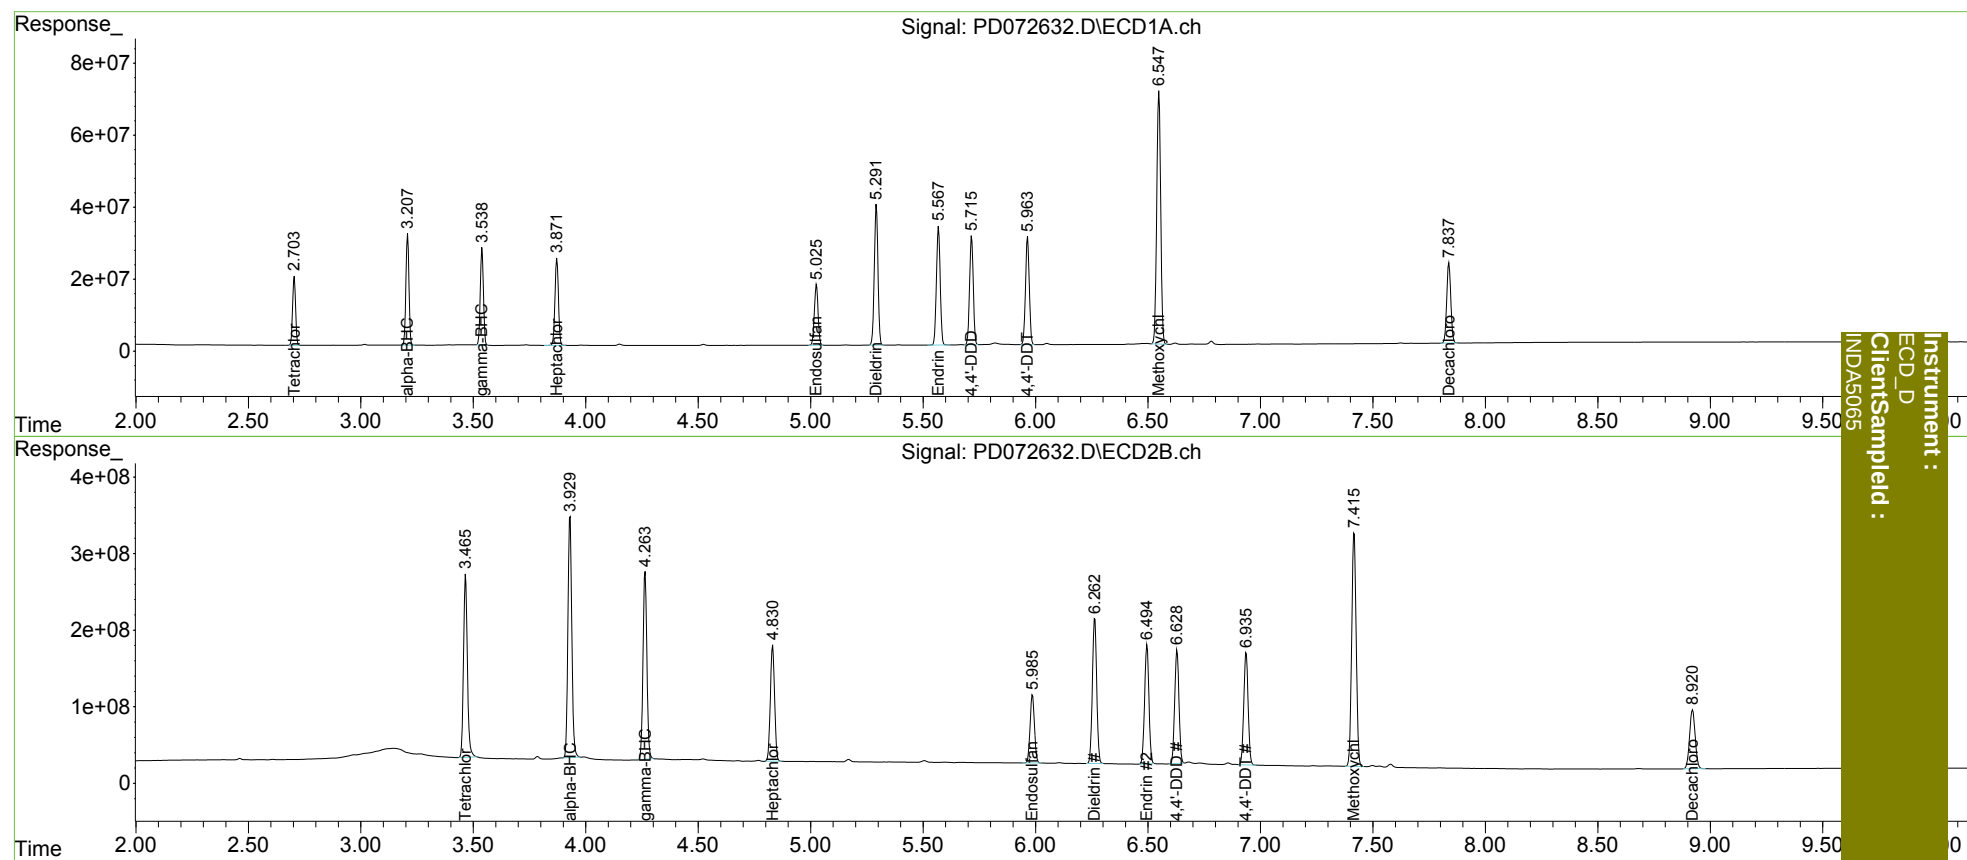

Instrument :
ECD_D
ClientSampled :
INDA5065