

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 10:49
 Operator : AR\AJ
 Sample : RESC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC043

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:57:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	45988823	793.6E6	19.781	19.803
27)	SA Decachlor...	7.838	8.922	79848215	387.3E6	40.678	41.186
Target Compounds							
2)	A alpha-BHC	3.209	3.930	32478065	550.5E6	9.301	10.378
3)	MA gamma-BHC...	3.540	4.264	29947908	441.8E6	9.449	10.395
4)	MA Heptachlor	3.872	4.831	31179943	318.6E6	9.609	10.715
5)	MB Aldrin	4.151	5.170	32679391	283.5E6	10.316	11.311
6)	B beta-BHC	3.842	4.480	15950803	187.9E6	10.499	11.076
7)	B delta-BHC	4.071	4.723	33470896	376.0E6	9.985	10.999
8)	B Heptachlo...	4.657	5.602	29122290	230.4E6	10.240	11.144
9)	A Endosulfan I	5.026	5.987	24765438	183.4E6	9.762	10.583
10)	B trans-Chl...	4.905	5.856	30365503	218.3E6	10.346	10.902
11)	B cis-Chlor...	4.969	5.931	29417891	210.8E6	10.304	10.815
12)	B 4,4'-DDE	5.157	6.105	54800363	387.5E6	20.132	21.702
13)	MA Dieldrin	5.292	6.264	52484041	370.4E6	19.048	20.786
14)	MA Endrin	5.570	6.496	46833321	309.3E6	19.324	21.143
15)	B Endosulfa...	5.868	6.726	49300066	312.4E6	20.962	21.867
16)	A 4,4'-DDD	5.716	6.630	40820862	273.5E6	19.171	20.262
17)	MA 4,4'-DDT	5.965	6.937	41117558	279.3E6	18.978	20.664
18)	B Endrin al...	6.050	6.857	41610283	259.6E6	21.133	21.666
19)	B Endosulfa...	6.273	7.090	47467507	284.6E6	20.738	21.620
20)	A Methoxychlor	6.549	7.417	116.0E6	625.8E6	99.903	103.451
21)	B Endrin ke...	6.784	7.579	56613339	314.0E6	21.225	21.924

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

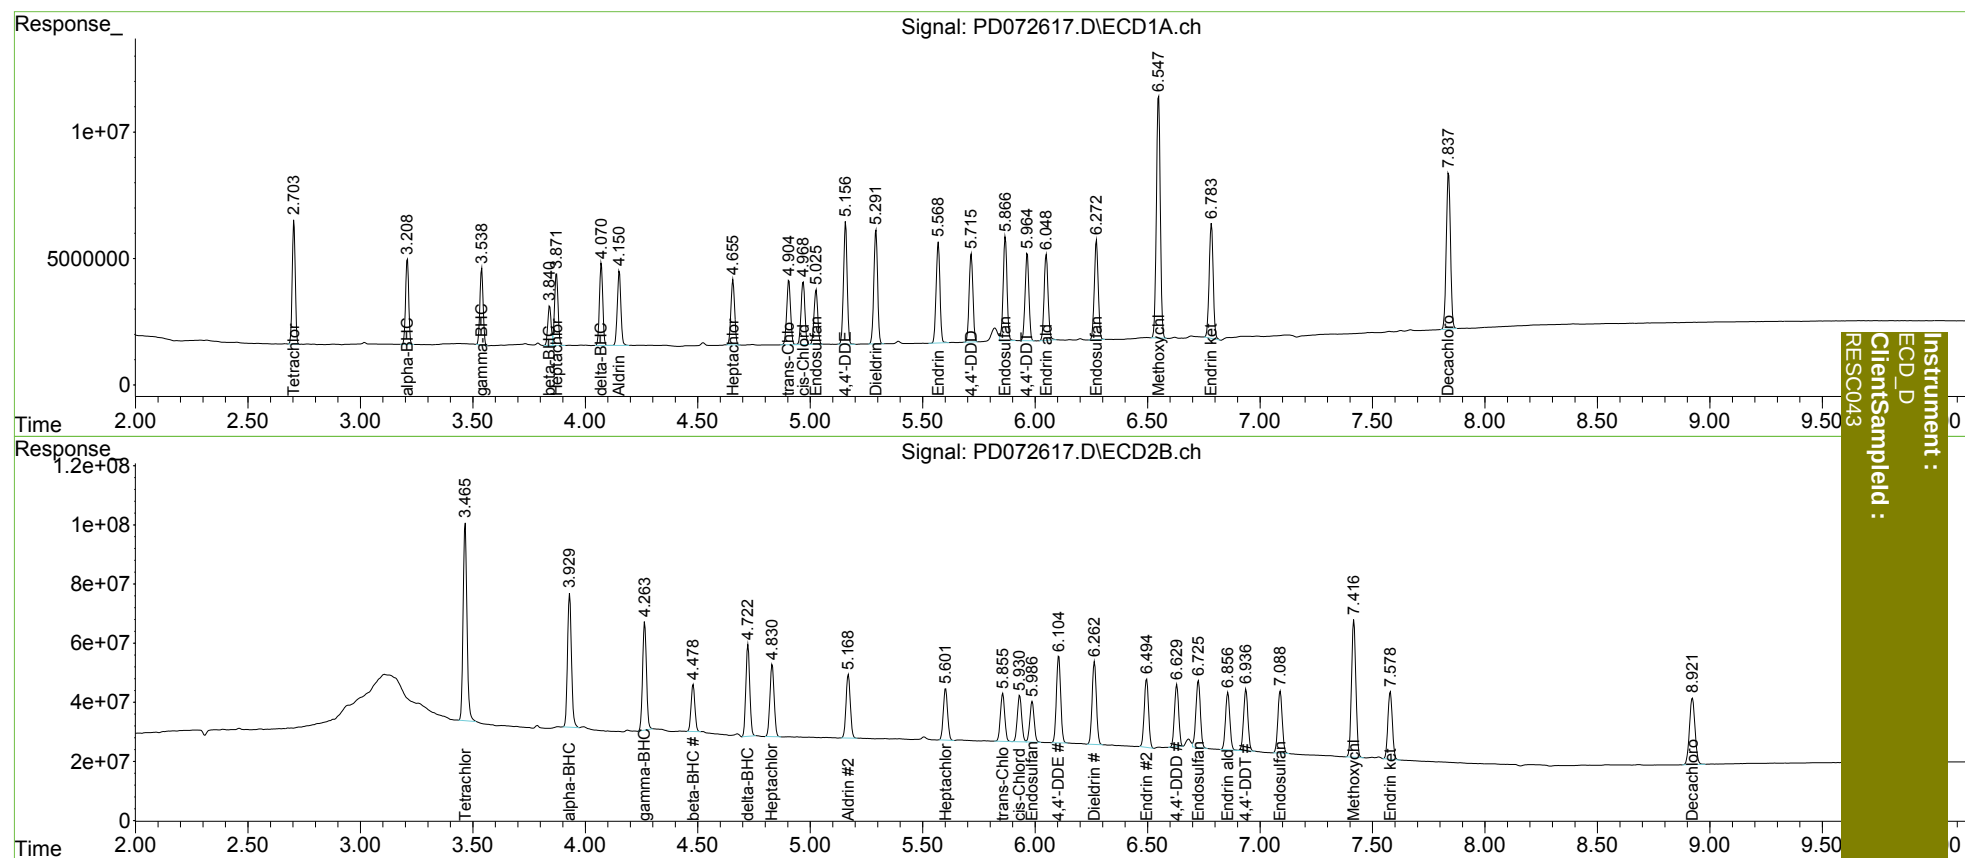

Instrument :
ECD_D
Client Sampled :
RESC043

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Title : GC Extractables
Last Update : Wed Oct 26 16:50:44 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
2.705	3.209	100.00%
3.209	3.540	100.00%
3.540	3.842	100.00%
3.842	3.872	73.52%
3.872	4.071	100.00%
4.071	4.151	100.00%
4.151	4.657	100.00%
4.657	4.905	100.00%
4.905	4.969	99.90%
4.969	5.026	100.00%
5.026	5.158	100.00%
5.158	5.292	100.00%
5.292	5.570	100.00%
5.570	5.716	100.00%
5.716	5.868	100.00%
5.868	5.965	99.77%
5.965	6.050	100.00%
6.050	6.273	100.00%
6.273	6.549	100.00%
6.549	6.784	100.00%
6.784	7.838	100.00%

Signal #2


3.466	3.930	100.00%
3.930	4.264	100.00%
4.264	4.480	100.00%
4.480	4.723	100.00%
4.723	4.831	100.00%
4.831	5.170	100.00%
5.170	5.602	100.00%
5.602	5.856	100.00%
5.856	5.931	98.95%
5.931	5.987	96.53%
5.987	6.105	100.00%
6.105	6.264	99.40%
6.264	6.496	100.00%
6.496	6.630	100.00%
6.630	6.726	100.00%
6.726	6.857	98.07%
6.857	6.937	99.32%
6.937	7.090	99.58%
7.090	7.417	100.00%
7.417	7.579	100.00%
7.579	8.923	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

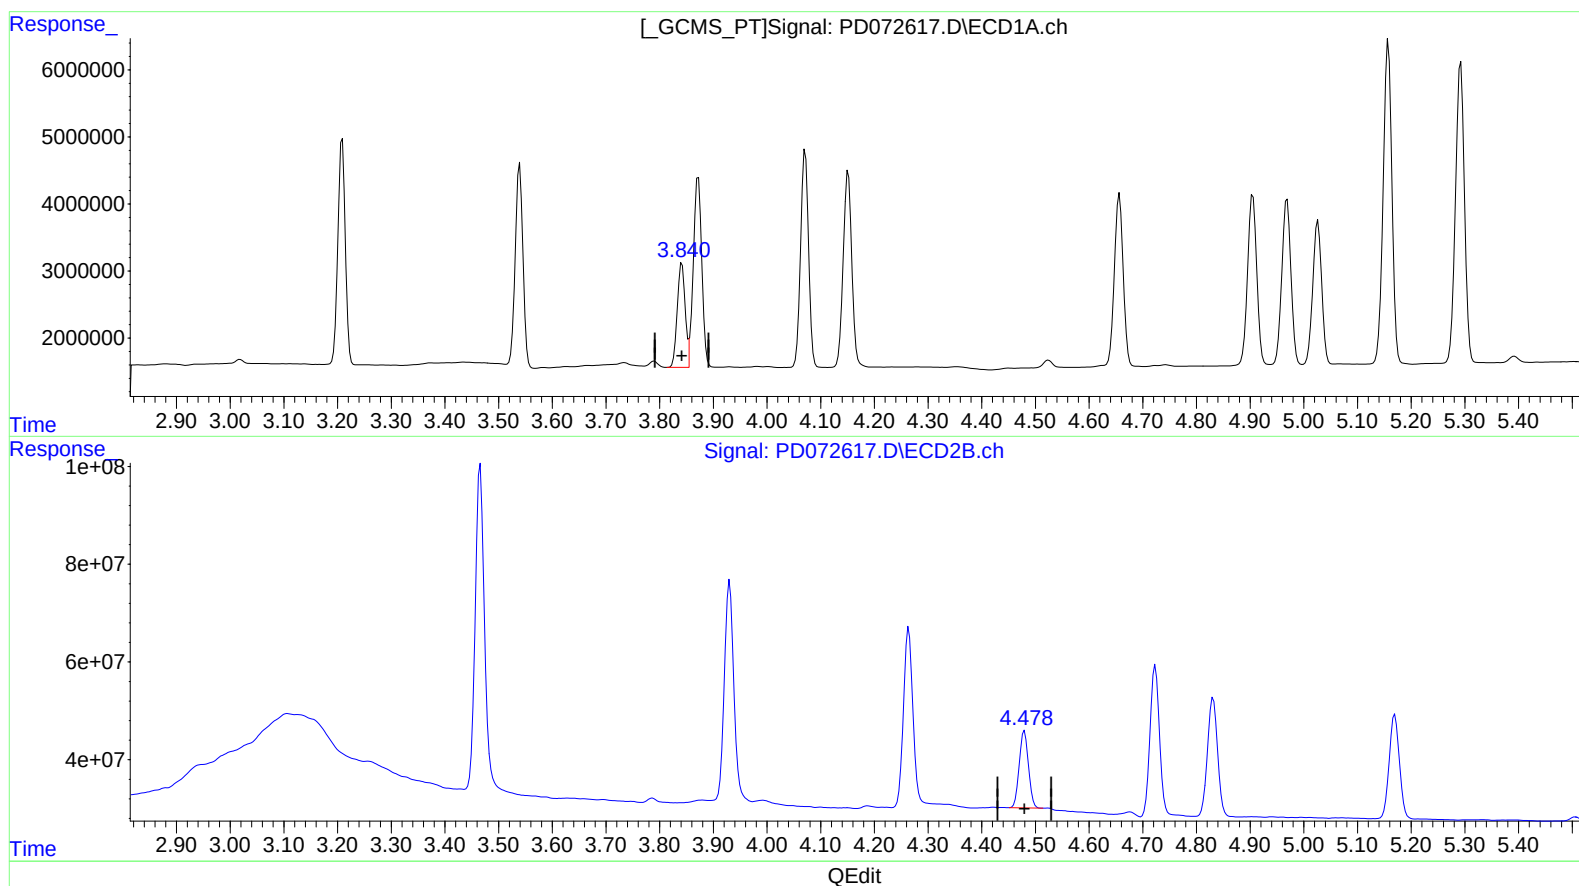

(6) beta-BHC (B)

3.842min 10.499 ng/ml

response 15950803

(6) beta-BHC #2 (B)

4.480min 11.076 ng/ml


response 187905017

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

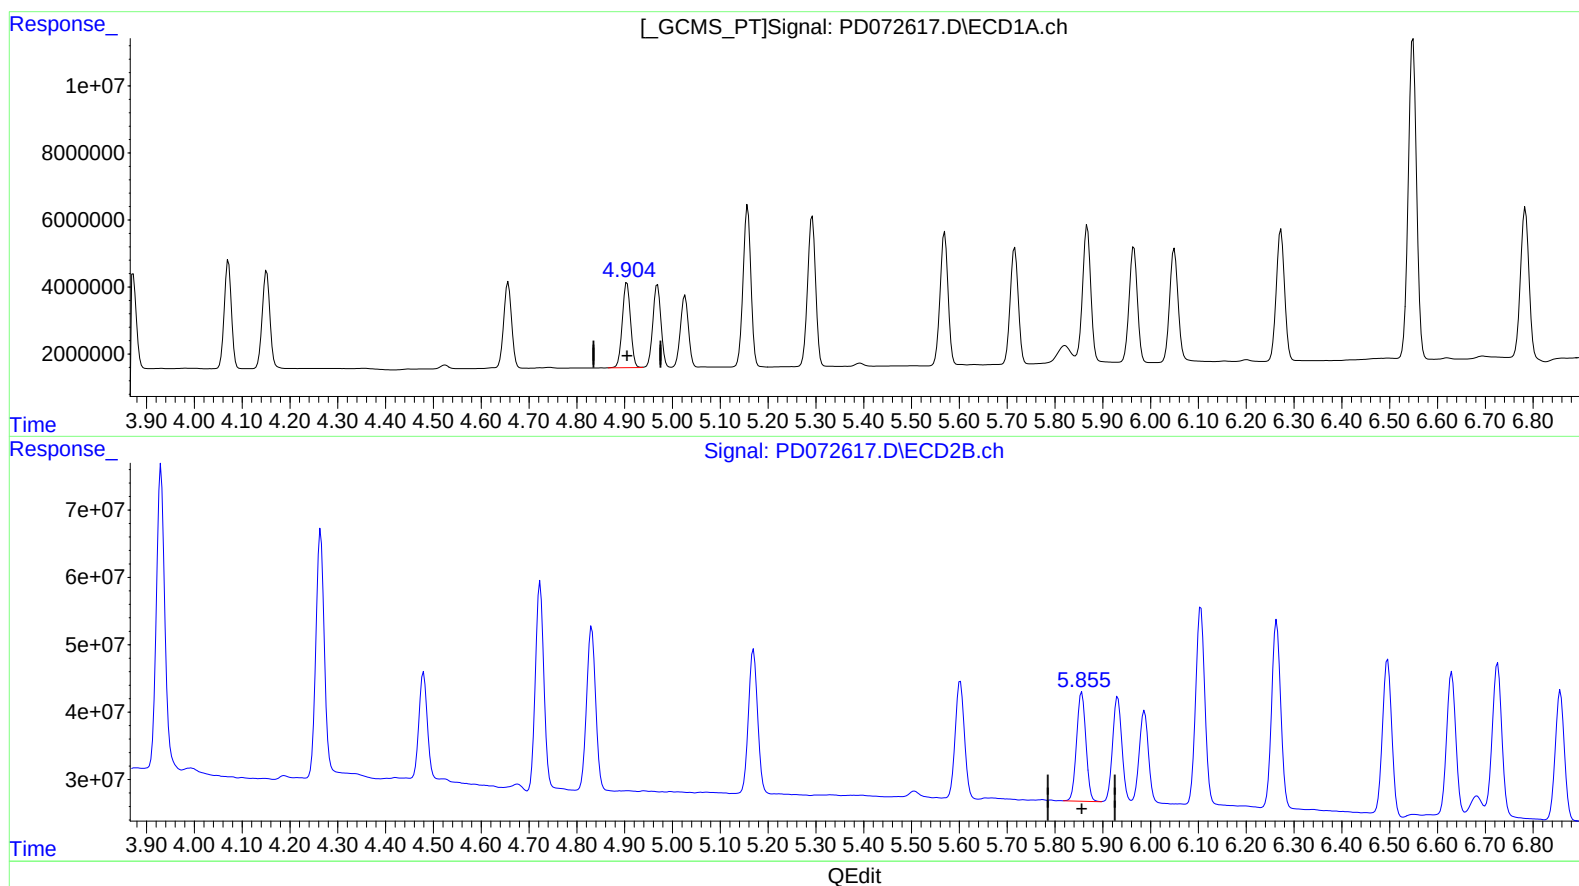

(10) trans-Chlordane (B)

4.905min 10.346 ng/ml

response 30365503

(10) trans-Chlordane #2 (B)

5.856min 10.902 ng/ml


response 218345954

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

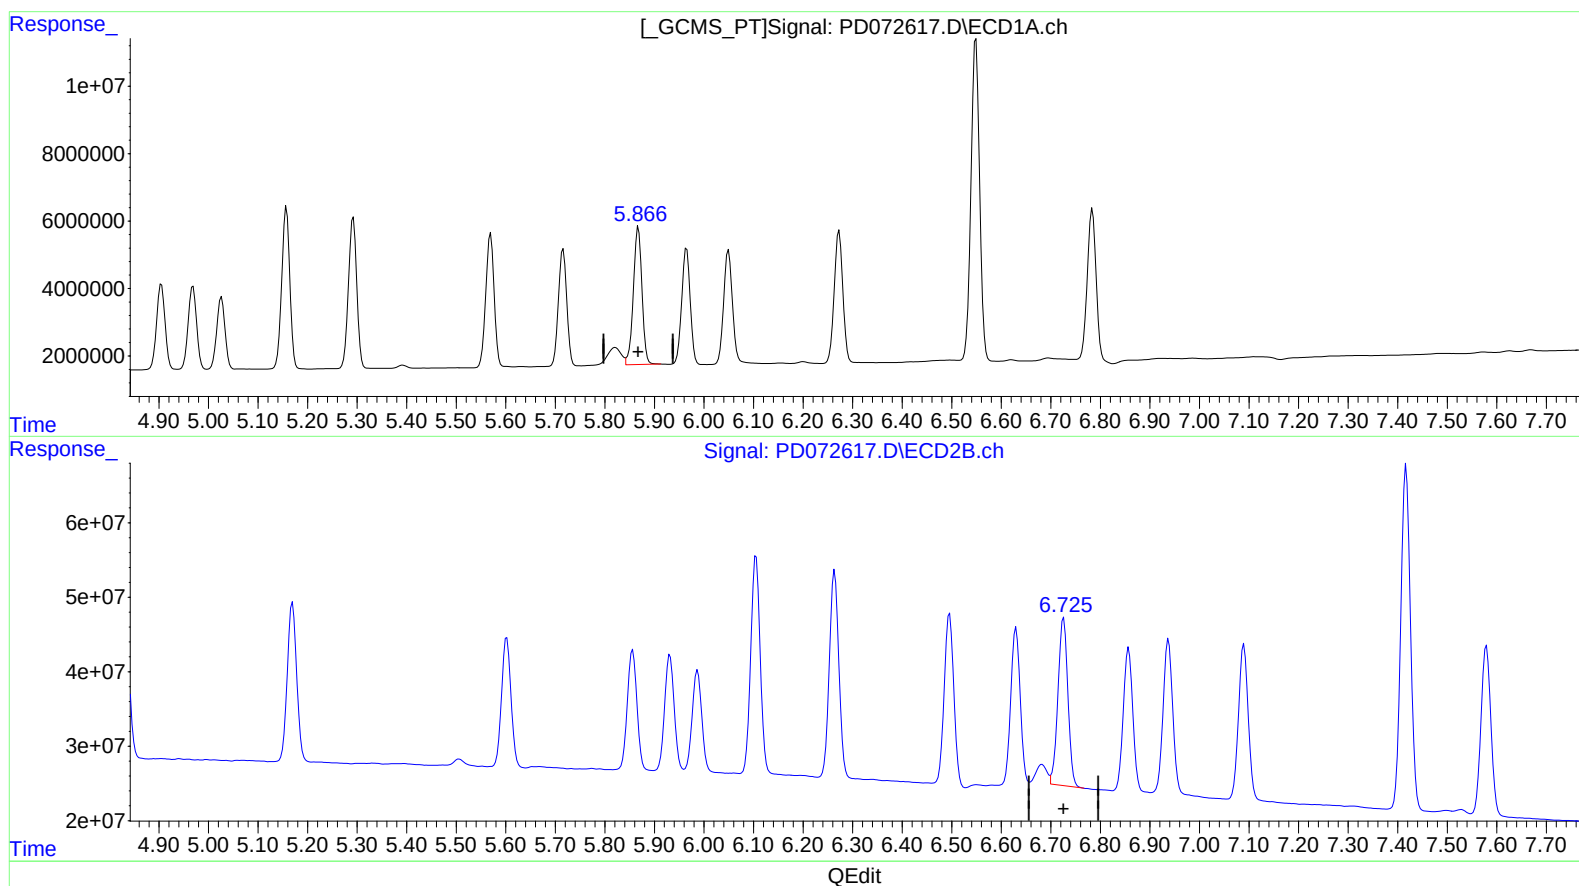

(15) Endosulfan II (B)
5.868min 20.962 ng/ml
response 49300066


(15) Endosulfan II #2 (B)
6.726min 21.867 ng/ml
response 312369754

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

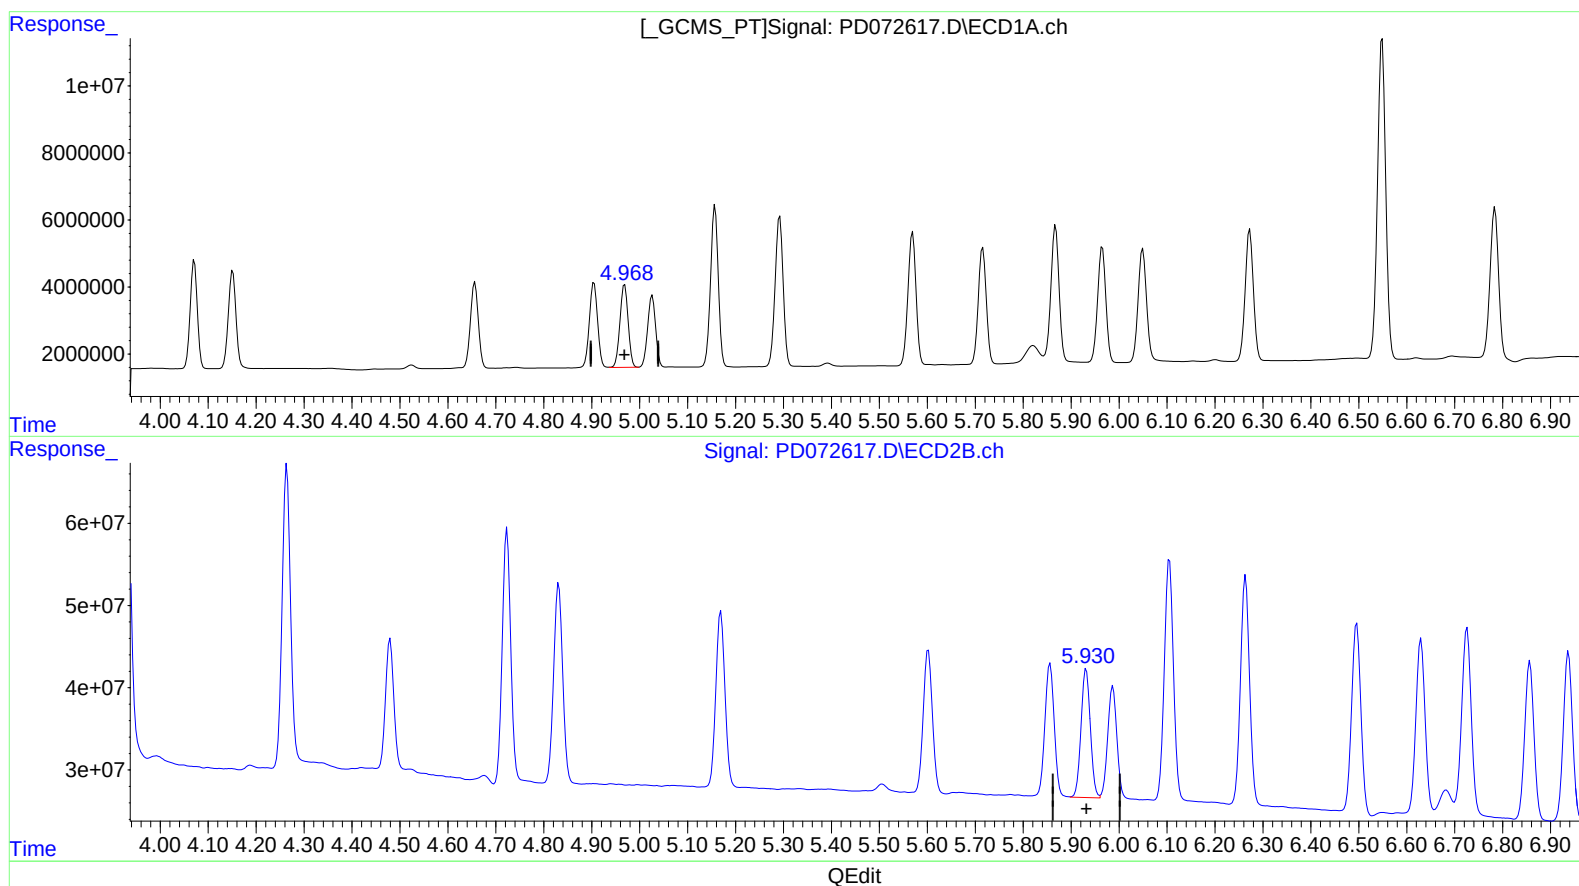

(11) cis-Chlordane (B)

4.969min 10.304 ng/ml

response 29417891

(11) cis-Chlordane #2 (B)

5.931min 10.815 ng/ml


response 210774139

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

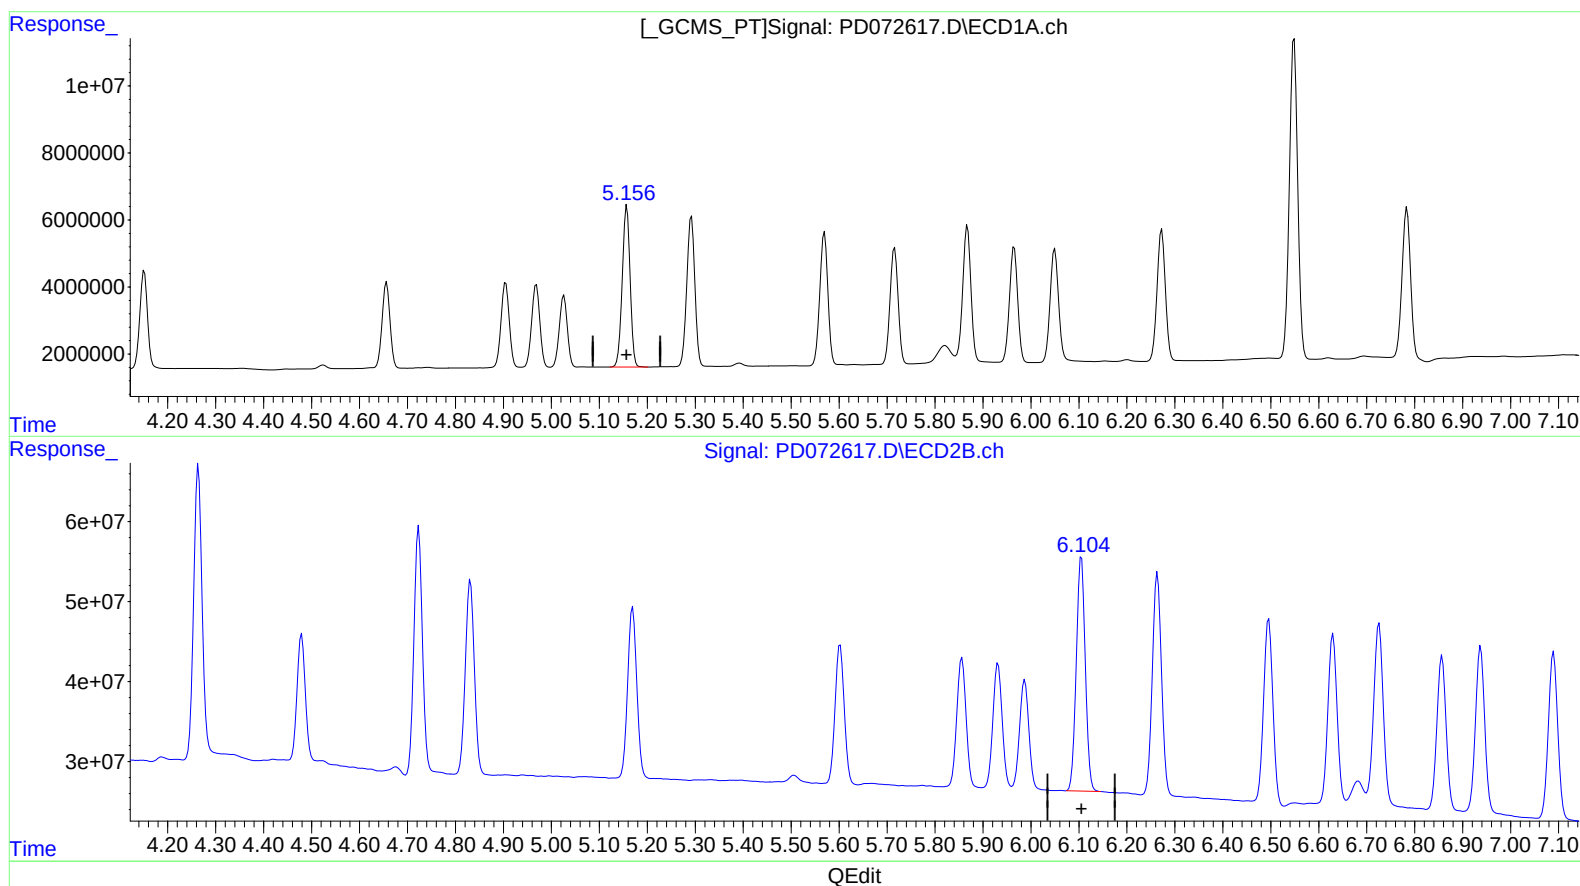

(12) 4,4'-DDE (B)

5.157min 20.132 ng/ml

response 54800363

(12) 4,4'-DDE #2 (B)

6.105min 21.702 ng/ml


response 387530772

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

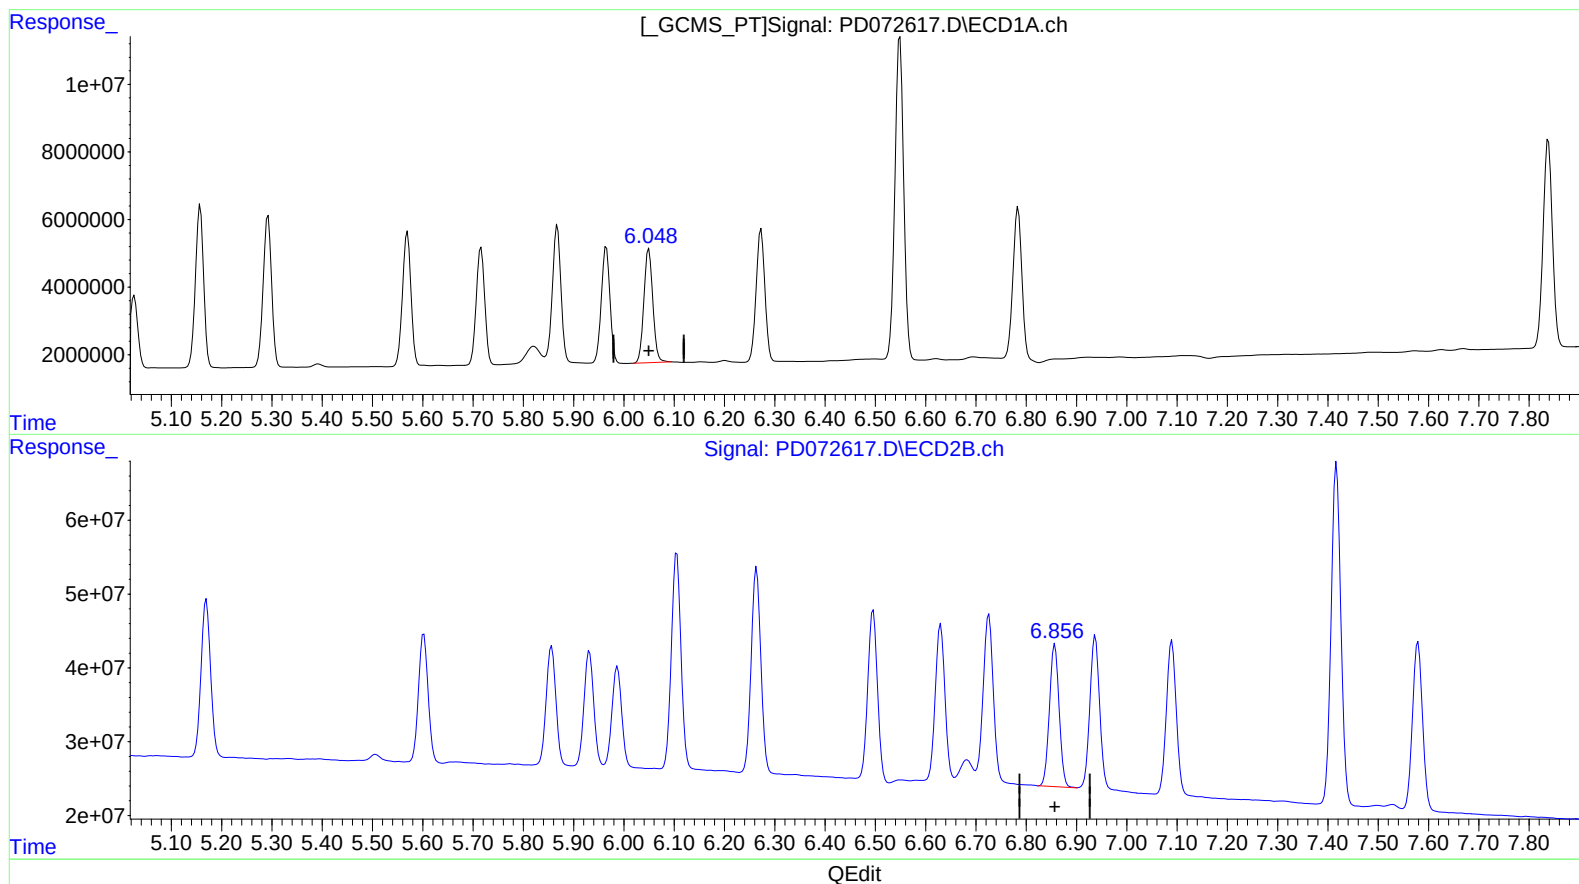

(18) Endrin aldehyde (B)

6.050min 21.133 ng/ml

response 41610283

(18) Endrin aldehyde #2 (B)

6.857min 21.666 ng/ml


response 259620464

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 10:49
Operator : AR\AJ
Sample : RESC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC043

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:57:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

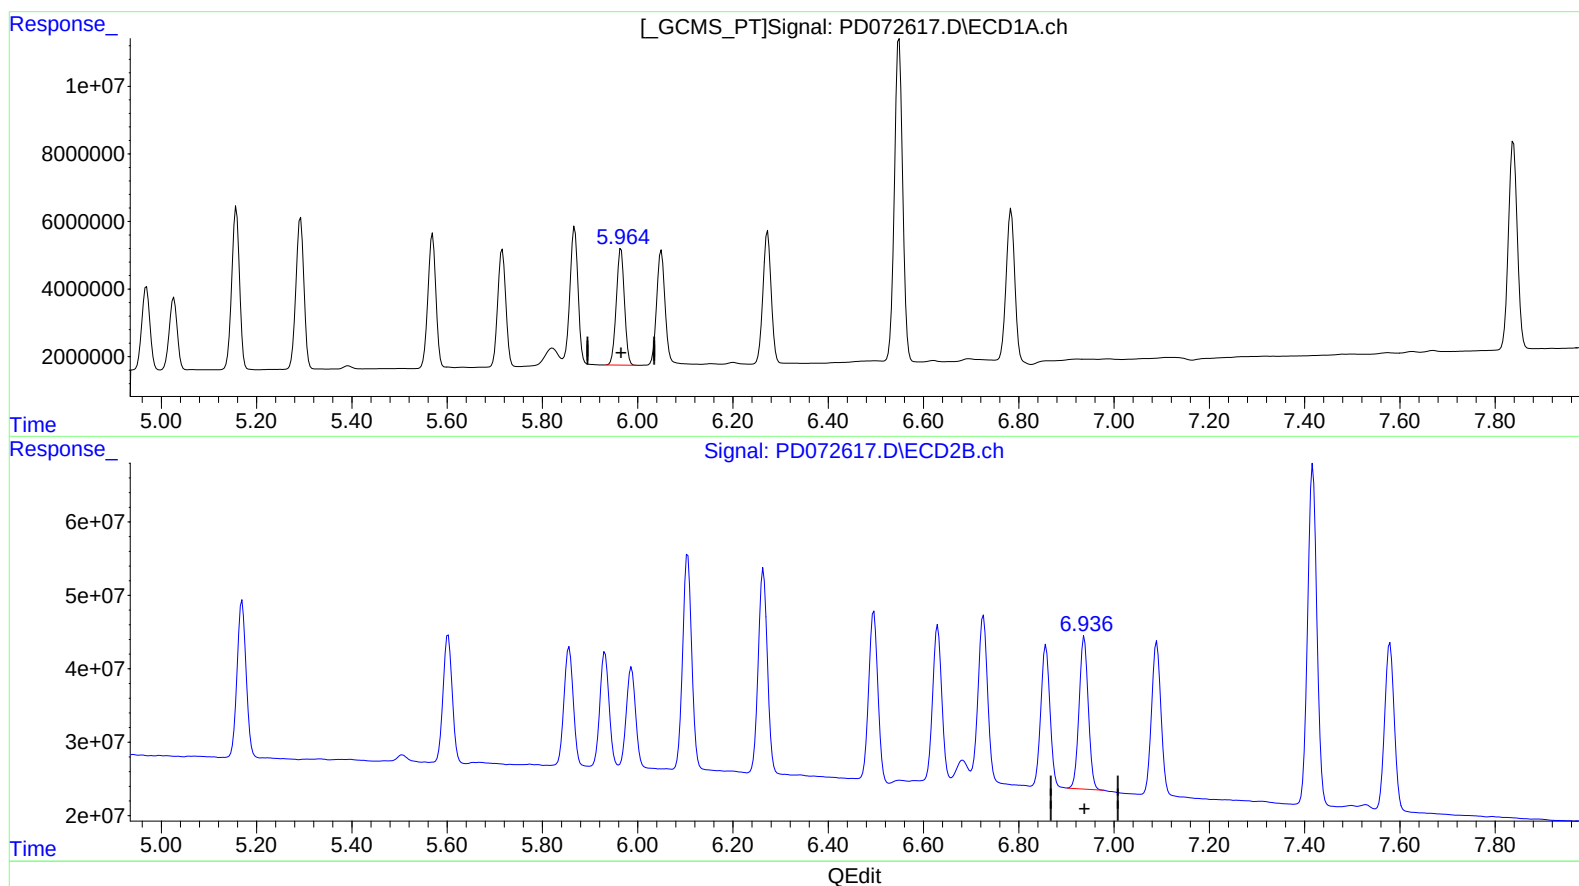

(17) 4,4'-DDT (MA)

5.965min 18.978 ng/ml

response 41117558

(17) 4,4'-DDT #2 (MA)

6.937min 20.664 ng/ml

response 279305389