

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 13:42
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4063

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 16:12:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:11:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.466	90658657	1522.4E6	39.954	38.691
27)	SA Decachlor...	7.838	8.921	148.4E6	722.8E6	77.334	77.989
Target Compounds							
2)	A alpha-BHC	3.208	3.930	144.3E6	2004.0E6	42.282	38.708
3)	MA gamma-BHC...	3.539	4.264	129.7E6	1582.5E6	41.836	38.040
4)	MA Heptachlor	3.872	4.831	129.9E6	1094.0E6	41.113	37.625
9)	A Endosulfan I	5.026	5.987	99463917	655.2E6	40.292	38.434
13)	MA Dieldrin	5.292	6.264	224.1E6	1362.1E6	83.115	77.610
14)	MA Endrin	5.569	6.496	197.3E6	1111.8E6	82.695	77.162
16)	A 4,4'-DDD	5.716	6.630	172.6E6	1047.6E6	82.516	78.679
17)	MA 4,4'-DDT	5.965	6.937	177.4E6	1050.0E6	83.458	78.702
20)	A Methoxychlor	6.549	7.416	454.5E6	2315.7E6	396.578	387.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 13:42
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 16:12:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:11:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

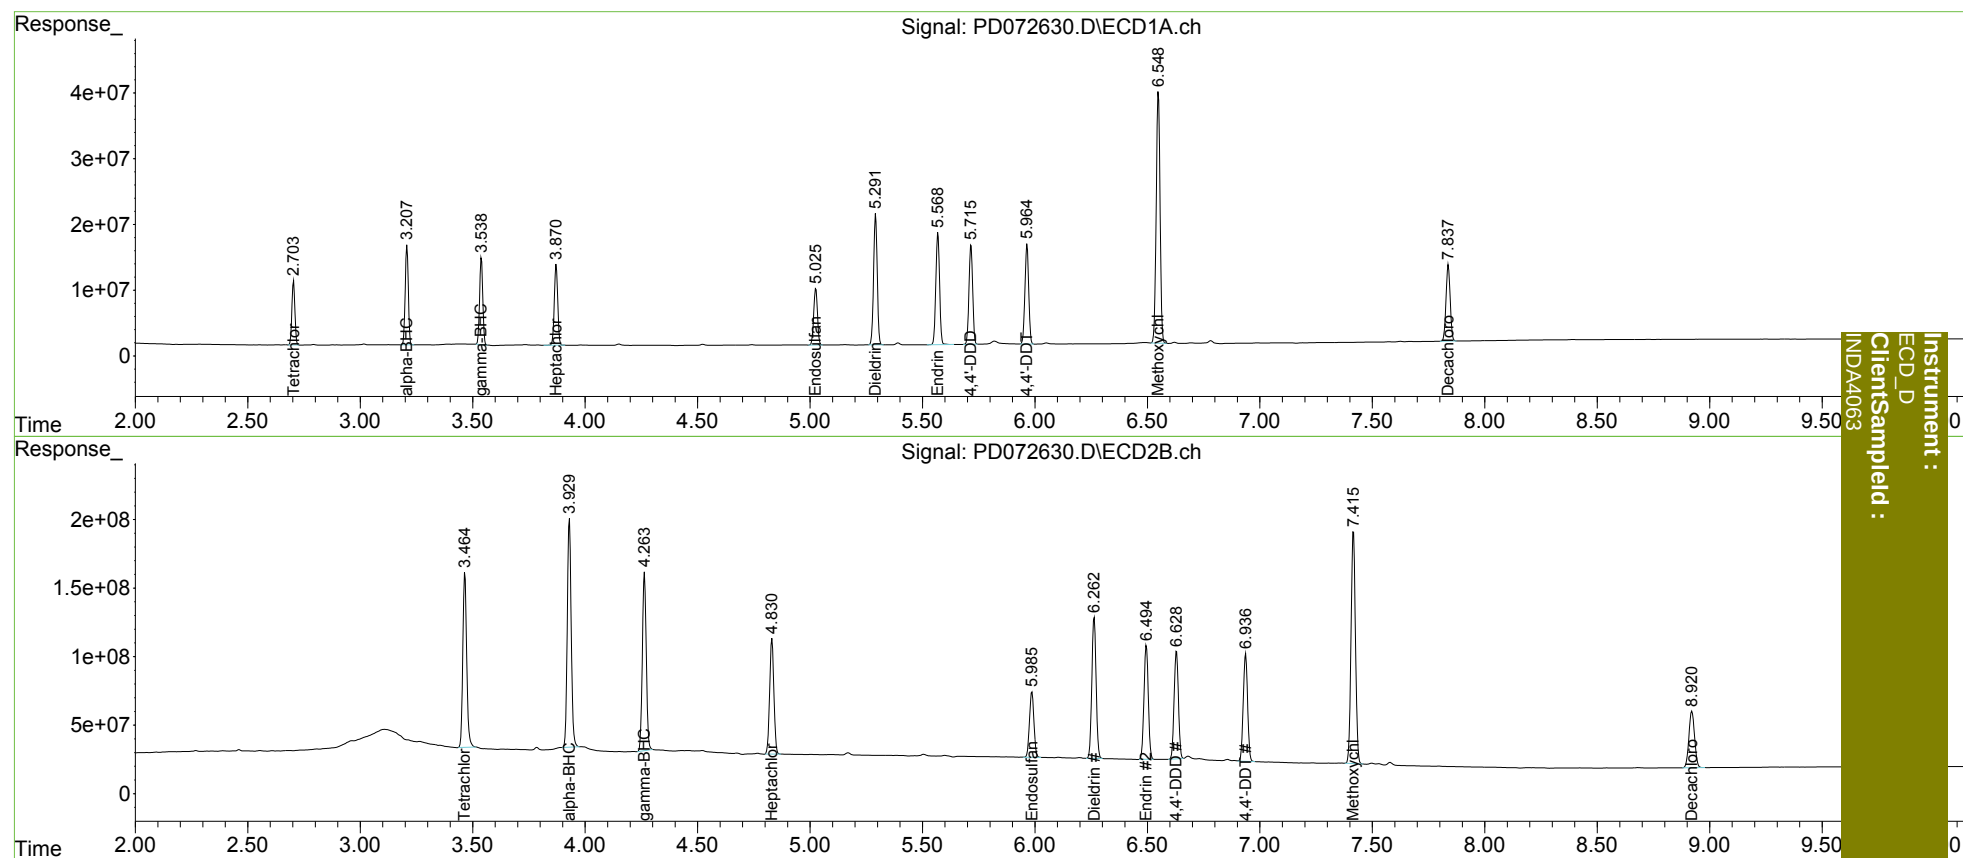

Instrument :
ECD_D
ClientSampled :
INDA4063