

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
 Data File : PD072639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2022 18:05
 Operator : AR\AJ
 Sample : INDA366
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3202

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 05:30:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.705	3.466	45234306	819.9E6	19.456	20.461
27)	SA Decachlor...	7.840	8.922	76120429	374.0E6	38.779	39.774
Target Compounds							
2)	A alpha-BHC	3.209	3.930	67866322	1054.8E6	19.436	19.884
3)	MA gamma-BHC...	3.540	4.264	61744524	843.9E6	19.481	19.858
4)	MA Heptachlor	3.872	4.831	62499498	590.3E6	19.261	19.852
9)	A Endosulfan I	5.027	5.987	48912671	343.9E6	19.281	19.850
13)	MA Dieldrin	5.293	6.264	107.1E6	705.9E6	38.854	39.614
14)	MA Endrin	5.570	6.496	93463392	578.7E6	38.565	39.561
16)	A 4,4'-DDD	5.717	6.630	82711187	538.0E6	38.844	39.865
17)	MA 4,4'-DDT	5.966	6.937	83723051	532.8E6	38.644	39.418
20)	A Methoxychlor	6.550	7.417	225.4E6	1196.6E6	194.148	197.826

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102622\
Data File : PD072639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2022 18:05
Operator : AR\AJ
Sample : INDA366
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 05:30:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

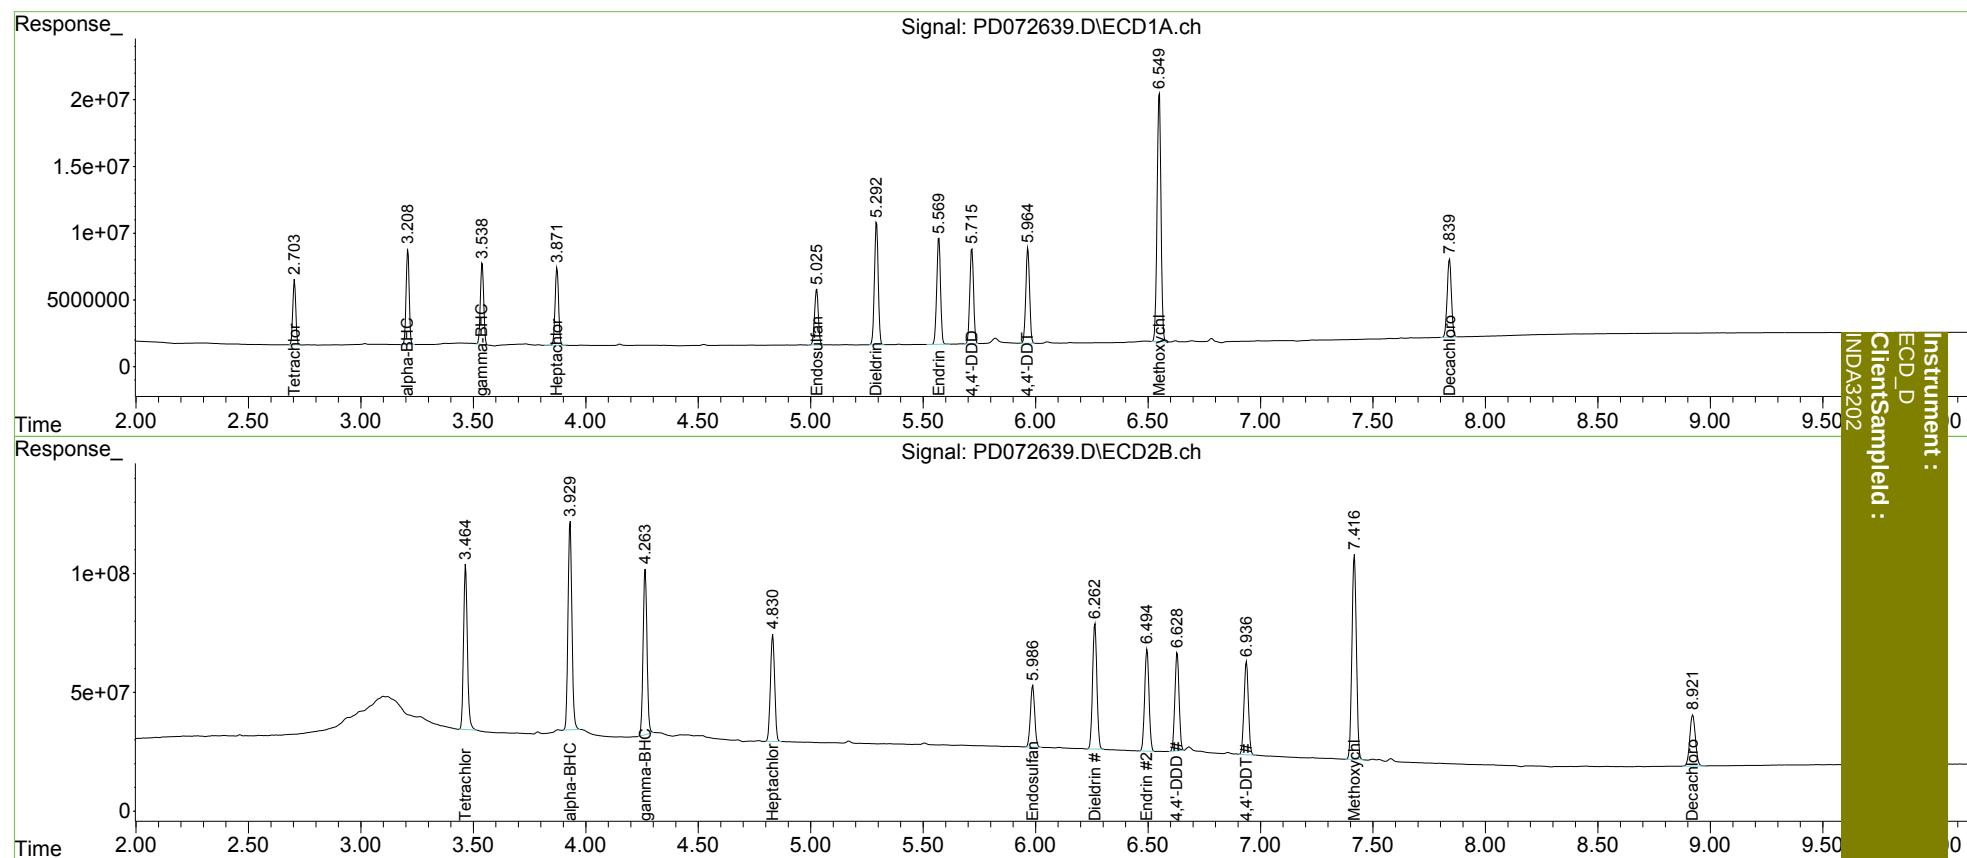

Instrument :
ECD_D
ClientSampled :
INDA3202