

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102623\
 Data File : PD079178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2023 16:01
 Operator : AR\AJ
 Sample : PB156664BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 22:52:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	27151036	40184122	16.816	17.356
28)	SA Decachlor...	9.116	7.955	34917997	45614909	17.407	18.714
Target Compounds							
2)	A alpha-BHC	4.024	3.299	225838	108694	0.085	0.031 #
3)	MA gamma-BHC...	0.000	3.657f	0	259628	N.D.	0.076 #
7)	B delta-BHC	4.798	0.000	947589	0	0.354	N.D. #
13)	MA Dieldrin	6.392	0.000	261612	0	0.112	N.D. #
15)	B Endosulfa...	6.853f	0.000	69004	0	0.034	N.D. #
17)	MA 4,4'-DDT	7.042f	0.000	150130	0	0.079	N.D. #
18)	B Endrin al...	0.000	6.120f	0	147581	N.D.	0.079 #
19)	B Endosulfa...	0.000	6.400f	0	114950	N.D.	0.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102623\
Data File : PD079178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2023 16:01
Operator : AR\AJ
Sample : PB156664BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 22:52:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

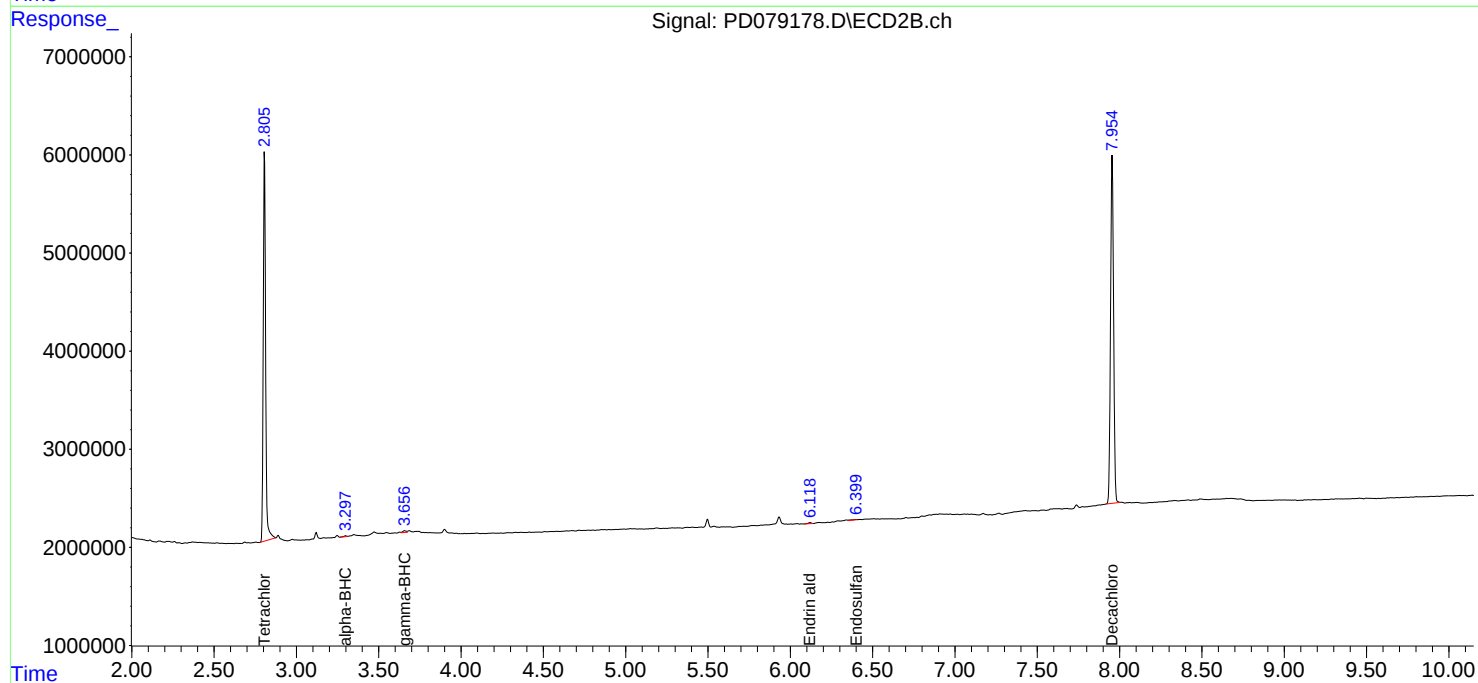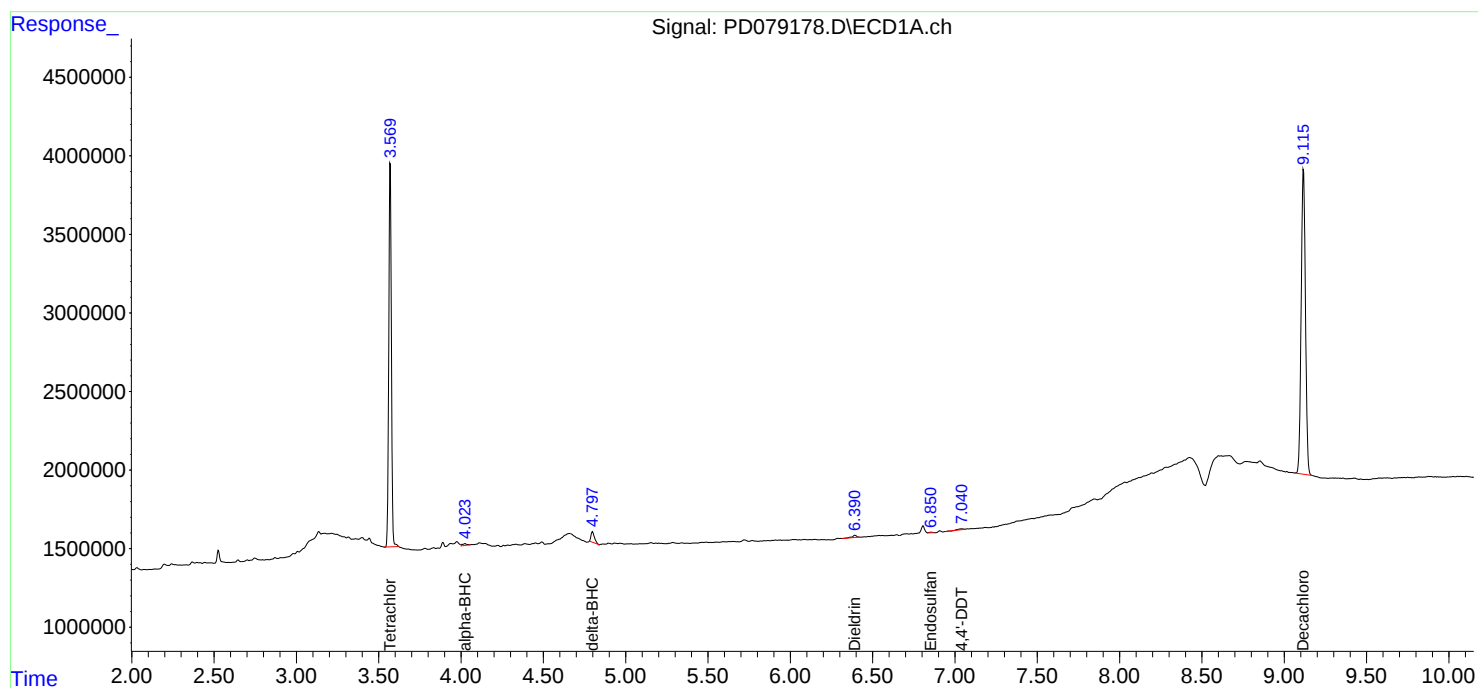


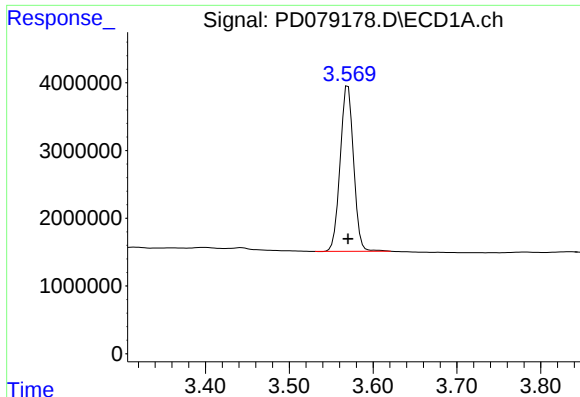

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 27151036
Conc: 16.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

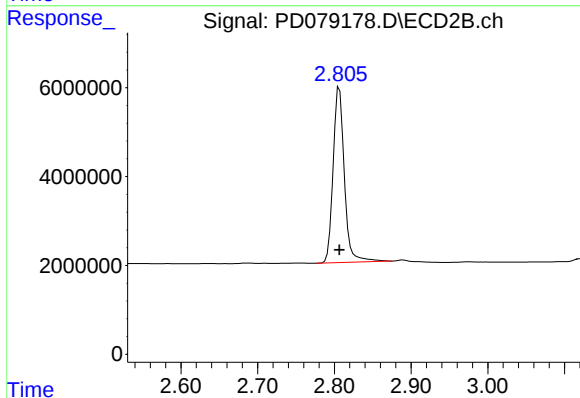


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 40184122
Conc: 17.36 ng/ml

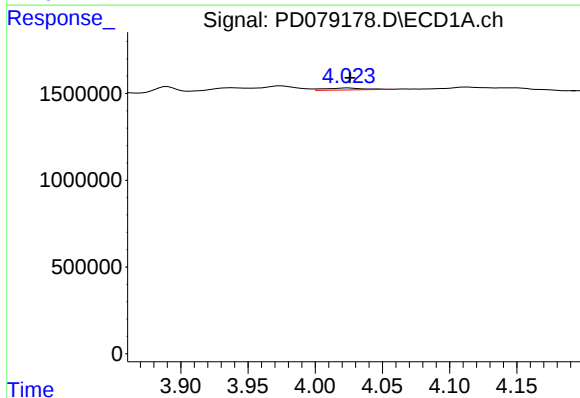


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: -0.002 min
Response: 225838
Conc: 0.08 ng/ml

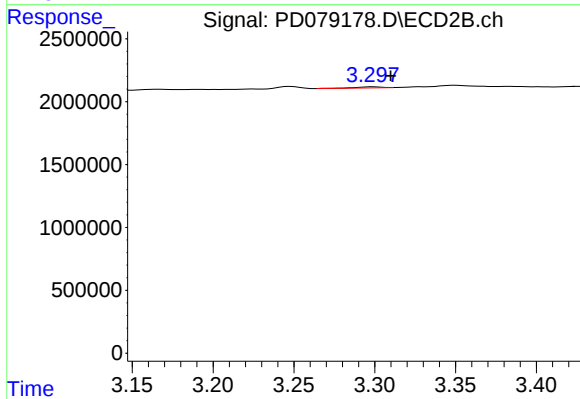

#2 alpha-BHC


R.T.: 3.299 min
Delta R.T.: -0.011 min
Response: 108694
Conc: 0.03 ng/ml

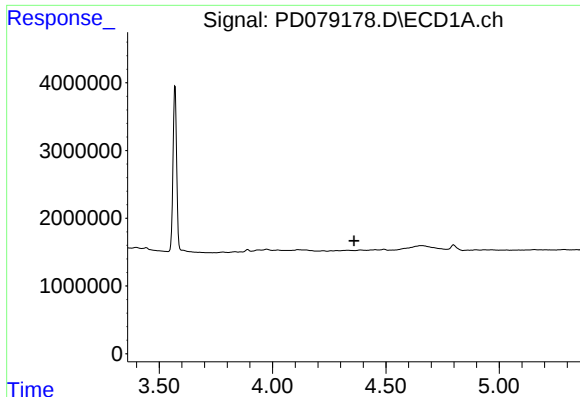

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.359 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

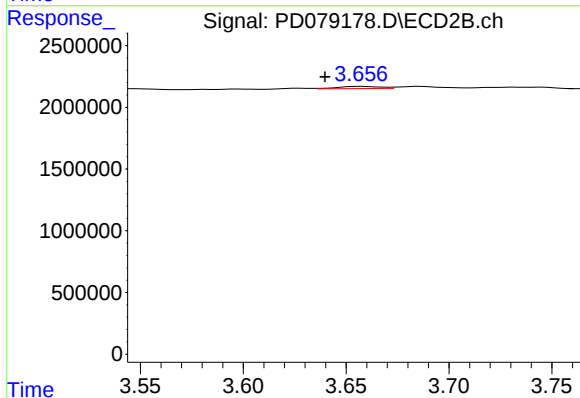


#3 gamma-BHC (Lindane)

R.T.: 3.657 min
Delta R.T.: 0.018 min
Response: 259628
Conc: 0.08 ng/ml

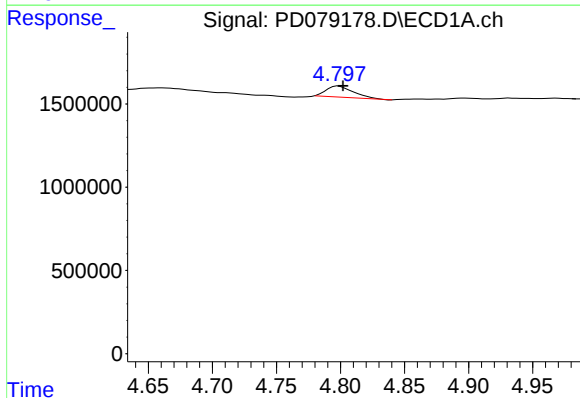


#7 delta-BHC

R.T.: 4.798 min
Delta R.T.: -0.004 min
Response: 947589
Conc: 0.35 ng/ml

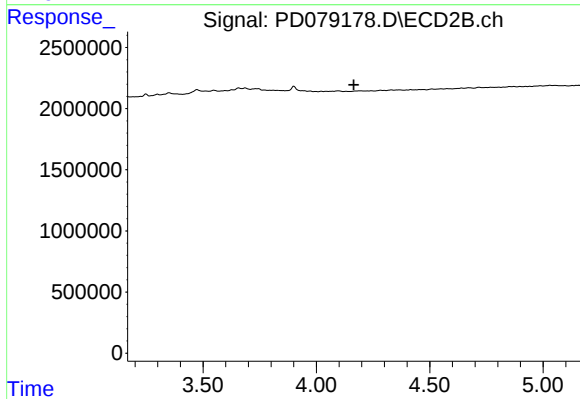

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.165 min
Response: 0
Conc: N.D.

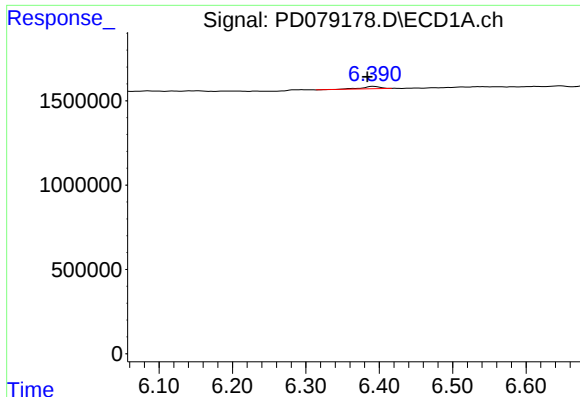

#13 Dieldrin


R.T.: 6.392 min
Delta R.T.: 0.008 min
Response: 261612
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

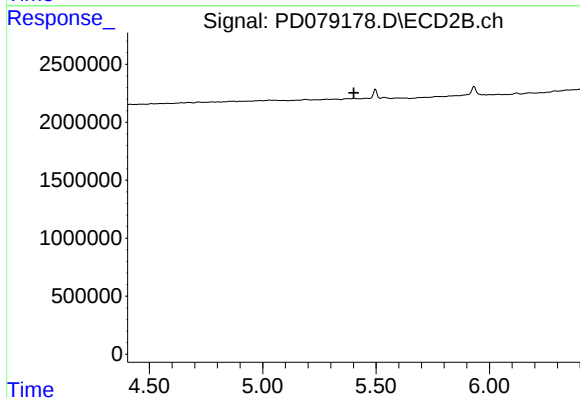


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.401 min
Response: 0
Conc: N.D.

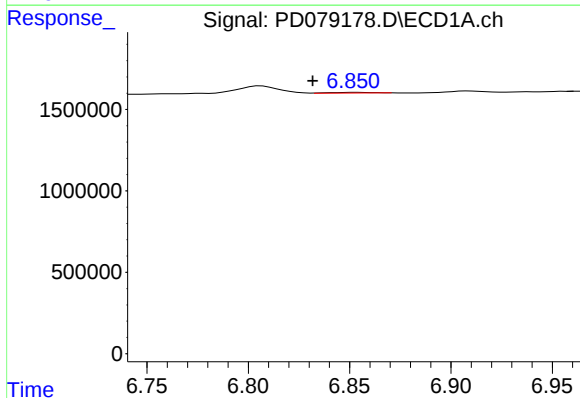


#15 Endosulfan II

R.T.: 6.853 min
Delta R.T.: 0.021 min
Response: 69004
Conc: 0.03 ng/ml

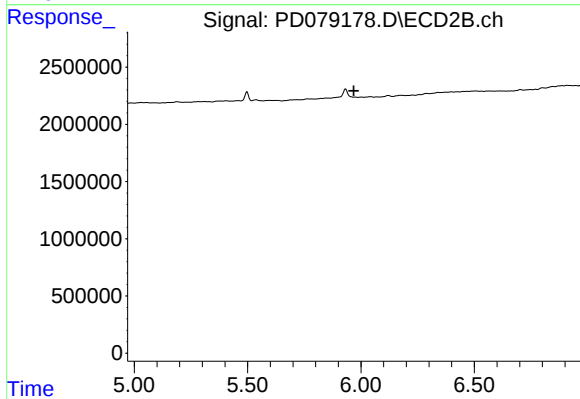

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.968 min
Response: 0
Conc: N.D.

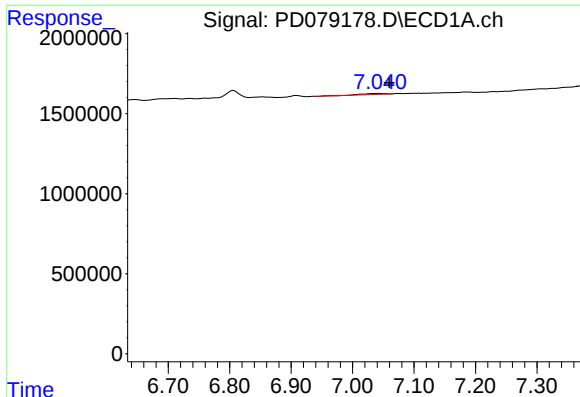

#17 4,4'-DDT


R.T.: 7.042 min
Delta R.T.: -0.018 min
Response: 150130
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

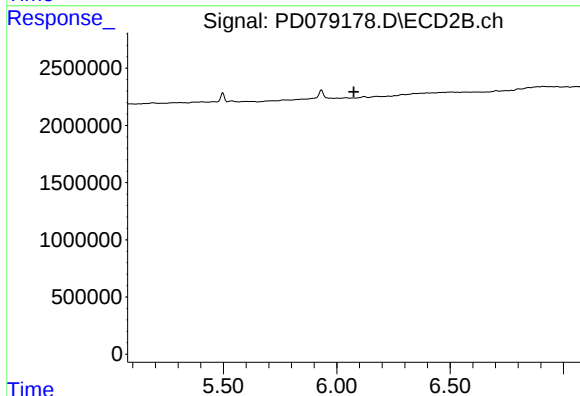


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

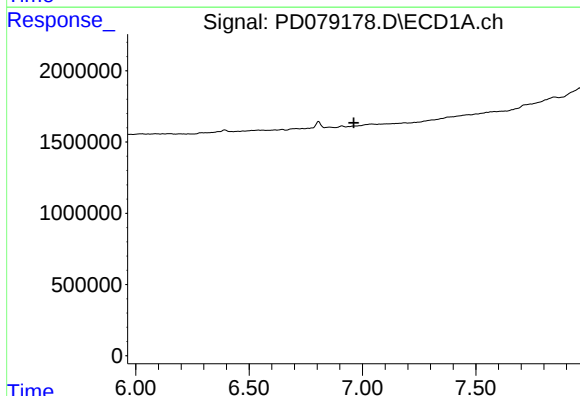


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

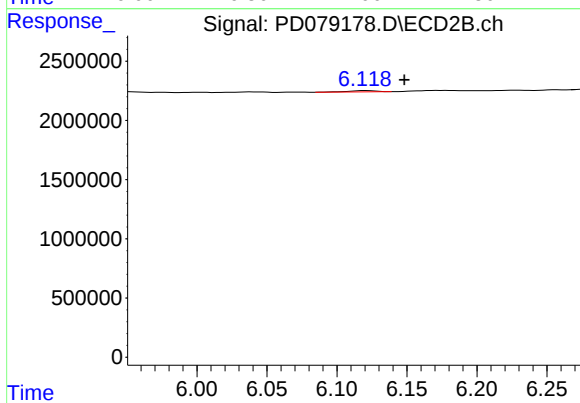

#18 Endrin aldehyde


R.T.: 6.120 min
Delta R.T.: -0.028 min
Response: 147581
Conc: 0.08 ng/ml

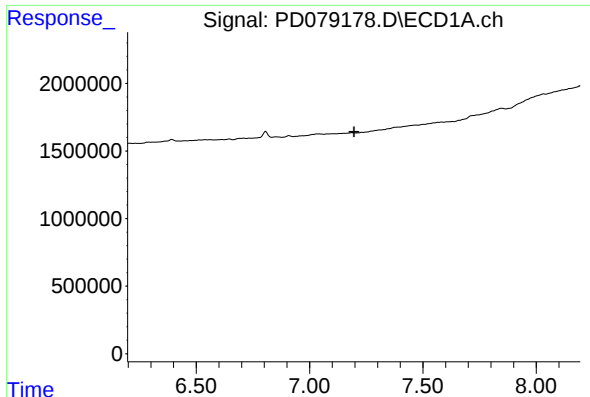

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.196 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

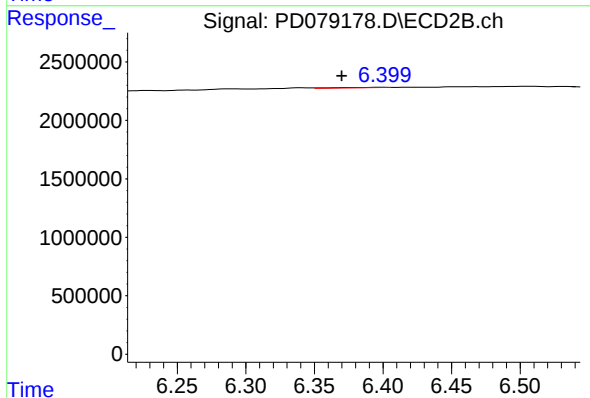


#19 Endosulfan Sulfate

R.T.: 6.400 min
Delta R.T.: 0.030 min
Response: 114950
Conc: 0.05 ng/ml

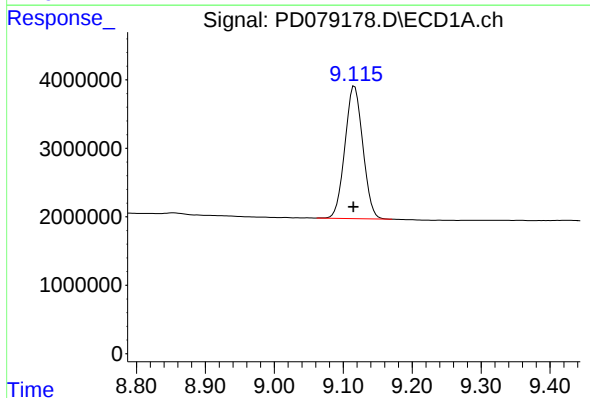

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.002 min
Response: 34917997
Conc: 17.41 ng/ml

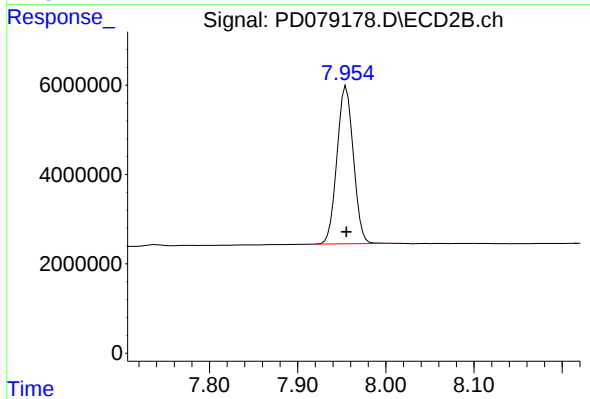

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 45614909
Conc: 18.71 ng/ml