

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102623\
 Data File : PD079176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2023 14:12
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 22:52:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.576	2.806	74157130	129.6E6	45.930	55.994
28)	SA Decachlor...	9.122	7.956	87046061	118.4E6	43.392	48.572
Target Compounds							
23)	Chlordane-1	4.744	3.809	38979496	43663745	501.355	502.720
24)	Chlordane-2	5.274	4.386	36651716	45306422	459.134	498.646
25)	Chlordane-3	5.985	5.017	153.6E6	139.0E6	495.512	521.219
26)	Chlordane-4	6.068	5.081	183.9E6	125.6E6	494.892	511.903
27)	Chlordane-5	6.918	5.976	33534638	52250778	477.257	524.269



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102623\
Data File : PD079176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2023 14:12
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 22:52:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

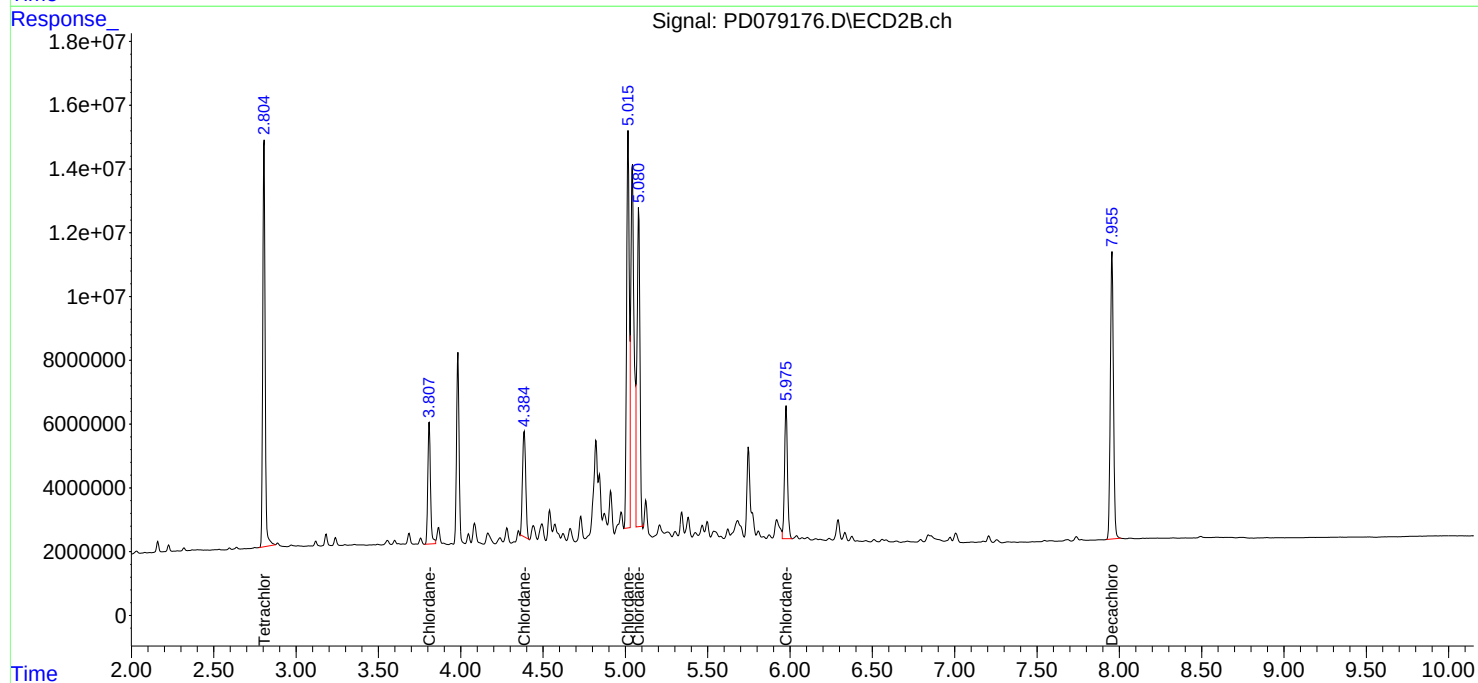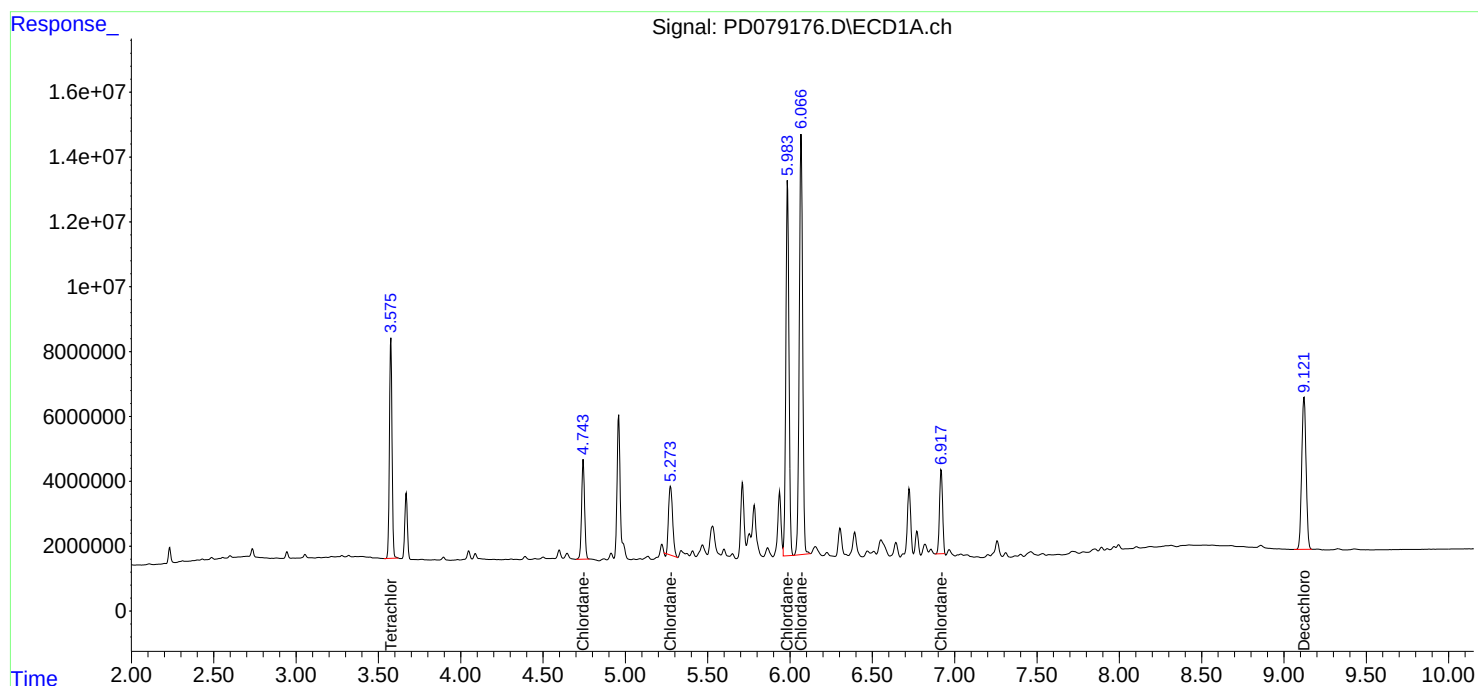


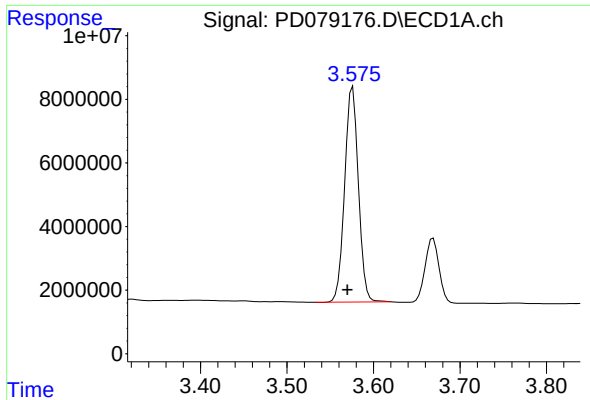

#1 Tetrachloro-m-xylene


R.T.: 3.576 min
Delta R.T.: 0.006 min
Response: 74157130
Conc: 45.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

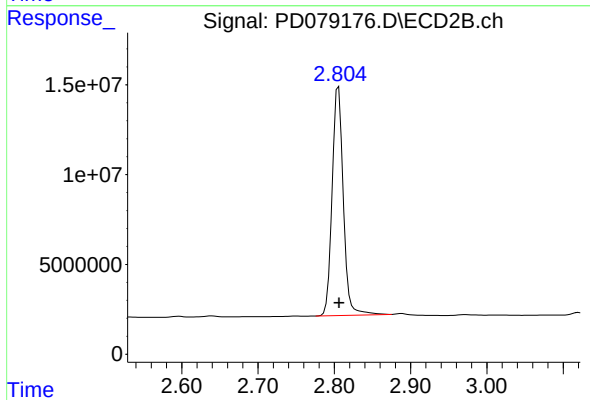


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 129641325
Conc: 55.99 ng/ml

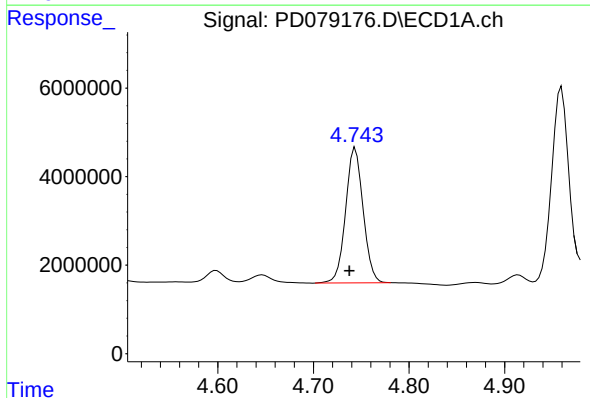


#23 Chlordane-1

R.T.: 4.744 min
Delta R.T.: 0.006 min
Response: 38979496
Conc: 501.35 ng/ml

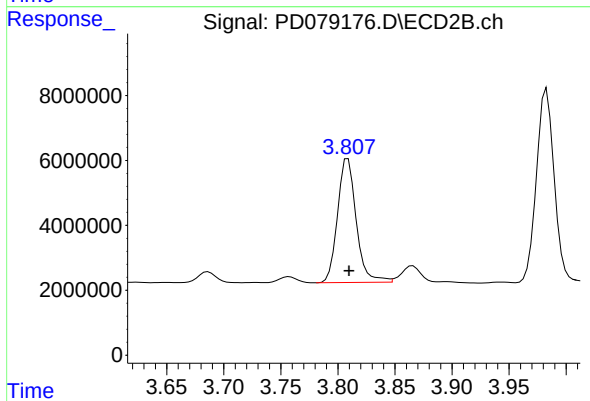

#23 Chlordane-1


R.T.: 3.809 min
Delta R.T.: 0.000 min
Response: 43663745
Conc: 502.72 ng/ml

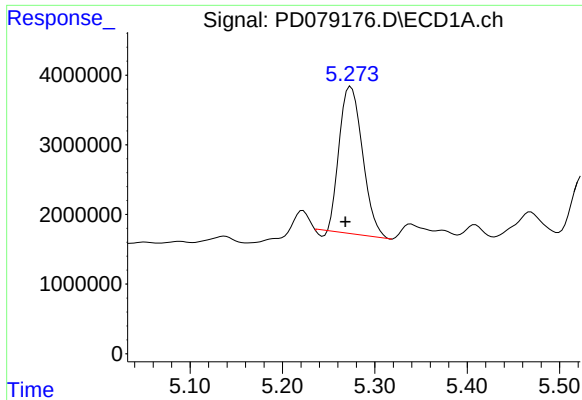

#24 Chlordane-2


R.T.: 5.274 min
Delta R.T.: 0.006 min
Response: 36651716
Conc: 459.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

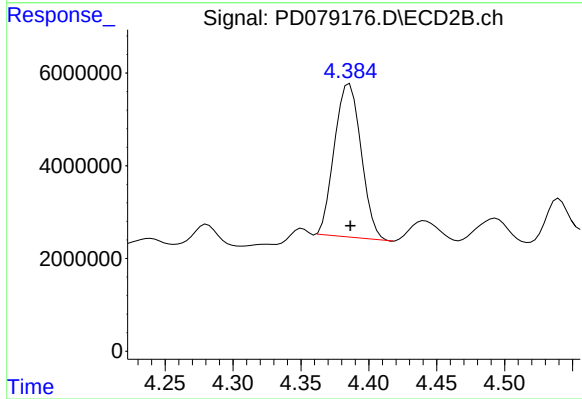


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 45306422
Conc: 498.65 ng/ml

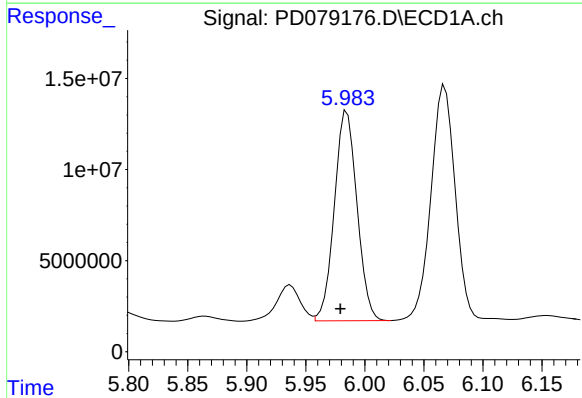


#25 Chlordane-3

R.T.: 5.985 min
Delta R.T.: 0.006 min
Response: 153611027
Conc: 495.51 ng/ml

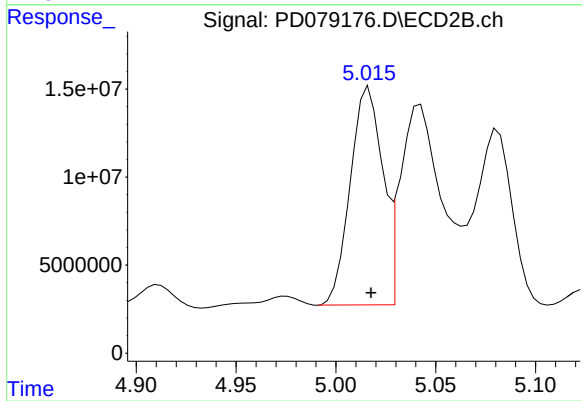

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 139025726
Conc: 521.22 ng/ml

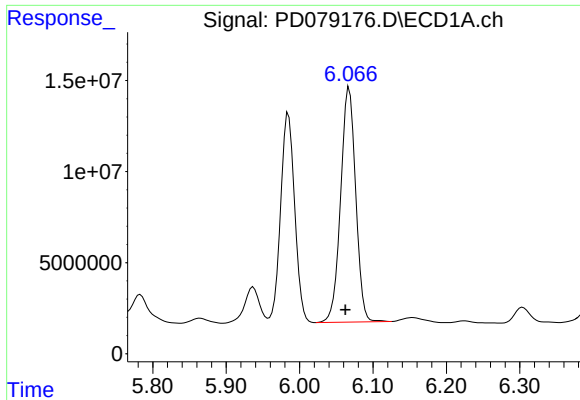

#26 Chlordane-4


R.T.: 6.068 min
Delta R.T.: 0.005 min
Response: 183864252
Conc: 494.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

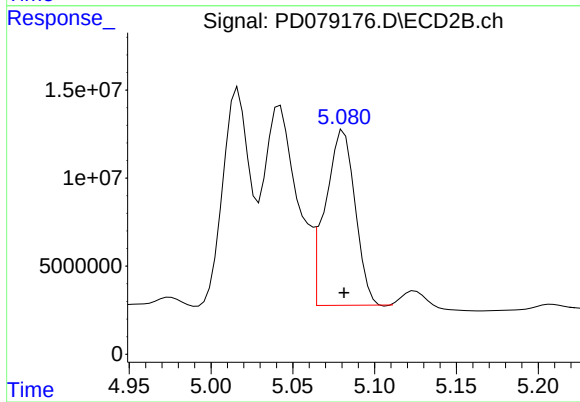


#26 Chlordane-4

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 125610216
Conc: 511.90 ng/ml

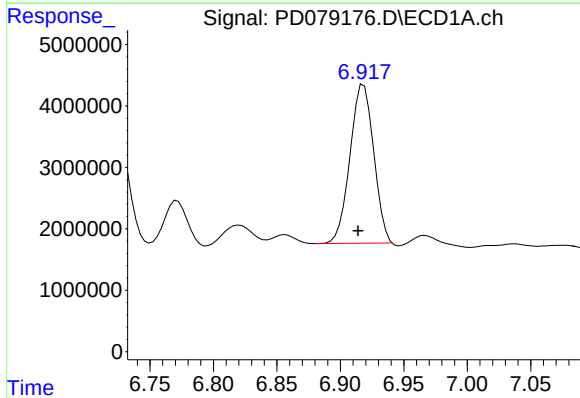


#27 Chlordane-5

R.T.: 6.918 min
Delta R.T.: 0.004 min
Response: 33534638
Conc: 477.26 ng/ml

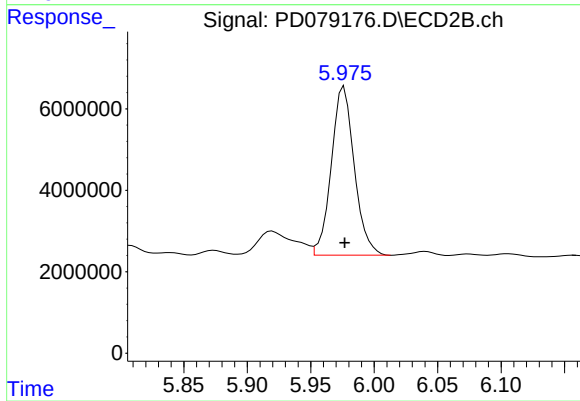

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 52250778
Conc: 524.27 ng/ml

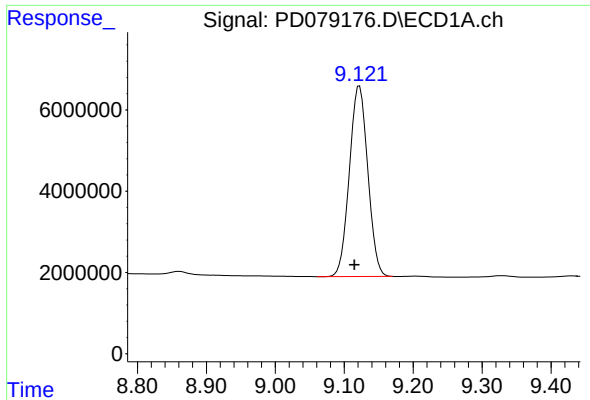

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.007 min
Response: 87046061
Conc: 43.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

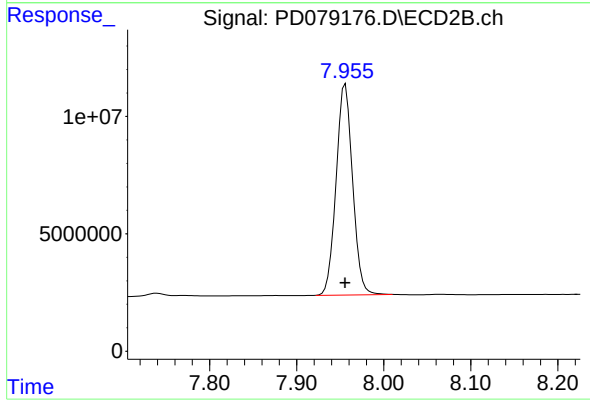

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 118393819
Conc: 48.57 ng/ml