

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
 Data File : PD066554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 12:27
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 15:41:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 15:40:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	10235386	49235077	5.353	5.708
27)	SA Decachlor...	8.167	9.024	13519353	59043677	11.695	11.265
Target Compounds							
2)	A alpha-BHC	3.877	4.363	14669604	60218092	5.098	5.564
3)	MA gamma-BHC...	4.158	4.647	14146431	55096044	5.163	5.480
4)	MA Heptachlor	4.452	5.147	14206327	55141650	5.019	5.650
9)	A Endosulfan I	5.475	6.197	11816106	43922534	5.187	5.613
13)	MA Dieldrin	5.717	6.454	24653351	87075161	9.901	10.927
14)	MA Endrin	5.974	6.674	21409677	74839778	10.087	10.986
16)	A 4,4'-DDD	6.099	6.799	17906294	70290779	9.857	10.848
17)	MA 4,4'-DDT	6.338	7.096	18458585	71919153	9.715	10.866
20)	A Methoxychlor	6.886	7.558	50527983	188.5E6	53.871	58.383


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 12:27
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 15:41:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 15:40:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

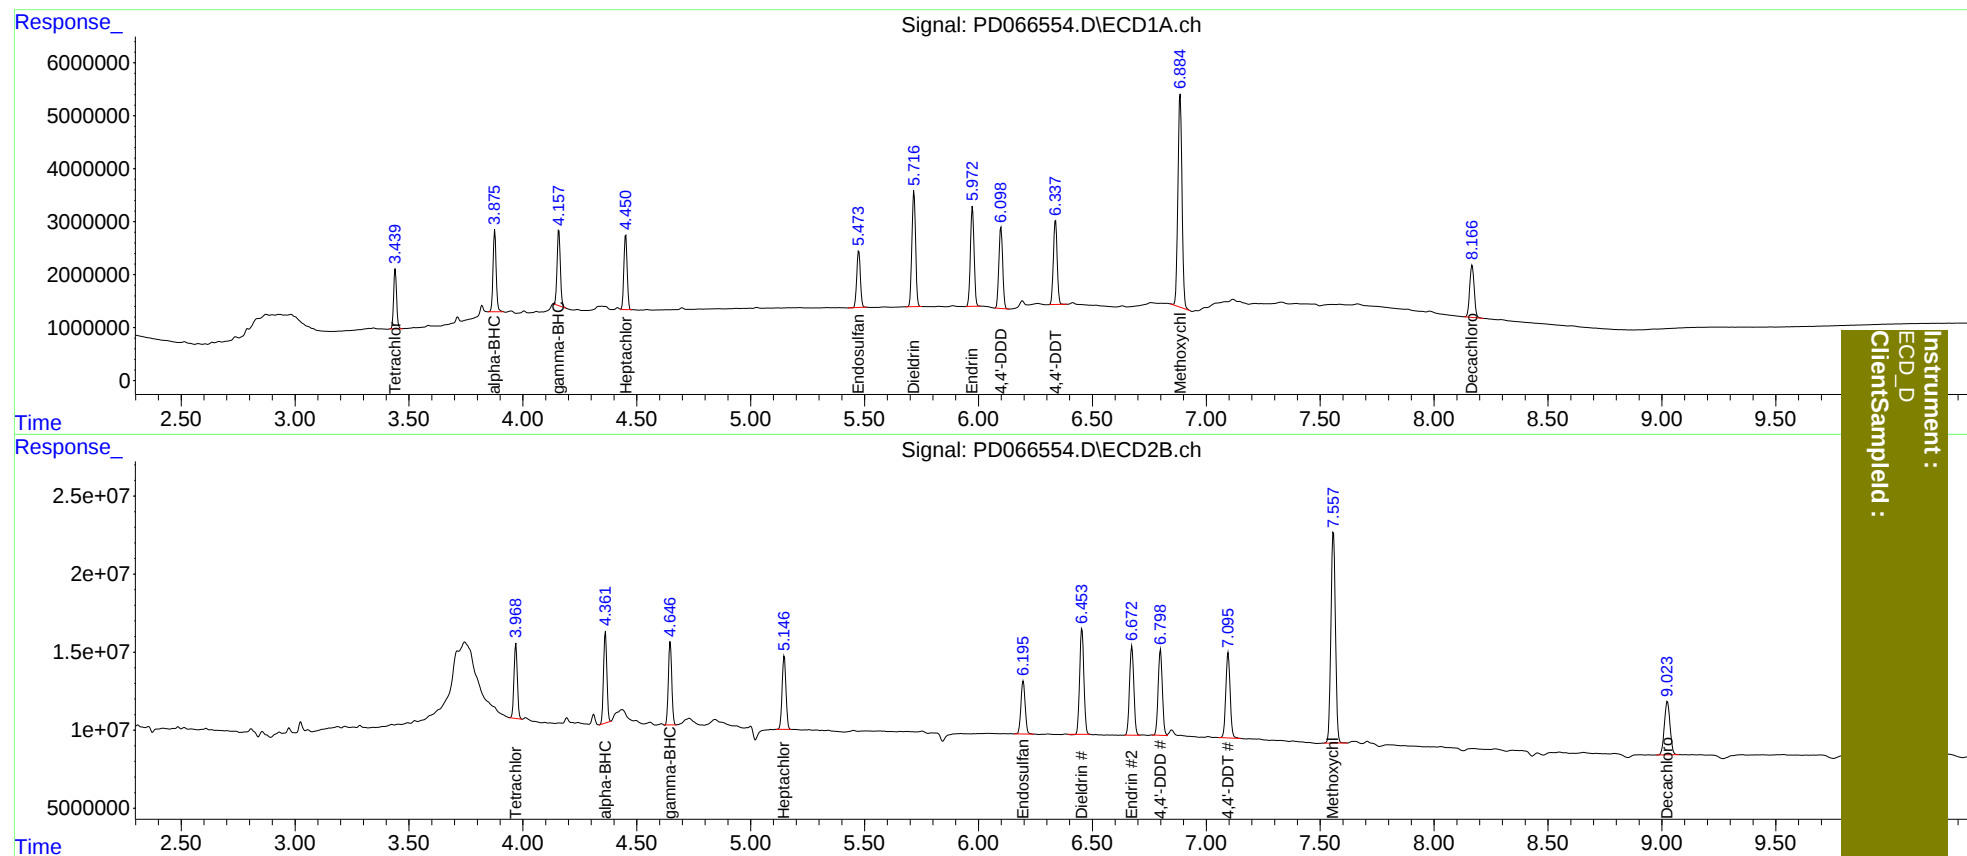


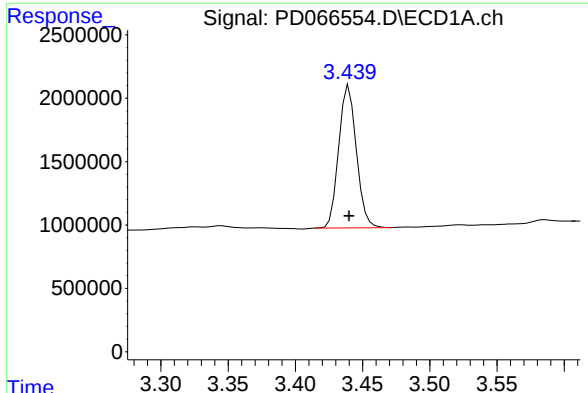

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 10235386
Conc: 5.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

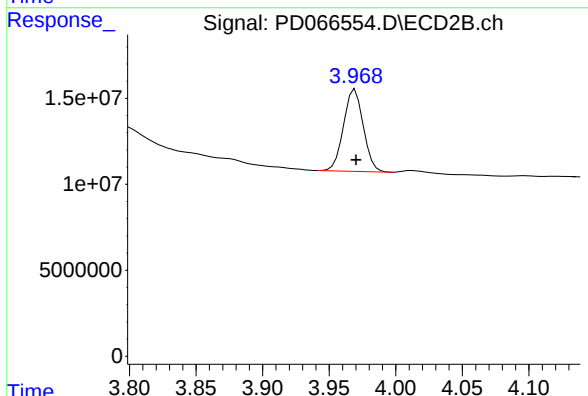


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 49235077
Conc: 5.71 ng/ml

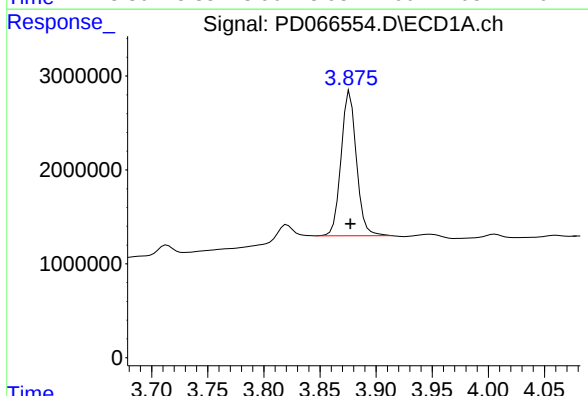


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 14669604
Conc: 5.10 ng/ml

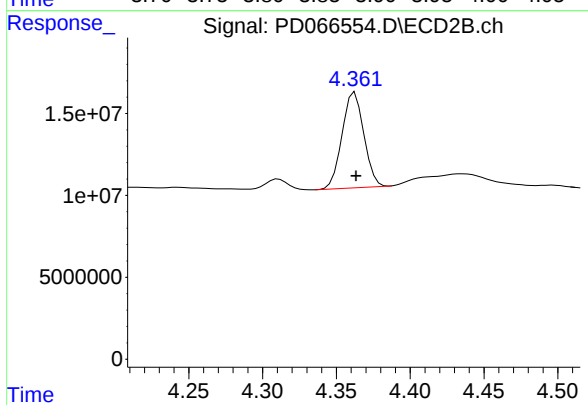

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 60218092
Conc: 5.56 ng/ml

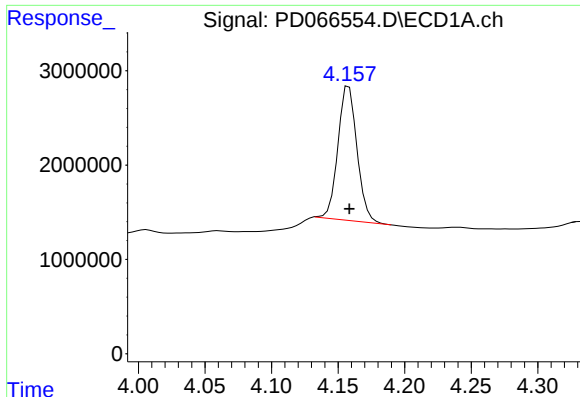

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 14146431
Conc: 5.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

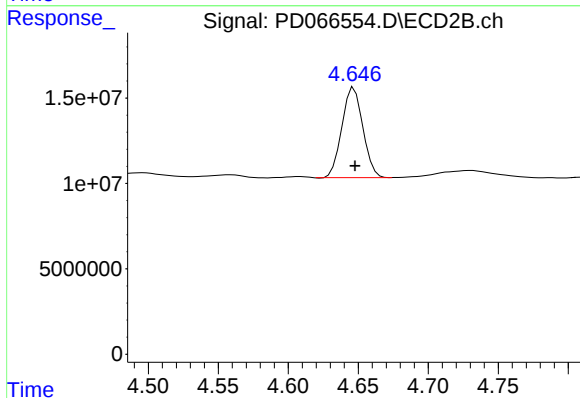


#3 gamma-BHC (Lindane)

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 55096044
Conc: 5.48 ng/ml

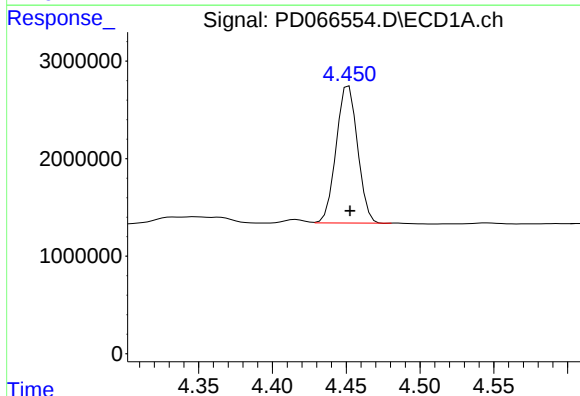


#4 Heptachlor

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 14206327
Conc: 5.02 ng/ml

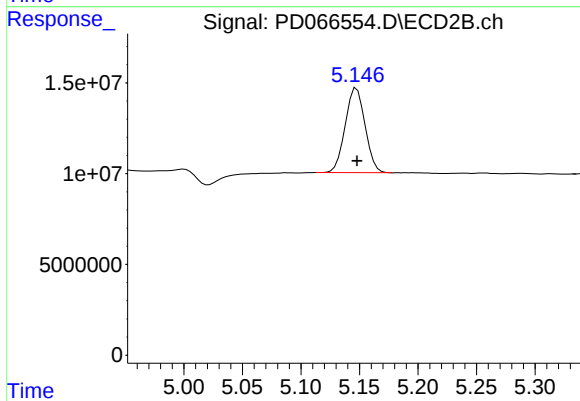

#4 Heptachlor


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 55141650
Conc: 5.65 ng/ml

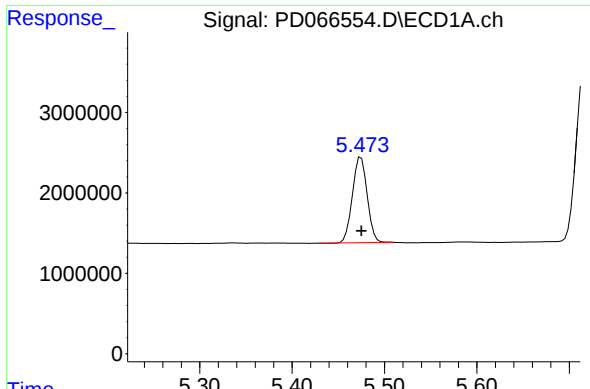

#9 Endosulfan I


R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 11816106
Conc: 5.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

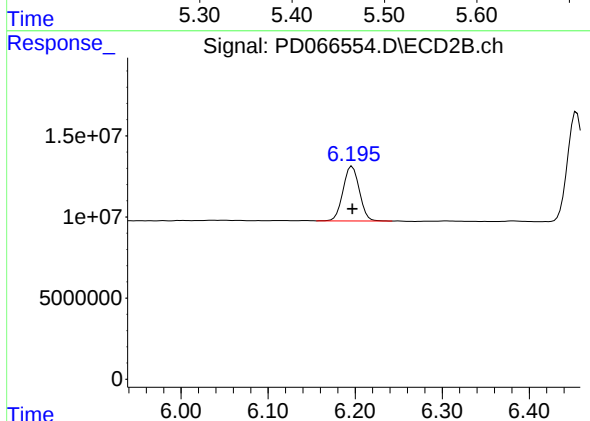


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 43922534
Conc: 5.61 ng/ml

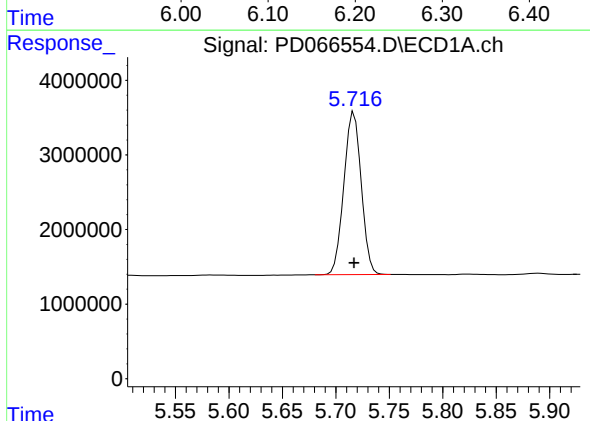


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 24653351
Conc: 9.90 ng/ml

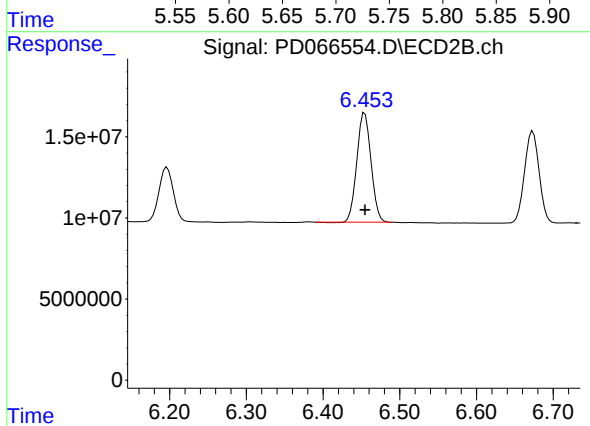

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 87075161
Conc: 10.93 ng/ml

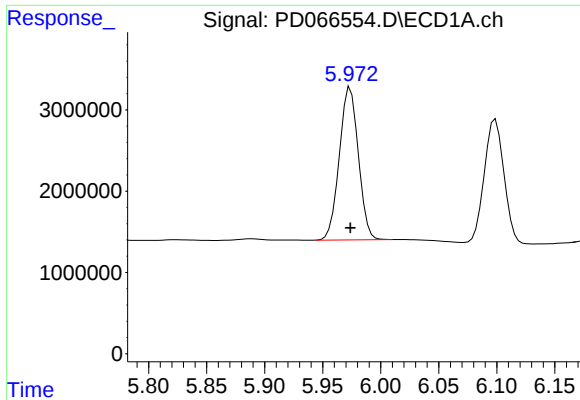

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 21409677
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

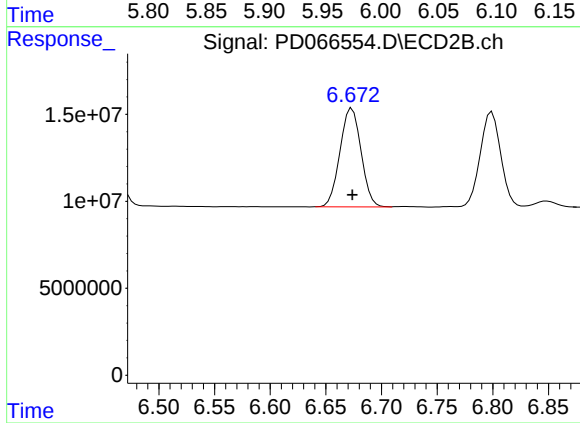


#14 Endrin

R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 74839778
Conc: 10.99 ng/ml

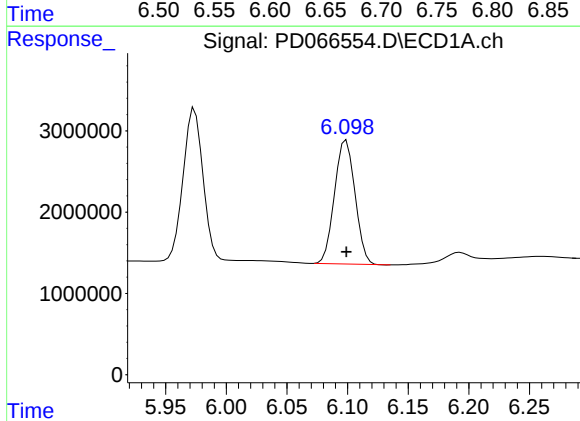


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 17906294
Conc: 9.86 ng/ml

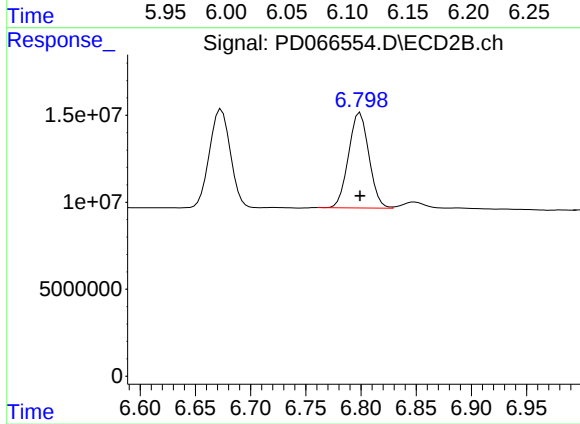

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 70290779
Conc: 10.85 ng/ml

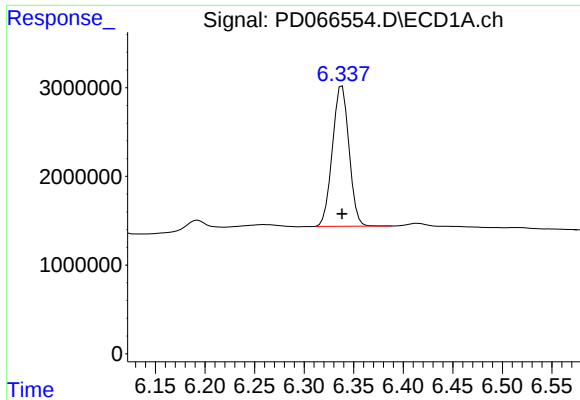

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 18458585
Conc: 9.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

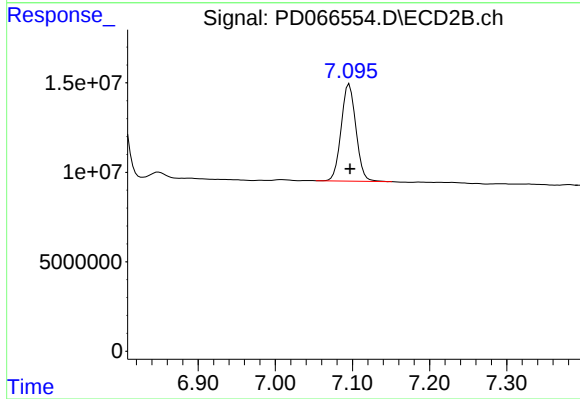


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: -0.001 min
Response: 71919153
Conc: 10.87 ng/ml

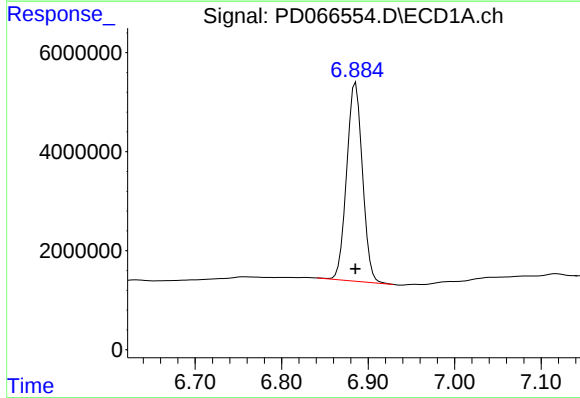


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 50527983
Conc: 53.87 ng/ml

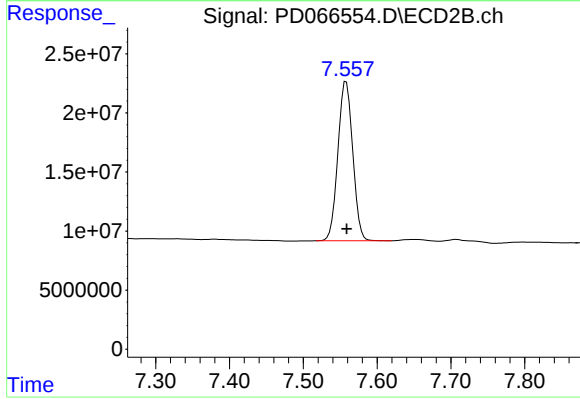

#20 Methoxychlor


R.T.: 7.558 min
Delta R.T.: 0.000 min
Response: 188532824
Conc: 58.38 ng/ml

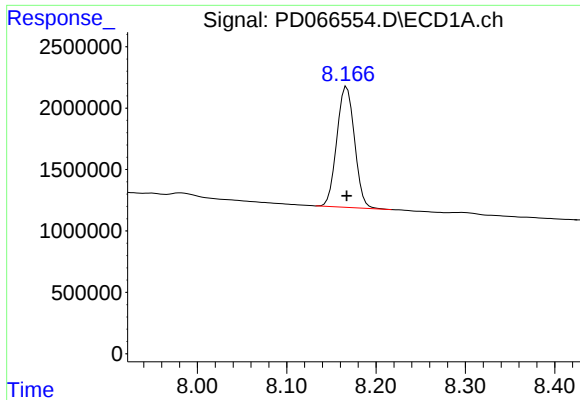

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 13519353
Conc: 11.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

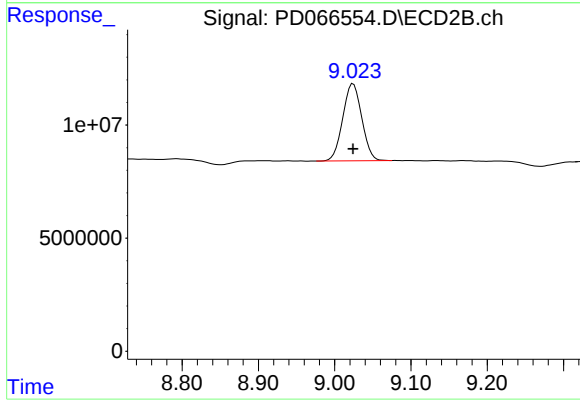

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 59043677
Conc: 11.27 ng/ml