

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
 Data File : PD066556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 12:54
 Operator : AJ\MA
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 15:41:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 15:40:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	19795575	92742007	10.353	10.753
27)	SA Decachlor...	8.167	9.024	24684468	111.3E6	21.354	21.227
Target Compounds							
2)	A alpha-BHC	3.876	4.363	28726075	114.9E6	9.982	10.619
3)	MA gamma-BHC...	4.158	4.647	27505121	106.3E6	10.038	10.572
4)	MA Heptachlor	4.452	5.147	28186182	104.0E6	9.959	10.656
9)	A Endosulfan I	5.474	6.197	22996806	83068621	10.095	10.616
13)	MA Dieldrin	5.717	6.455	49037528	167.3E6	19.695	20.994
14)	MA Endrin	5.974	6.673	41929550	143.9E6	19.755	21.127
16)	A 4,4'-DDD	6.099	6.799	35546623	134.9E6	19.567	20.825
17)	MA 4,4'-DDT	6.338	7.096	36795551	137.1E6	19.366	20.716
20)	A Methoxychlor	6.885	7.558	96037876	344.2E6	102.392	106.588


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 12:54
Operator : AJ\MA
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 15:41:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 15:40:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

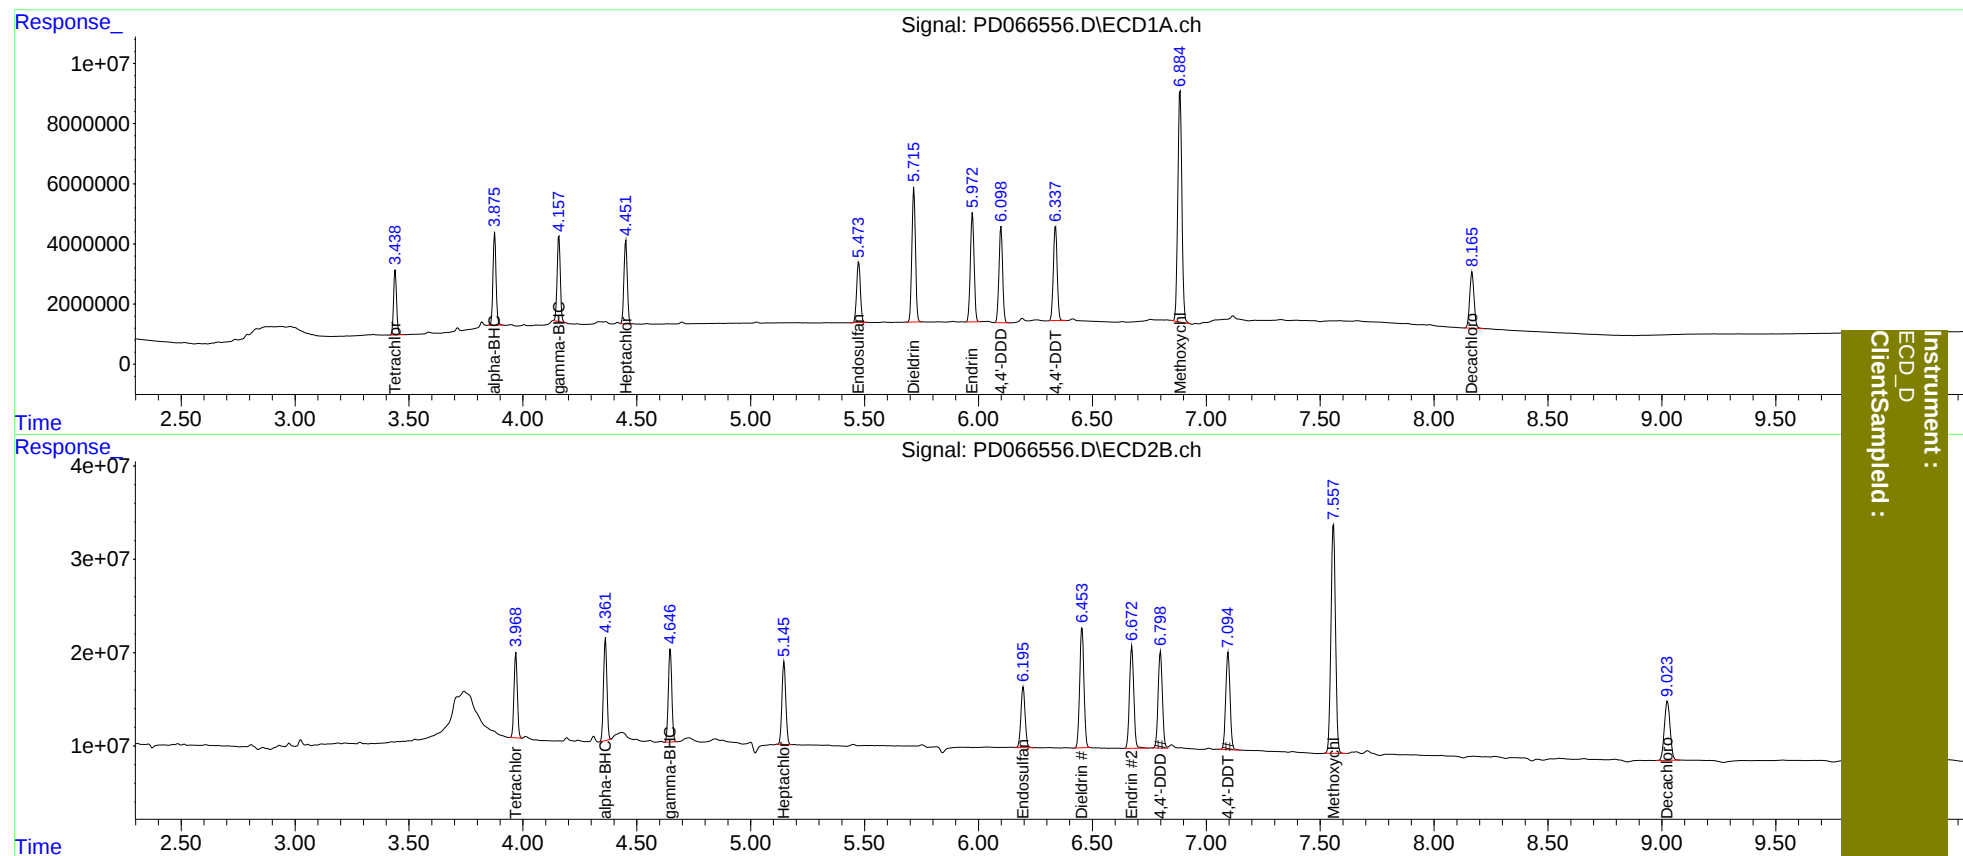


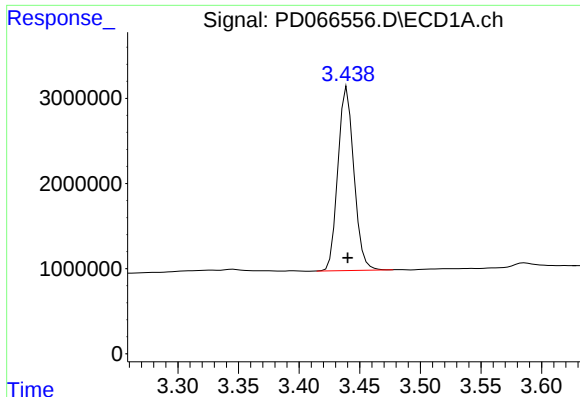

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 19795575
Conc: 10.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

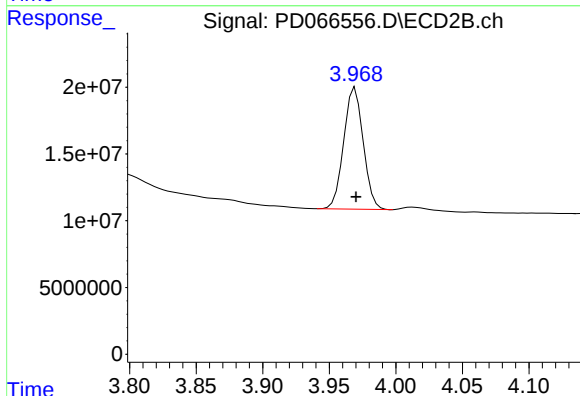


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 92742007
Conc: 10.75 ng/ml

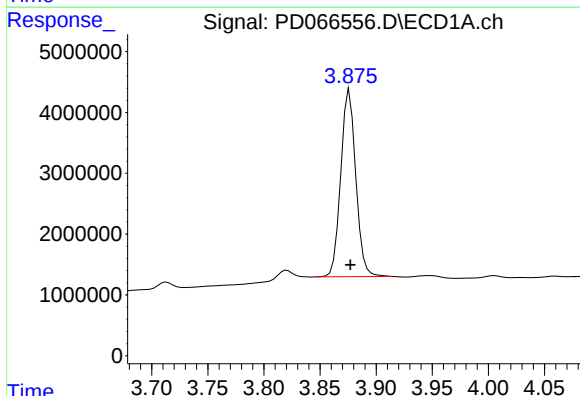


#2 alpha-BHC

R.T.: 3.876 min
Delta R.T.: 0.000 min
Response: 28726075
Conc: 9.98 ng/ml

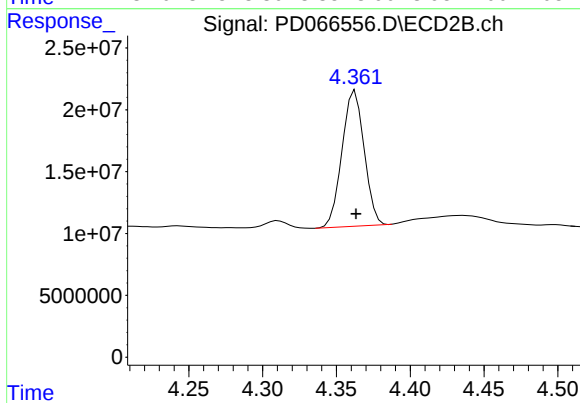

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 114916900
Conc: 10.62 ng/ml

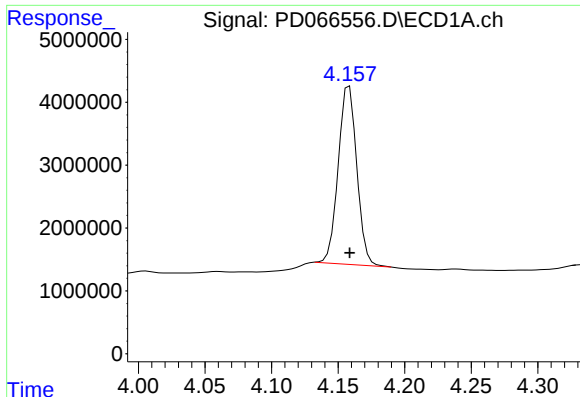

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 27505121
Conc: 10.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

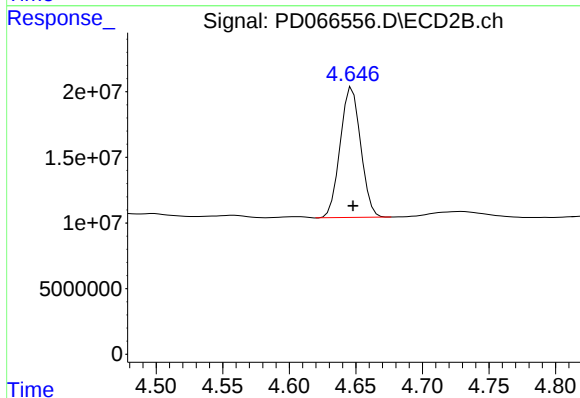


#3 gamma-BHC (Lindane)

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 106288491
Conc: 10.57 ng/ml

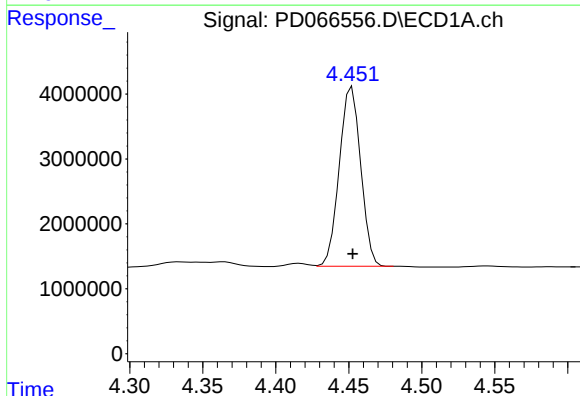


#4 Heptachlor

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 28186182
Conc: 9.96 ng/ml

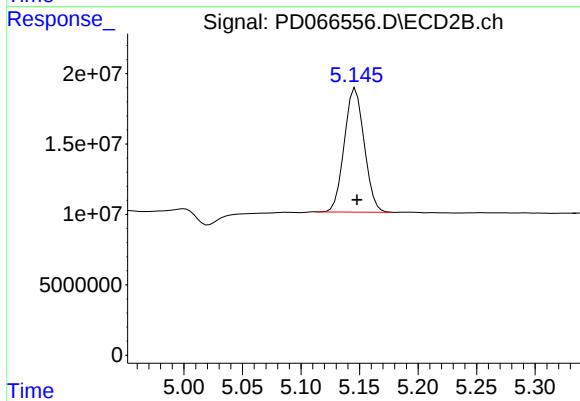

#4 Heptachlor


R.T.: 5.147 min
Delta R.T.: -0.001 min
Response: 103994037
Conc: 10.66 ng/ml

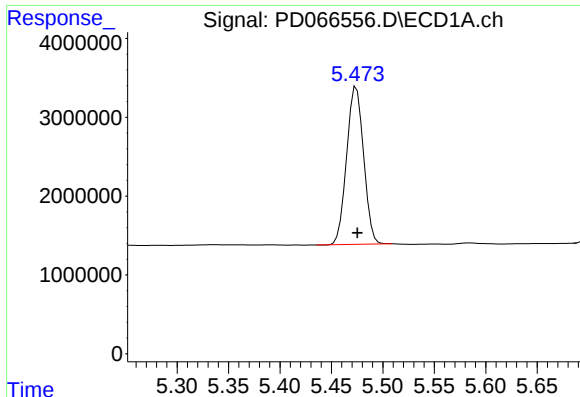

#9 Endosulfan I


R.T.: 5.474 min
Delta R.T.: 0.000 min
Response: 22996806
Conc: 10.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

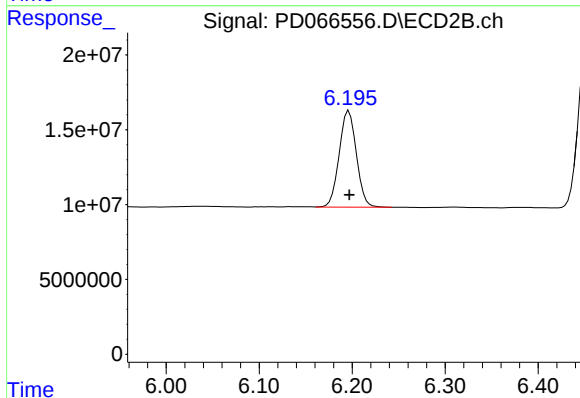


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 83068621
Conc: 10.62 ng/ml

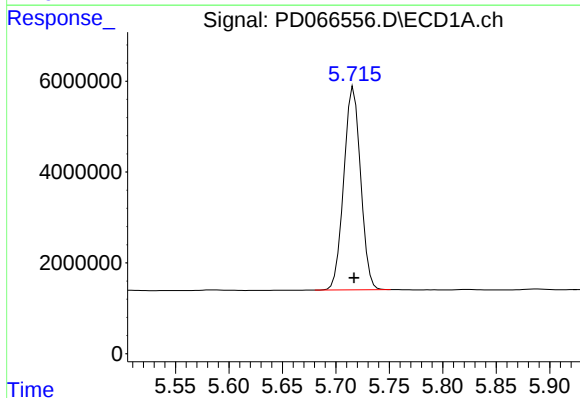


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 49037528
Conc: 19.69 ng/ml

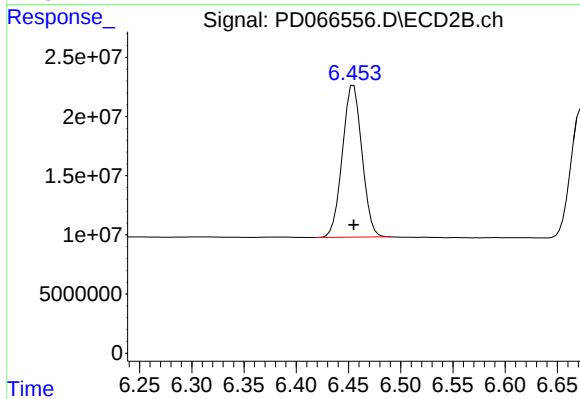

#13 Dieldrin


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 167300792
Conc: 20.99 ng/ml

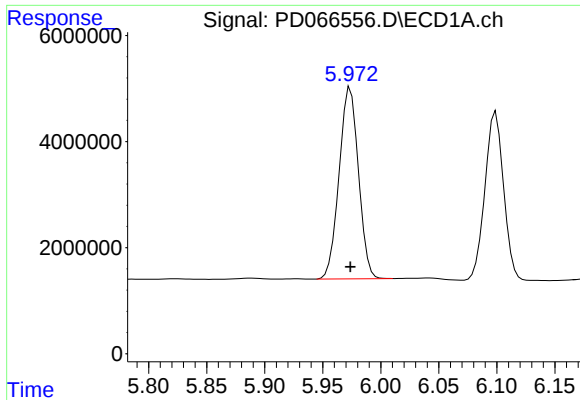

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 41929550
Conc: 19.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

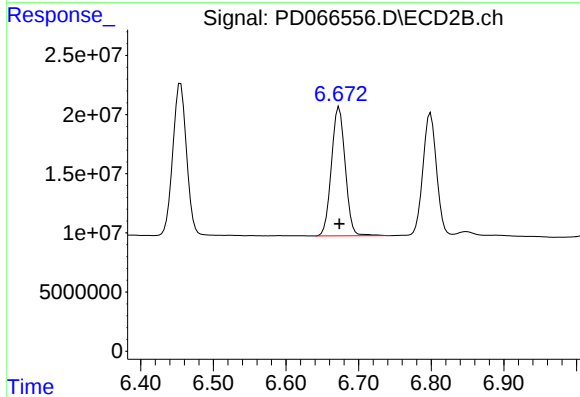


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 143920407
Conc: 21.13 ng/ml

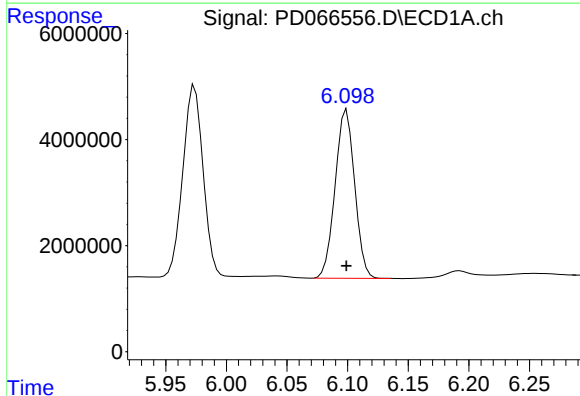


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 35546623
Conc: 19.57 ng/ml

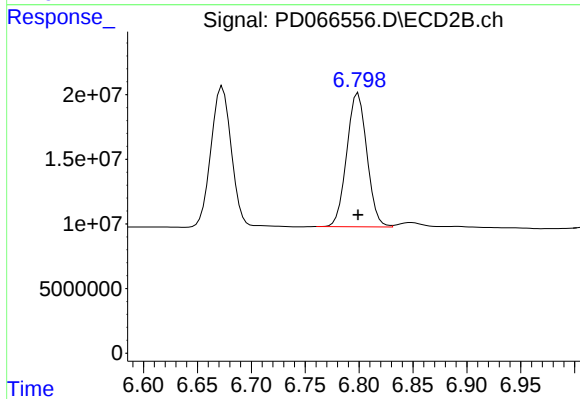

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 134940658
Conc: 20.83 ng/ml

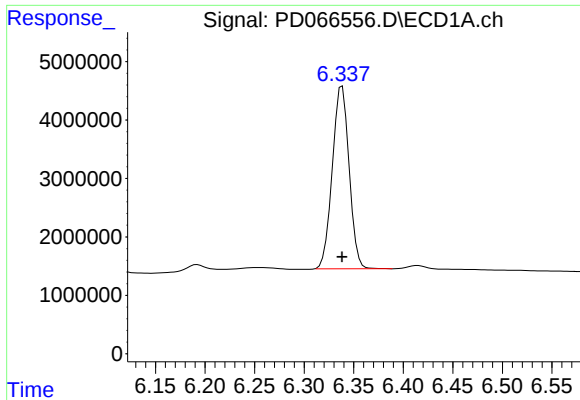

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 36795551
Conc: 19.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

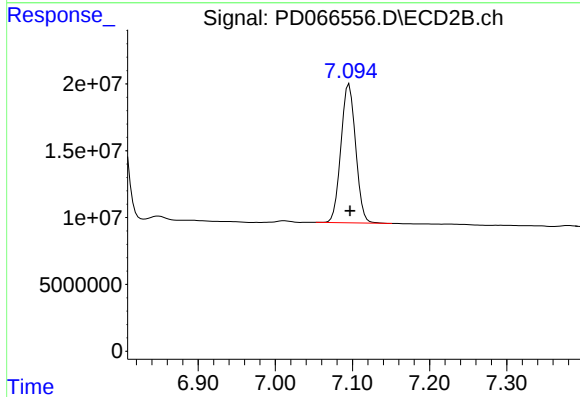


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: -0.001 min
Response: 137108567
Conc: 20.72 ng/ml

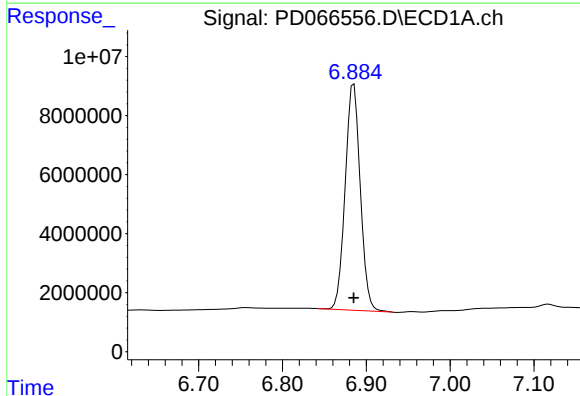


#20 Methoxychlor

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 96037876
Conc: 102.39 ng/ml

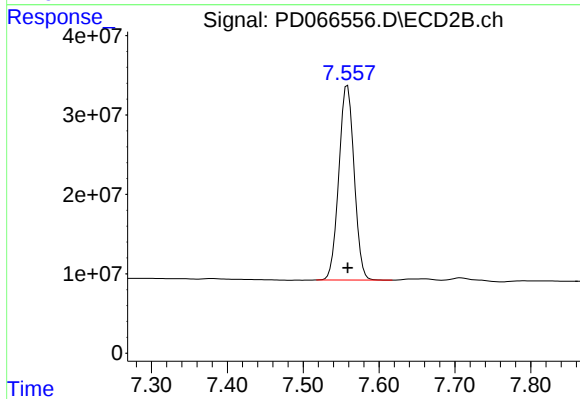

#20 Methoxychlor


R.T.: 7.558 min
Delta R.T.: 0.000 min
Response: 344196674
Conc: 106.59 ng/ml

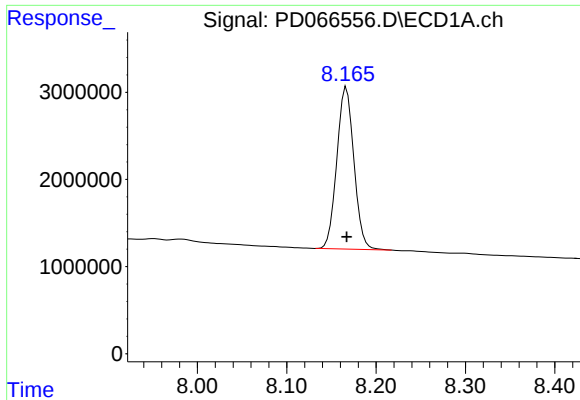

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 24684468
Conc: 21.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

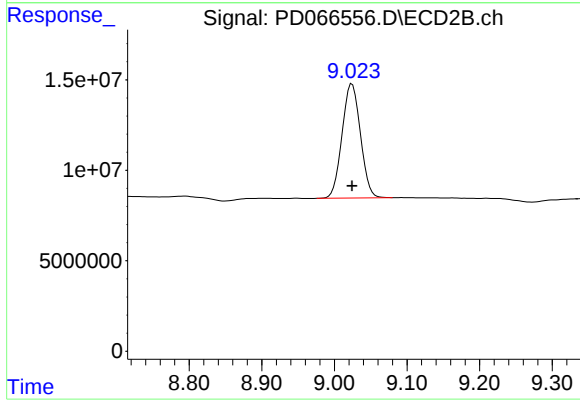

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 111259245
Conc: 21.23 ng/ml