

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
 Data File : PD066560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 13:49
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 15:41:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 15:40:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	74195037	317.6E6	38.804	36.827
27)	SA Decachlor...	8.167	9.025	85996166	383.1E6	74.393	73.100
Target Compounds							
2)	A alpha-BHC	3.877	4.363	116.7E6	408.2E6	40.550	37.718
3)	MA gamma-BHC...	4.159	4.648	108.8E6	379.3E6	39.694	37.724
4)	MA Heptachlor	4.453	5.148	112.9E6	361.7E6	39.884	37.063
9)	A Endosulfan I	5.475	6.197	89179521	288.7E6	39.149	36.896
13)	MA Dieldrin	5.717	6.455	198.8E6	598.2E6	79.824	75.070
14)	MA Endrin	5.975	6.674	166.6E6	506.4E6	78.470	74.333
16)	A 4,4'-DDD	6.100	6.800	143.1E6	484.0E6	78.760	74.689
17)	MA 4,4'-DDT	6.339	7.097	151.1E6	497.5E6	79.538	75.171
20)	A Methoxychlor	6.886	7.559	356.1E6	1158.1E6	379.665	358.635


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 13:49
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 15:41:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 15:40:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

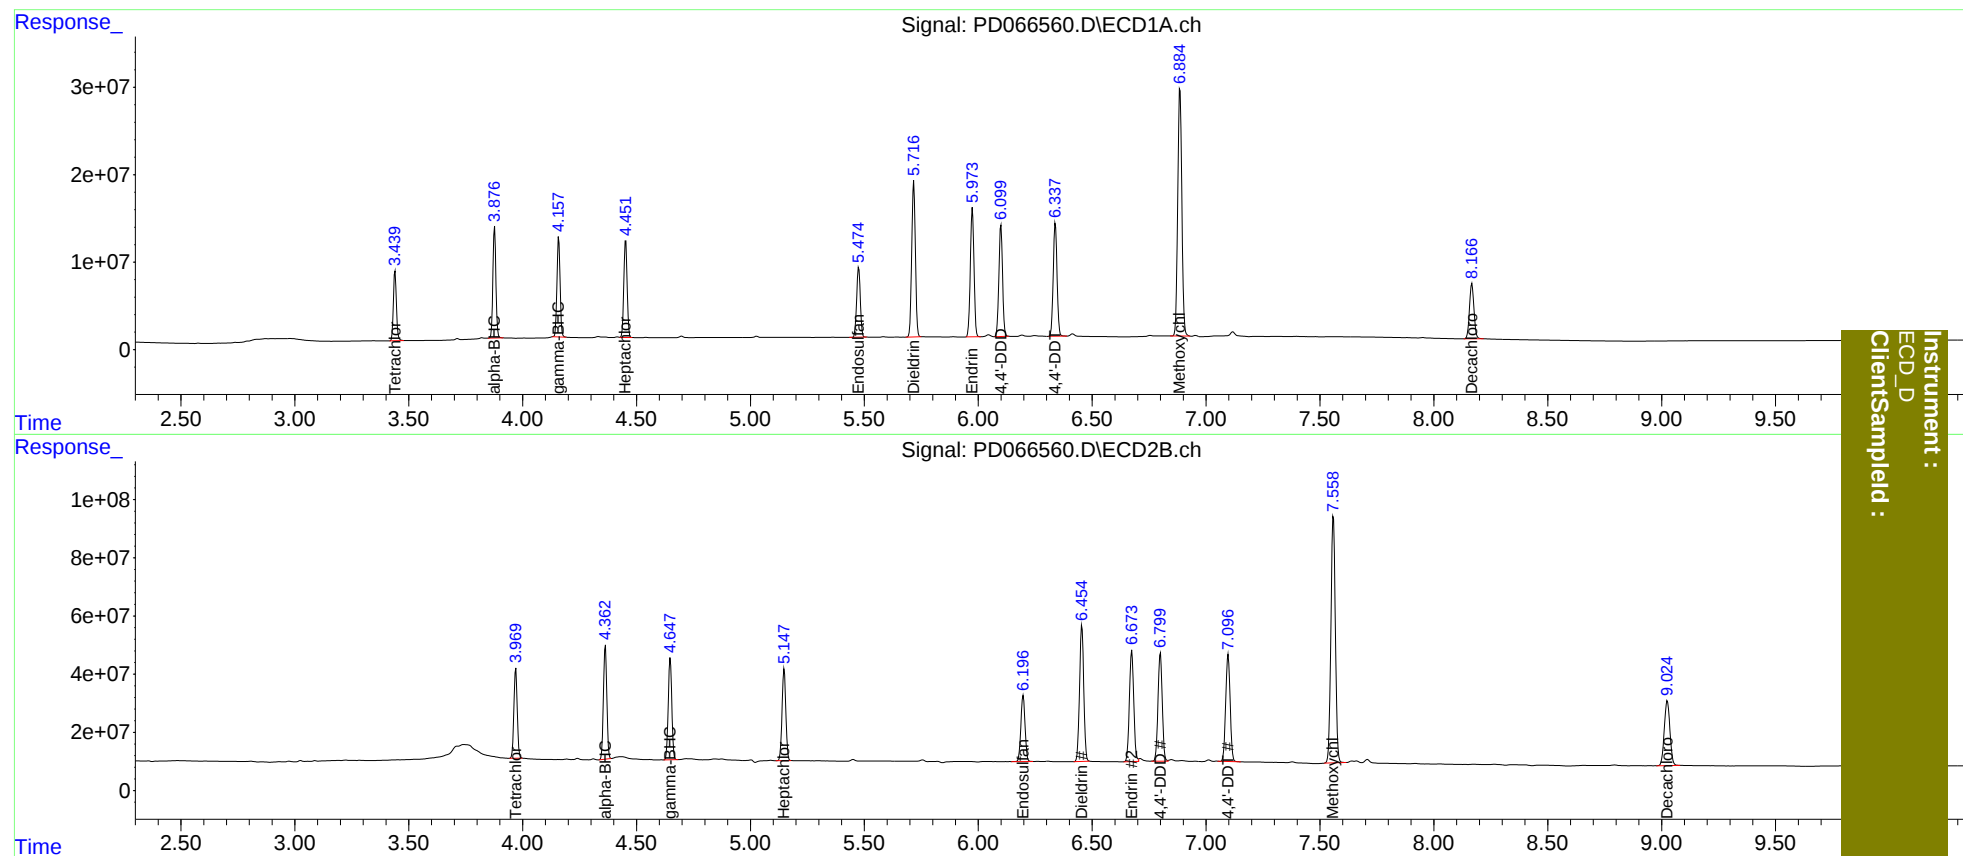


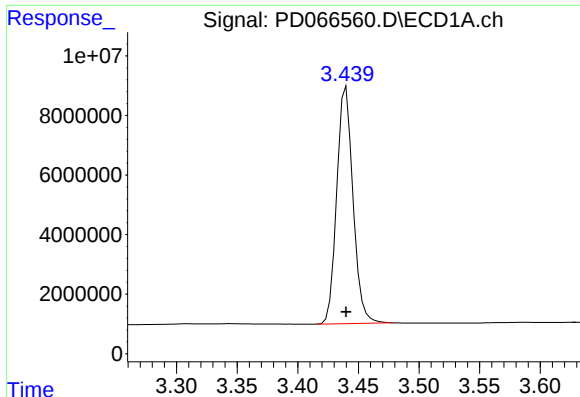

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 74195037
Conc: 38.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

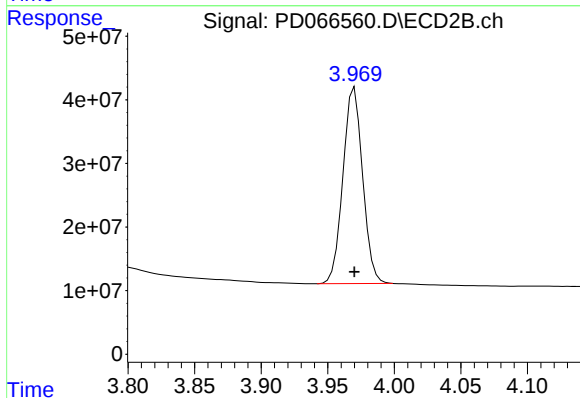


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 317638649
Conc: 36.83 ng/ml

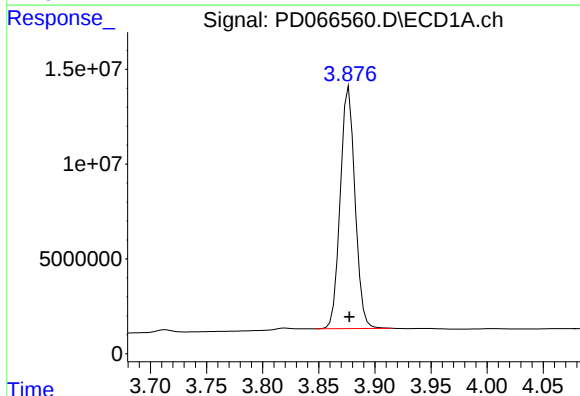


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 116693567
Conc: 40.55 ng/ml

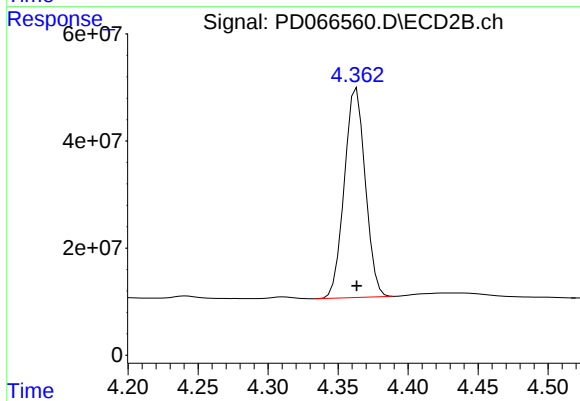

#2 alpha-BHC


R.T.: 4.363 min
Delta R.T.: 0.000 min
Response: 408190664
Conc: 37.72 ng/ml

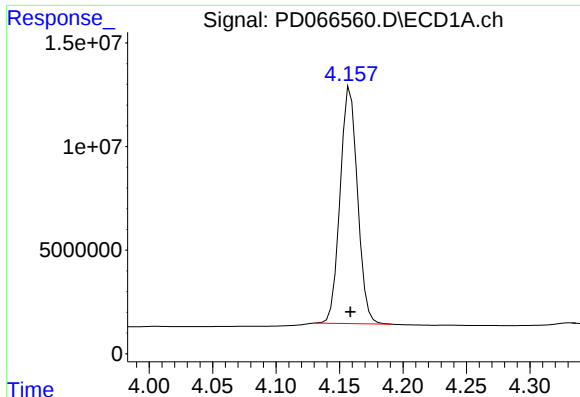

#3 gamma-BHC (Lindane)


R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 108770724
Conc: 39.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

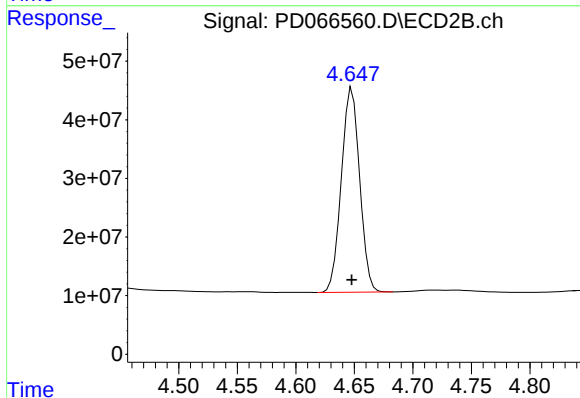


#3 gamma-BHC (Lindane)

R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 379279616
Conc: 37.72 ng/ml

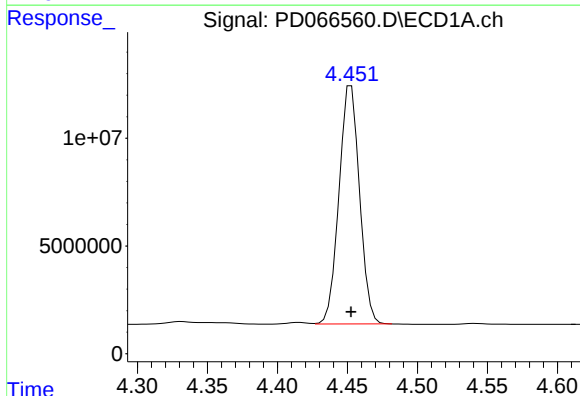


#4 Heptachlor

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 112884809
Conc: 39.88 ng/ml

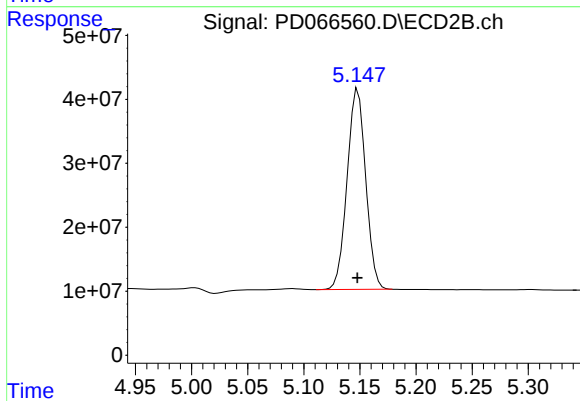

#4 Heptachlor


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 361693365
Conc: 37.06 ng/ml

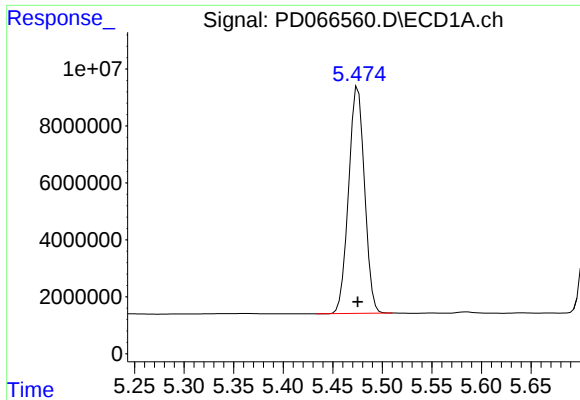

#9 Endosulfan I


R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 89179521
Conc: 39.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

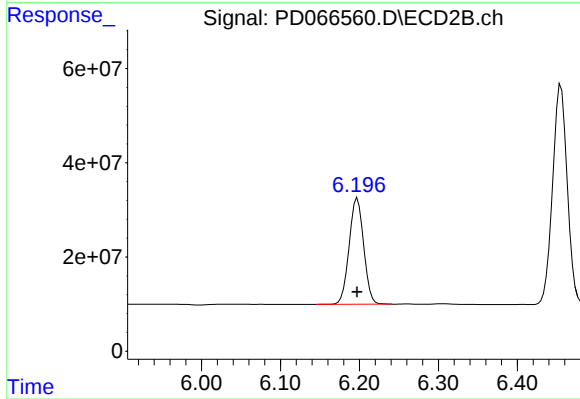


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 288700903
Conc: 36.90 ng/ml

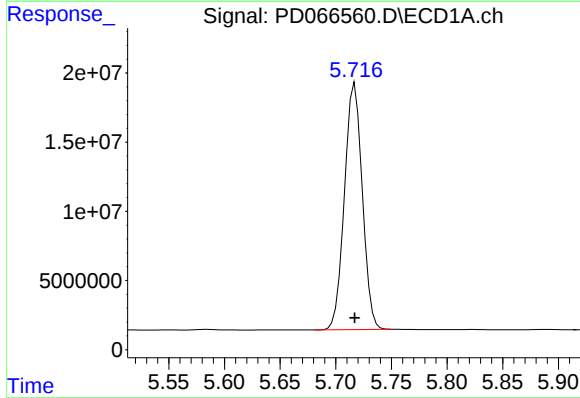


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 198751473
Conc: 79.82 ng/ml

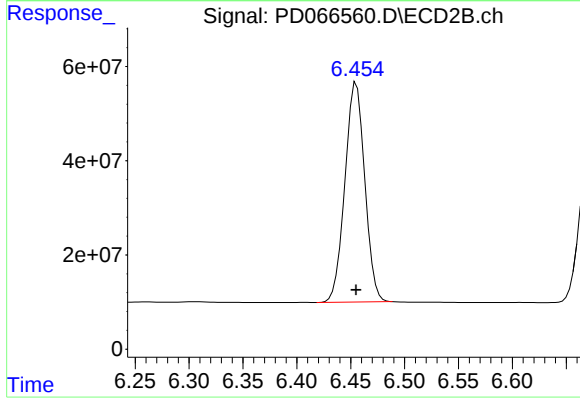

#13 Dieldrin


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 598223930
Conc: 75.07 ng/ml

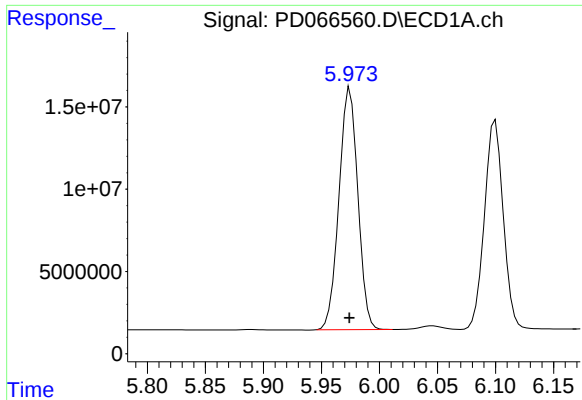

#14 Endrin


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 166550467
Conc: 78.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

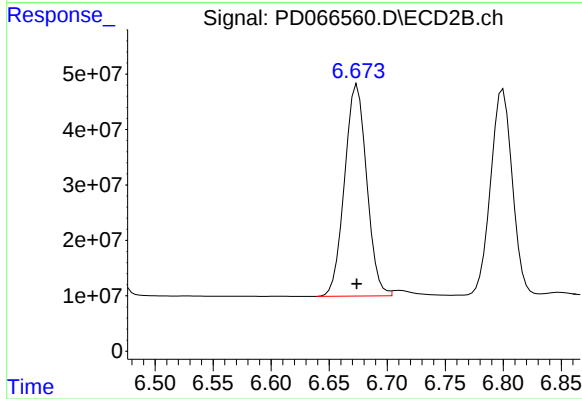


#14 Endrin

R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 506380675
Conc: 74.33 ng/ml

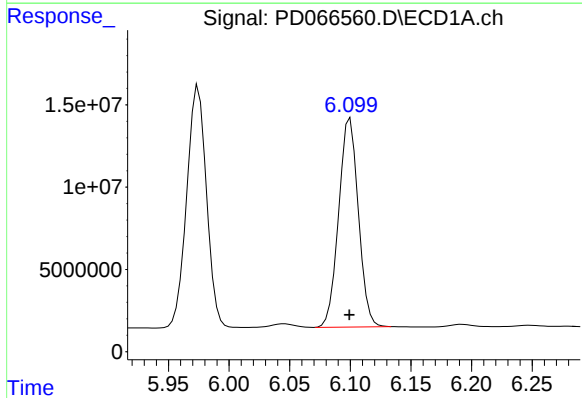


#16 4,4'-DDD

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 143079434
Conc: 78.76 ng/ml

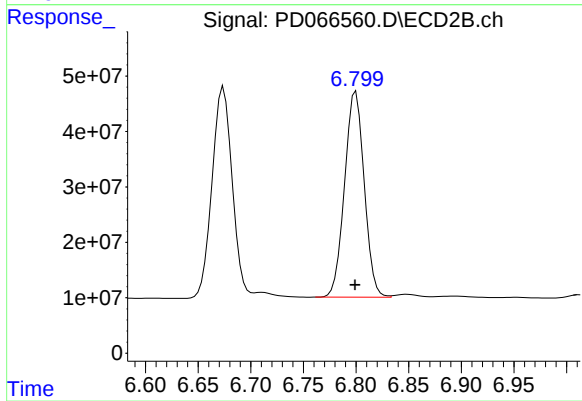

#16 4,4'-DDD


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 483961255
Conc: 74.69 ng/ml

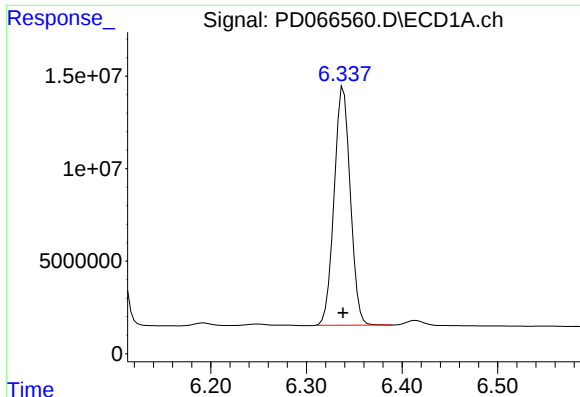

#17 4,4'-DDT


R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 151125808
Conc: 79.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

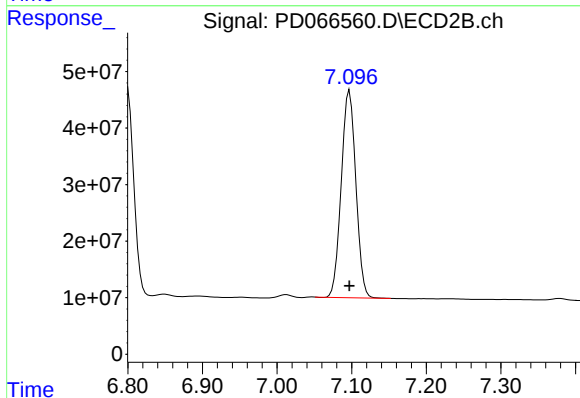


#17 4,4'-DDT

R.T.: 7.097 min
Delta R.T.: 0.000 min
Response: 497512849
Conc: 75.17 ng/ml

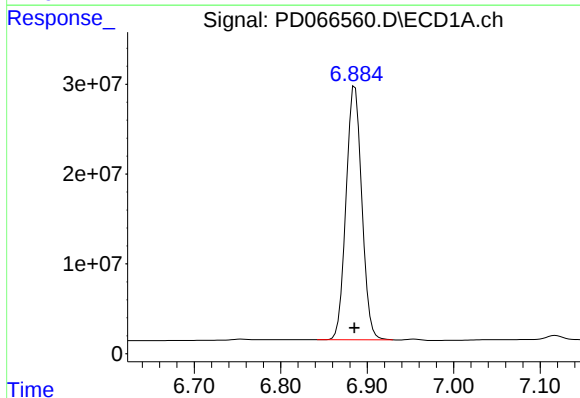


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 356104803
Conc: 379.66 ng/ml

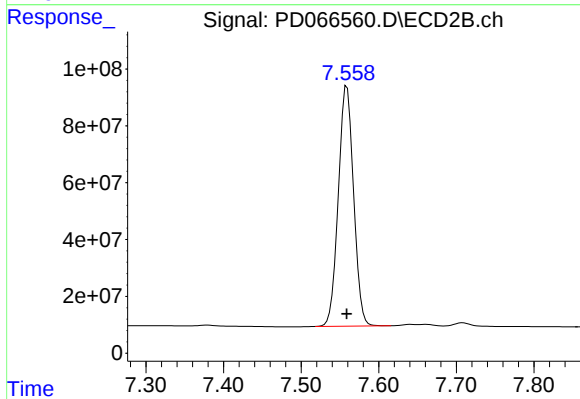

#20 Methoxychlor


R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 1158111189
Conc: 358.64 ng/ml

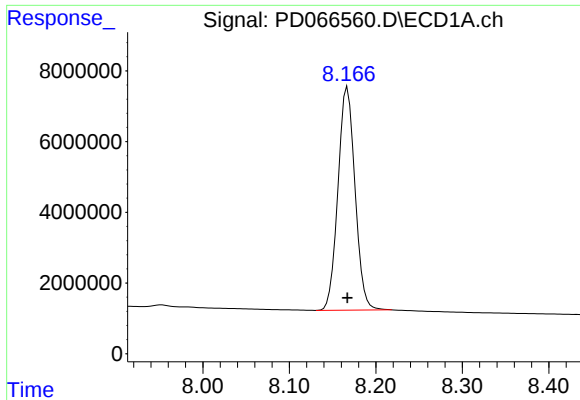

#27 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.000 min
Response: 85996166
Conc: 74.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

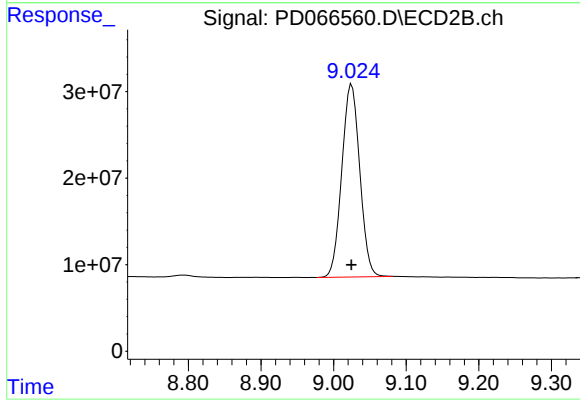

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 383137577
Conc: 73.10 ng/ml