

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
 Data File : PD066562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 16:20
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 16:38:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:24:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.969	149.7E6	609.2E6	78.318	70.631
27)	SA Decachlor...	8.168	9.023	166.6E6	732.6E6	144.132	139.766
Target Compounds							
2)	A alpha-BHC	3.877	4.362	242.7E6	808.7E6	84.332	74.726
3)	MA gamma-BHC...	4.158	4.647	224.3E6	747.5E6	81.857	74.349
4)	MA Heptachlor	4.452	5.147	232.9E6	702.3E6	82.305	71.968
9)	A Endosulfan I	5.475	6.197	183.3E6	559.1E6	80.448	71.455
13)	MA Dieldrin	5.717	6.455	413.7E6	1179.1E6	166.166	147.969
14)	MA Endrin	5.974	6.673	341.9E6	977.6E6	161.080	143.504
16)	A 4,4'-DDD	6.099	6.799	300.4E6	955.9E6	165.348	147.521
17)	MA 4,4'-DDT	6.338	7.097	316.6E6	983.4E6	166.650	148.578
20)	A Methoxychlor	6.886	7.559	709.5E6	2257.3E6	756.466	699.039


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 16:20
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 16:38:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:24:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

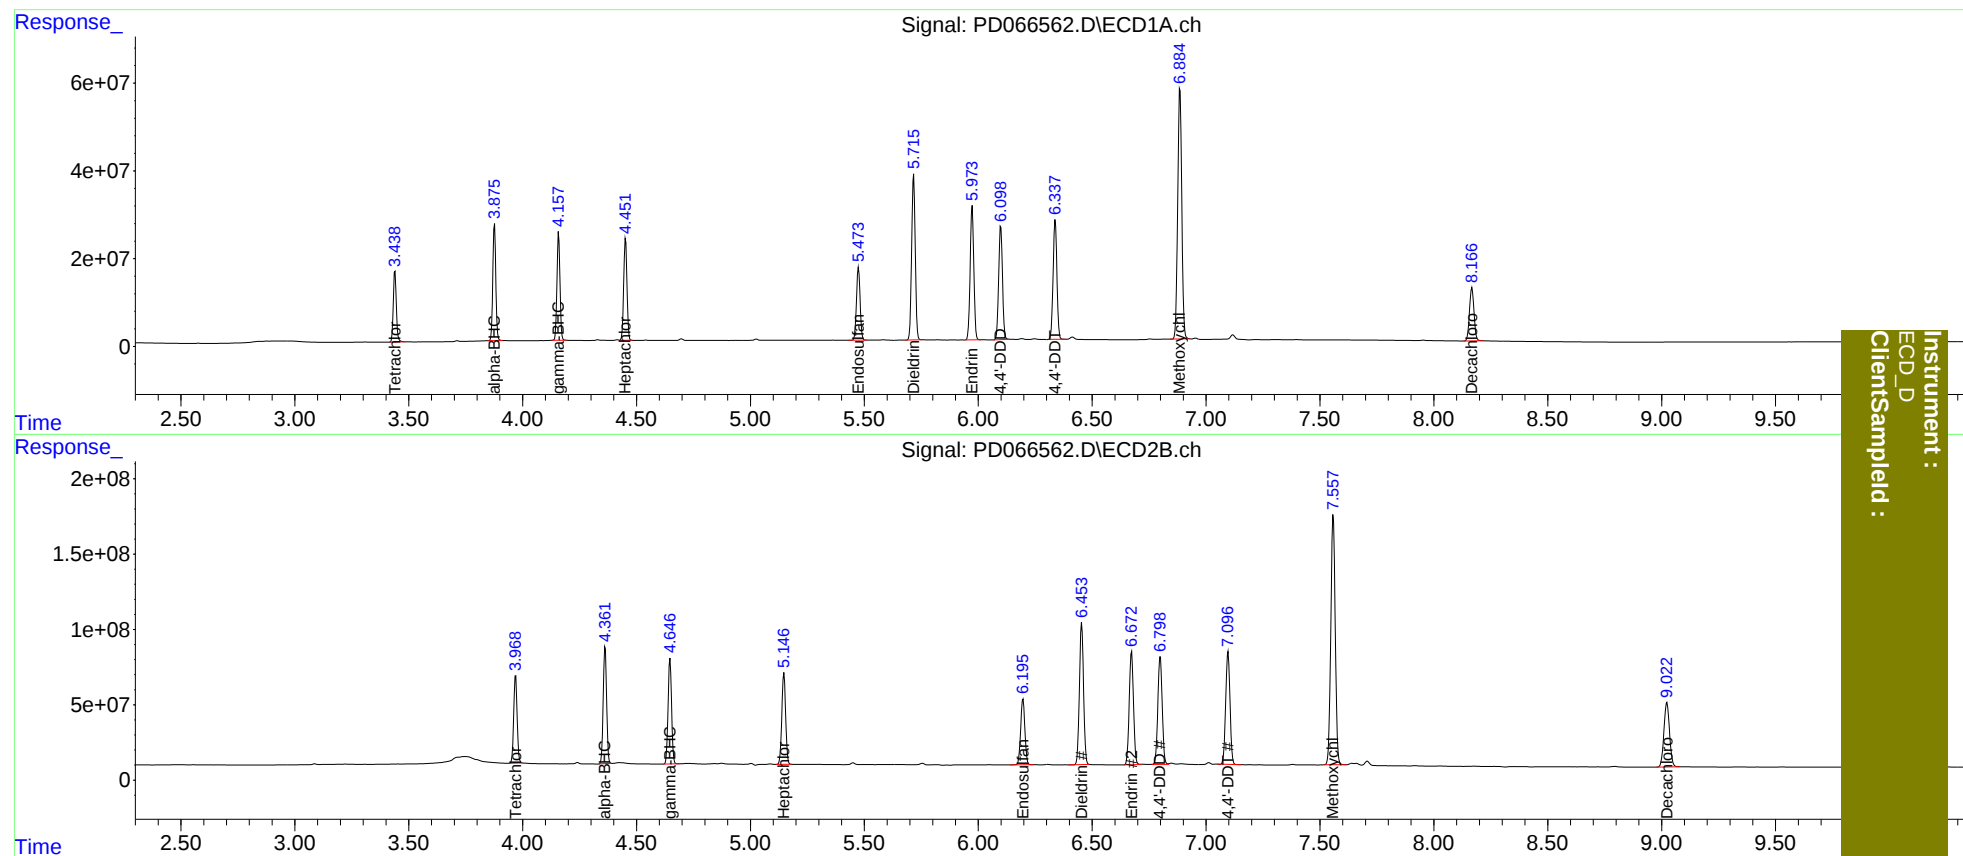


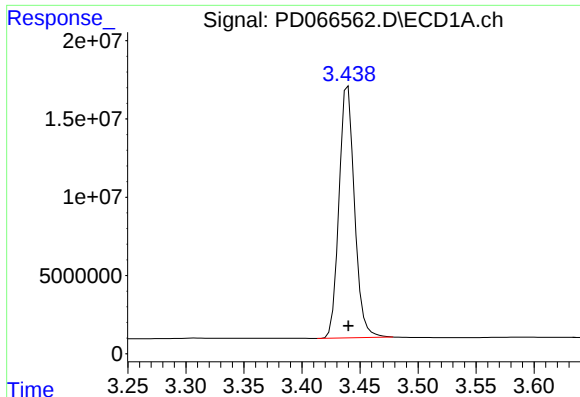

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.000 min
Response: 149746190
Conc: 78.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

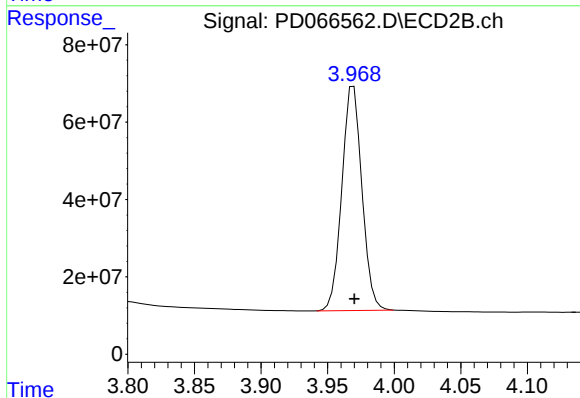


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 609201133
Conc: 70.63 ng/ml

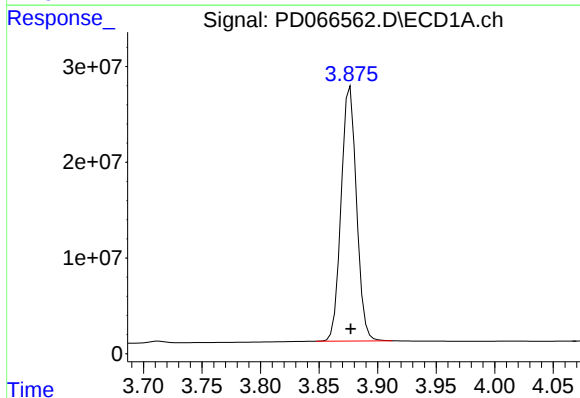


#2 alpha-BHC

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 242688057
Conc: 84.33 ng/ml

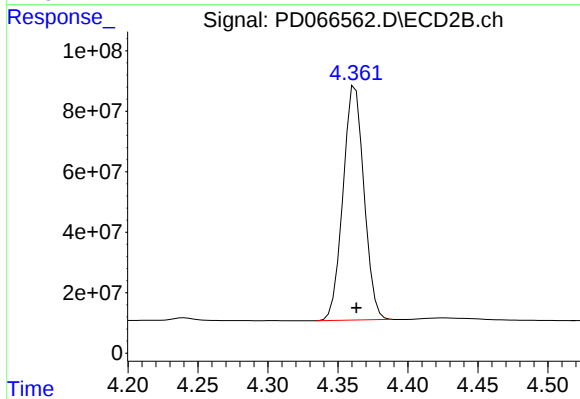

#2 alpha-BHC


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 808685870
Conc: 74.73 ng/ml

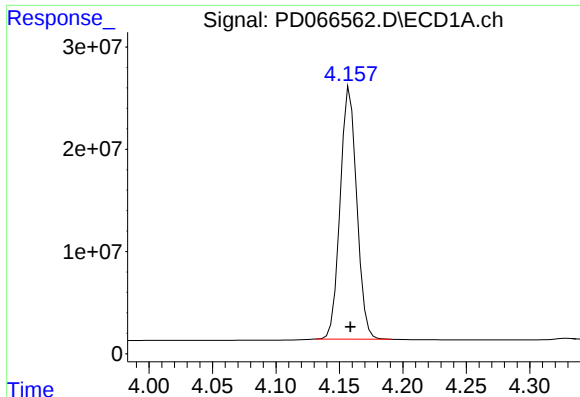

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 224304562
Conc: 81.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

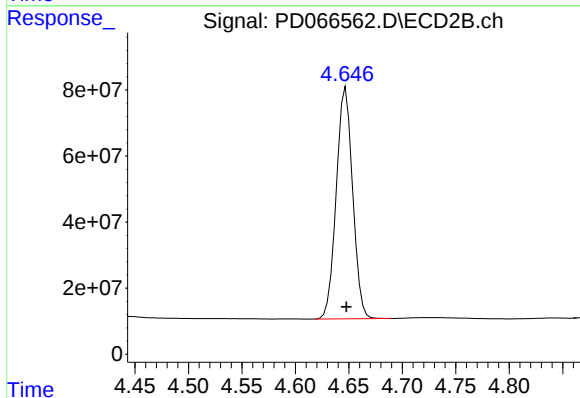


#3 gamma-BHC (Lindane)

R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 747509941
Conc: 74.35 ng/ml

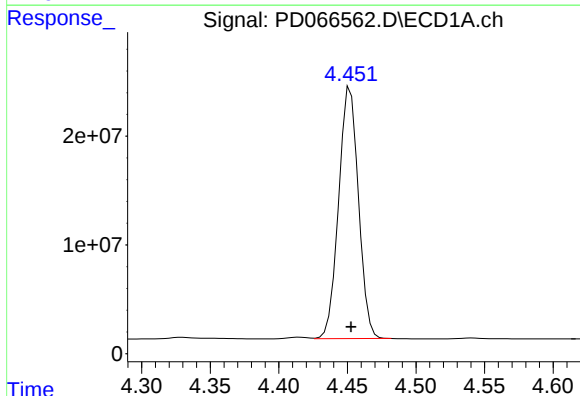


#4 Heptachlor

R.T.: 4.452 min
Delta R.T.: 0.000 min
Response: 232948406
Conc: 82.30 ng/ml

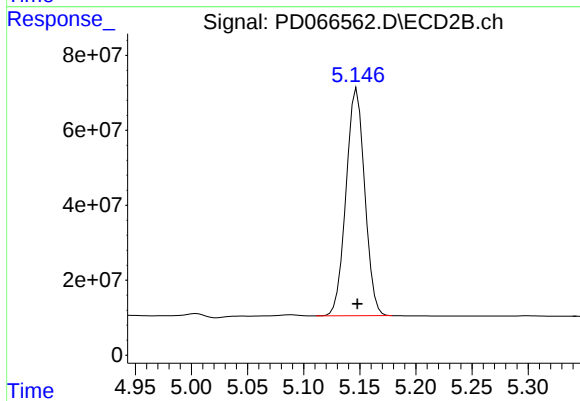

#4 Heptachlor


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 702330543
Conc: 71.97 ng/ml

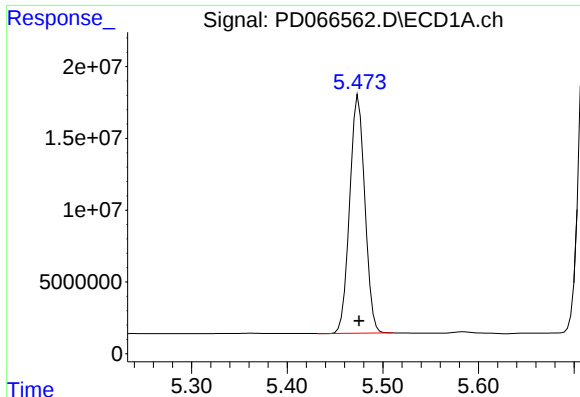

#9 Endosulfan I


R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 183255075
Conc: 80.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

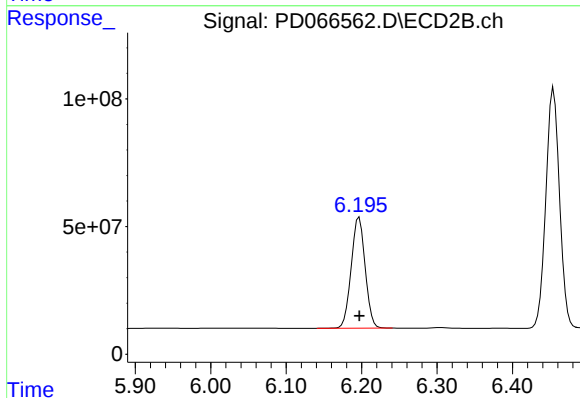


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 559122290
Conc: 71.46 ng/ml

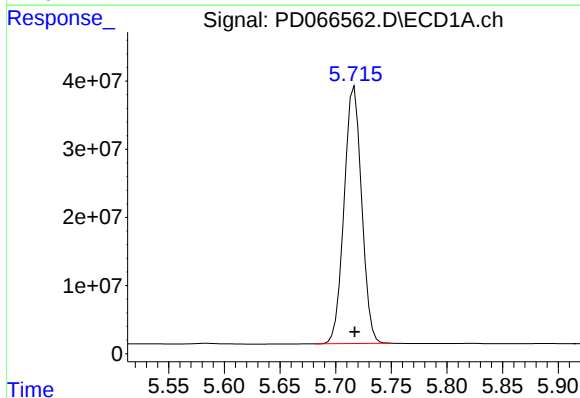


#13 Dieldrin

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 413730179
Conc: 166.17 ng/ml

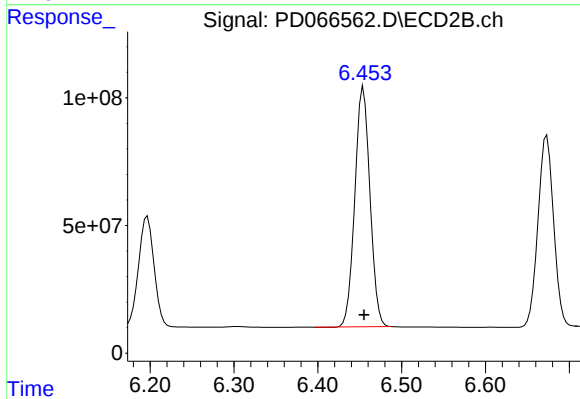

#13 Dieldrin


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 1179136270
Conc: 147.97 ng/ml

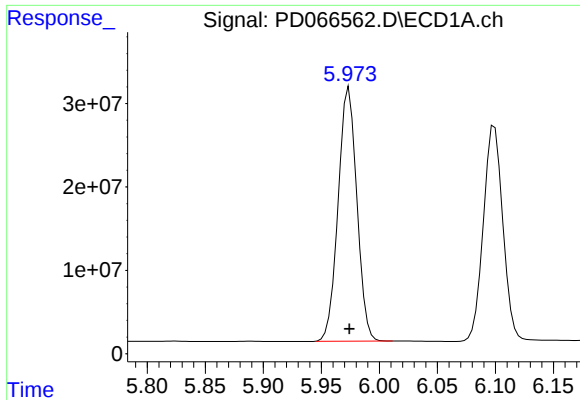

#14 Endrin


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 341887301
Conc: 161.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

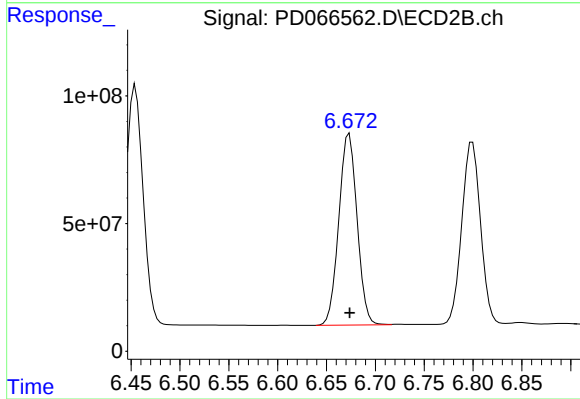


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 977590872
Conc: 143.50 ng/ml

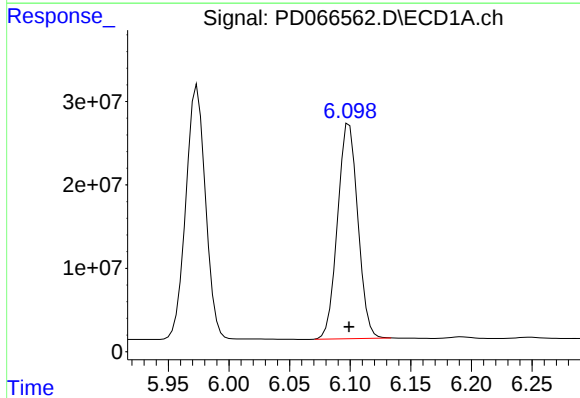


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 300378331
Conc: 165.35 ng/ml

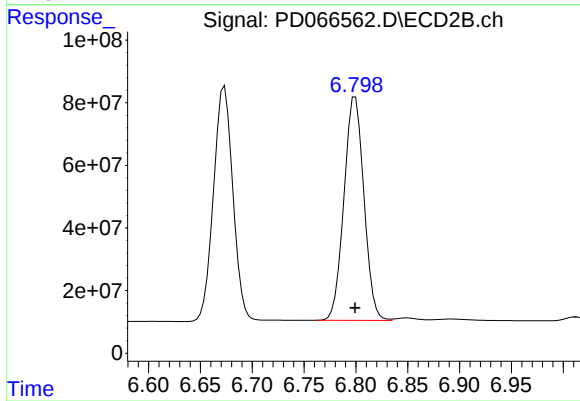

#16 4,4'-DDD


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 955886652
Conc: 147.52 ng/ml

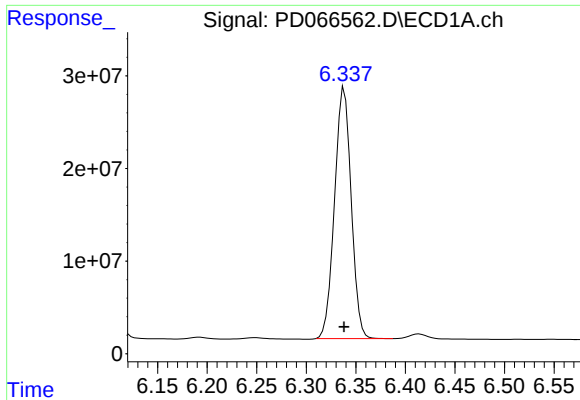

#17 4,4'-DDT


R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 316641517
Conc: 166.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

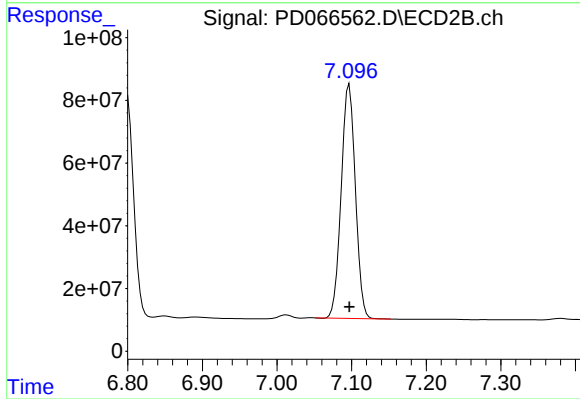


#17 4,4'-DDT

R.T.: 7.097 min
Delta R.T.: 0.000 min
Response: 983356236
Conc: 148.58 ng/ml

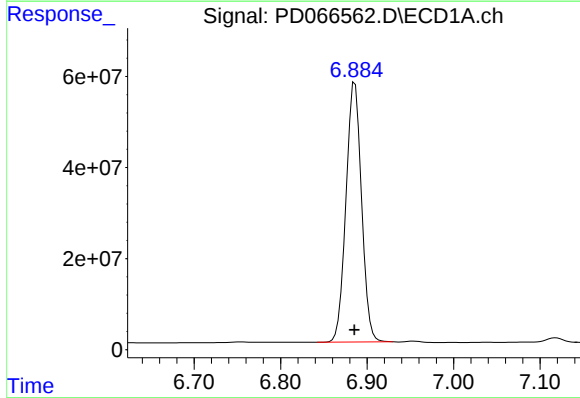


#20 Methoxychlor

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 709523839
Conc: 756.47 ng/ml

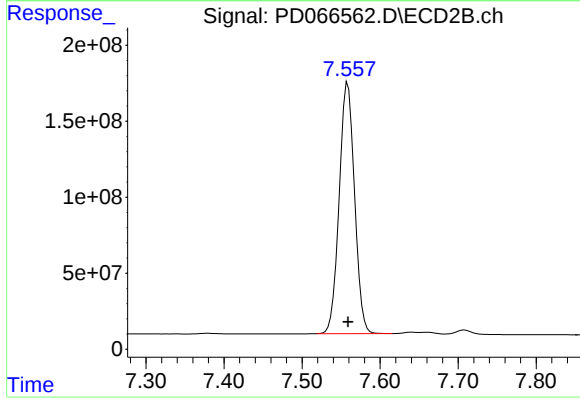

#20 Methoxychlor


R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 2257349216
Conc: 699.04 ng/ml

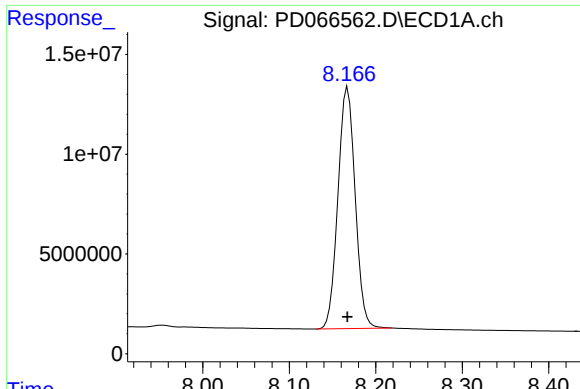

#27 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 166611530
Conc: 144.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

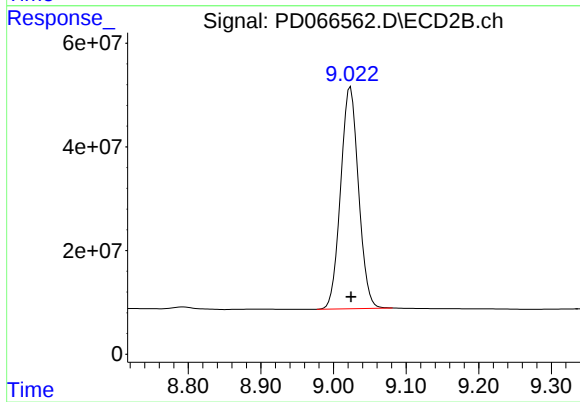

#27 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 732554609
Conc: 139.77 ng/ml