

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
 Data File : PD066547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 10:50
 Operator : AJ\MA
 Sample : RESC004
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC012

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 18:03:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	3.970	38438612	172.6E6	19.885	19.928
27)	SA Decachlor...	8.168	9.024	45831239	207.1E6	39.116	39.715
Target Compounds							
2)	A alpha-BHC	3.877	4.363	28319257	114.4E6	9.675	10.459
3)	MA gamma-BHC...	4.159	4.647	26779069	105.1E6	9.672	10.397
4)	MA Heptachlor	4.453	5.148	27896816	103.9E6	9.806	10.600
5)	MB Aldrin	4.698	5.451	28924307	100.4E6	10.046	10.658
6)	B beta-BHC	4.407	4.825	13633474	52795964	10.854	10.715
7)	B delta-BHC	4.609	5.039	25961254	102.6E6	9.795	10.371
8)	B Heptachlo...	5.139	5.839	25484884	75829692	10.026	10.087
9)	A Endosulfan I	5.476	6.197	22637412	82933112	9.876	10.599
10)	B trans-Chl...	5.363	6.074	25650337	90102806	9.924	10.463
11)	B cis-Chlor...	5.421	6.145	25349127	89192236	9.950	10.394
12)	B 4,4'-DDE	5.586	6.306	44885858	158.4E6	19.652	20.799
13)	MA Dieldrin	5.718	6.455	48280792	164.9E6	19.347	20.666
14)	MA Endrin	5.974	6.674	41699859	139.5E6	19.710	20.553
15)	B Endosulfa...	6.248	6.888	41333947	151.0E6	19.906	21.054
16)	A 4,4'-DDD	6.100	6.799	35211608	131.8E6	19.453	20.410
17)	MA 4,4'-DDT	6.339	7.096	35888814	135.5E6	18.981	20.515
18)	B Endrin al...	6.416	7.012	29066461	108.7E6	19.951	20.433
19)	B Endosulfa...	6.628	7.235	36779713	144.0E6	20.163	20.895
20)	A Methoxychlor	6.886	7.559	93829350	328.1E6	100.116	101.533
21)	B Endrin ke...	7.120	7.708	42949681	164.5E6	20.844	20.984

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 10:50
Operator : AJ\MA
Sample : RESC004
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 18:03:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

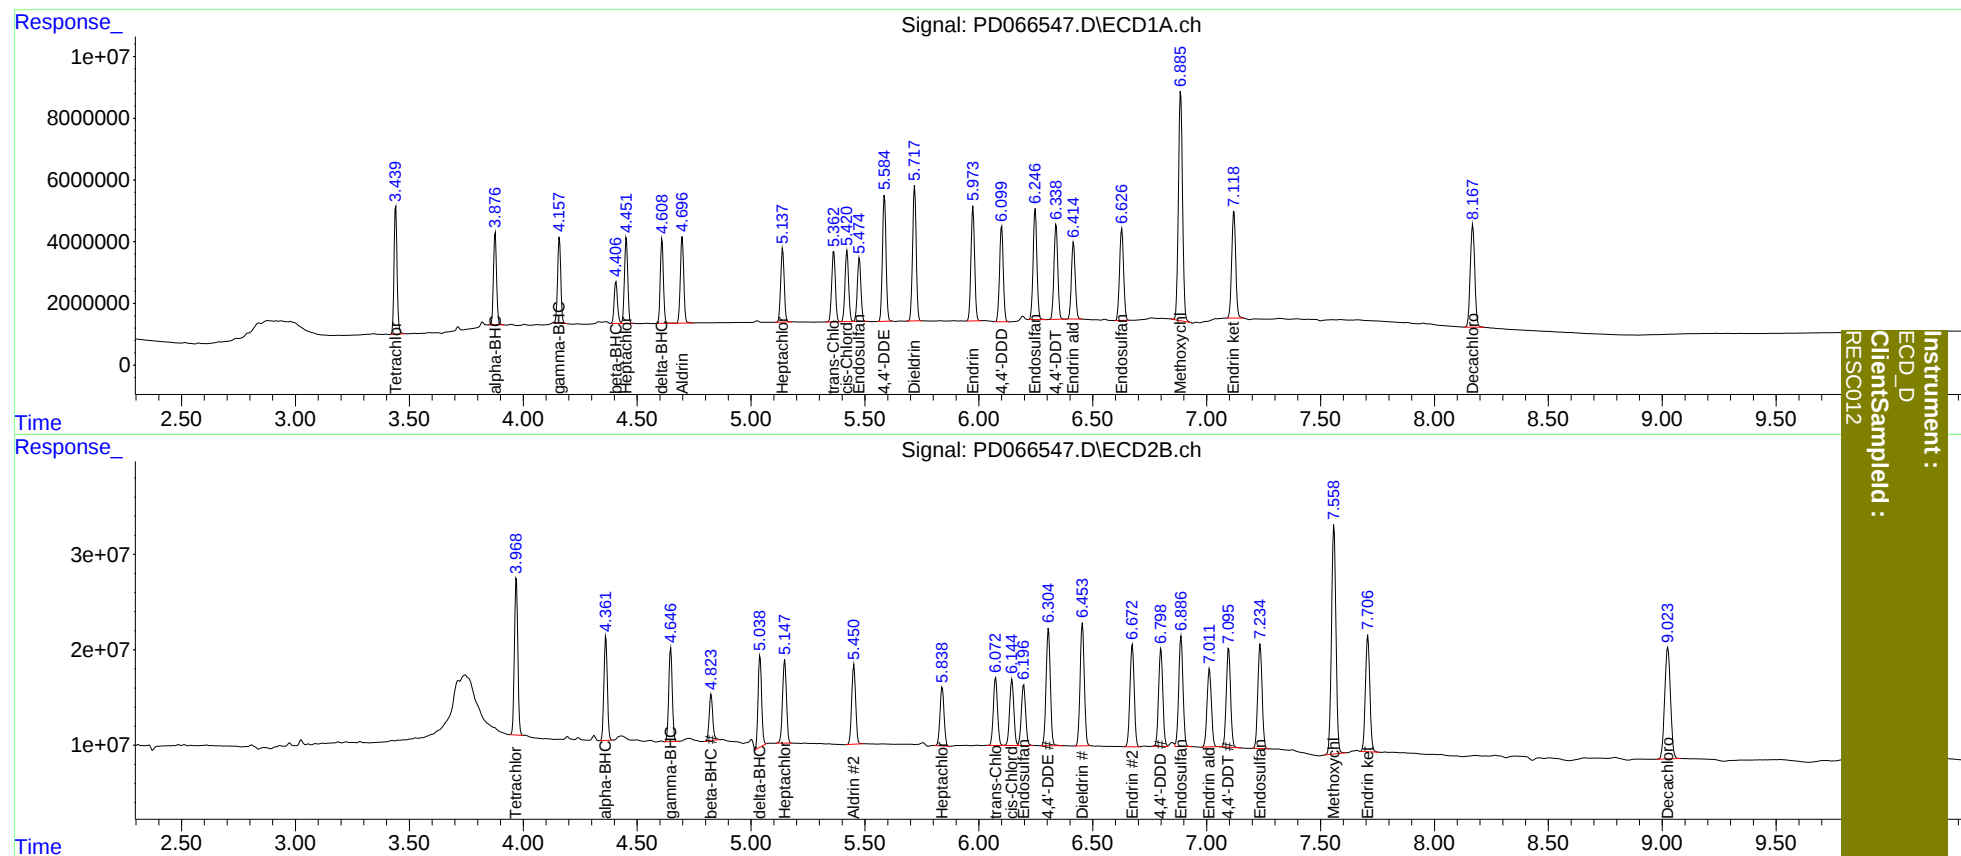

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066547.D
Acq On : 27 Oct 2021 10:50
Operator : AJ\MA
Sample : RESC004
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Title : GC Extractables
Last Update : Wed Oct 27 16:50:52 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.440	3.877	100.00%
3.877	4.159	100.00%
4.159	4.407	100.00%
4.407	4.453	98.70%
4.453	4.609	100.00%
4.609	4.698	100.00%
4.698	5.139	100.00%
5.139	5.363	100.00%
5.363	5.421	100.00%
5.421	5.476	100.00%
5.476	5.586	100.00%
5.586	5.718	100.00%
5.718	5.974	100.00%
5.974	6.100	100.00%
6.100	6.248	100.00%
6.248	6.339	100.00%
6.339	6.416	100.00%
6.416	6.628	100.00%
6.628	6.886	100.00%
6.886	7.120	100.00%
7.120	8.168	100.00%

Signal #2


3.970	4.363	100.00%
4.363	4.647	100.00%
4.647	4.825	100.00%
4.825	5.039	100.00%
5.039	5.148	100.00%
5.148	5.451	100.00%
5.451	5.839	100.00%
5.839	6.074	100.00%
6.074	6.145	100.00%
6.145	6.197	97.97%
6.197	6.306	100.00%
6.306	6.455	100.00%
6.455	6.674	100.00%
6.674	6.799	100.00%
6.799	6.888	100.00%
6.888	7.012	100.00%
7.012	7.096	100.00%
7.096	7.235	100.00%
7.235	7.559	100.00%
7.559	7.708	100.00%
7.708	9.024	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 10:50
Operator : AJ\MA
Sample : RESC004
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 18:03:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

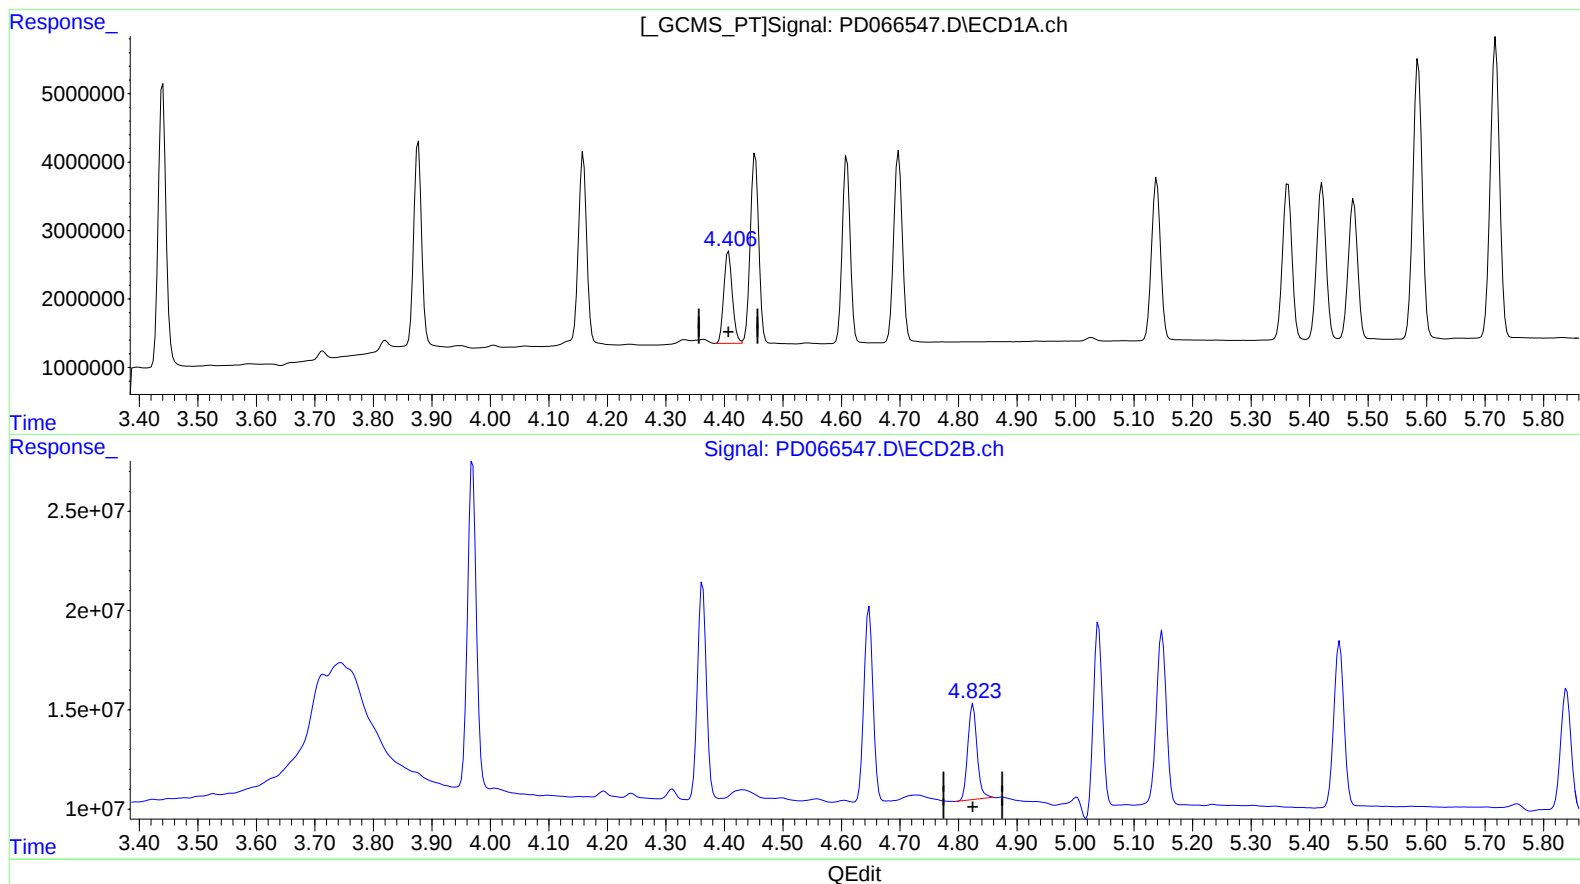

(6) beta-BHC (B)

4.407min 10.854 ng/ml

response 13633474

(6) beta-BHC #2 (B)

4.825min 10.715 ng/ml


response 52795964

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102721\
Data File : PD066547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 10:50
Operator : AJ\MA
Sample : RESC004
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 18:03:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

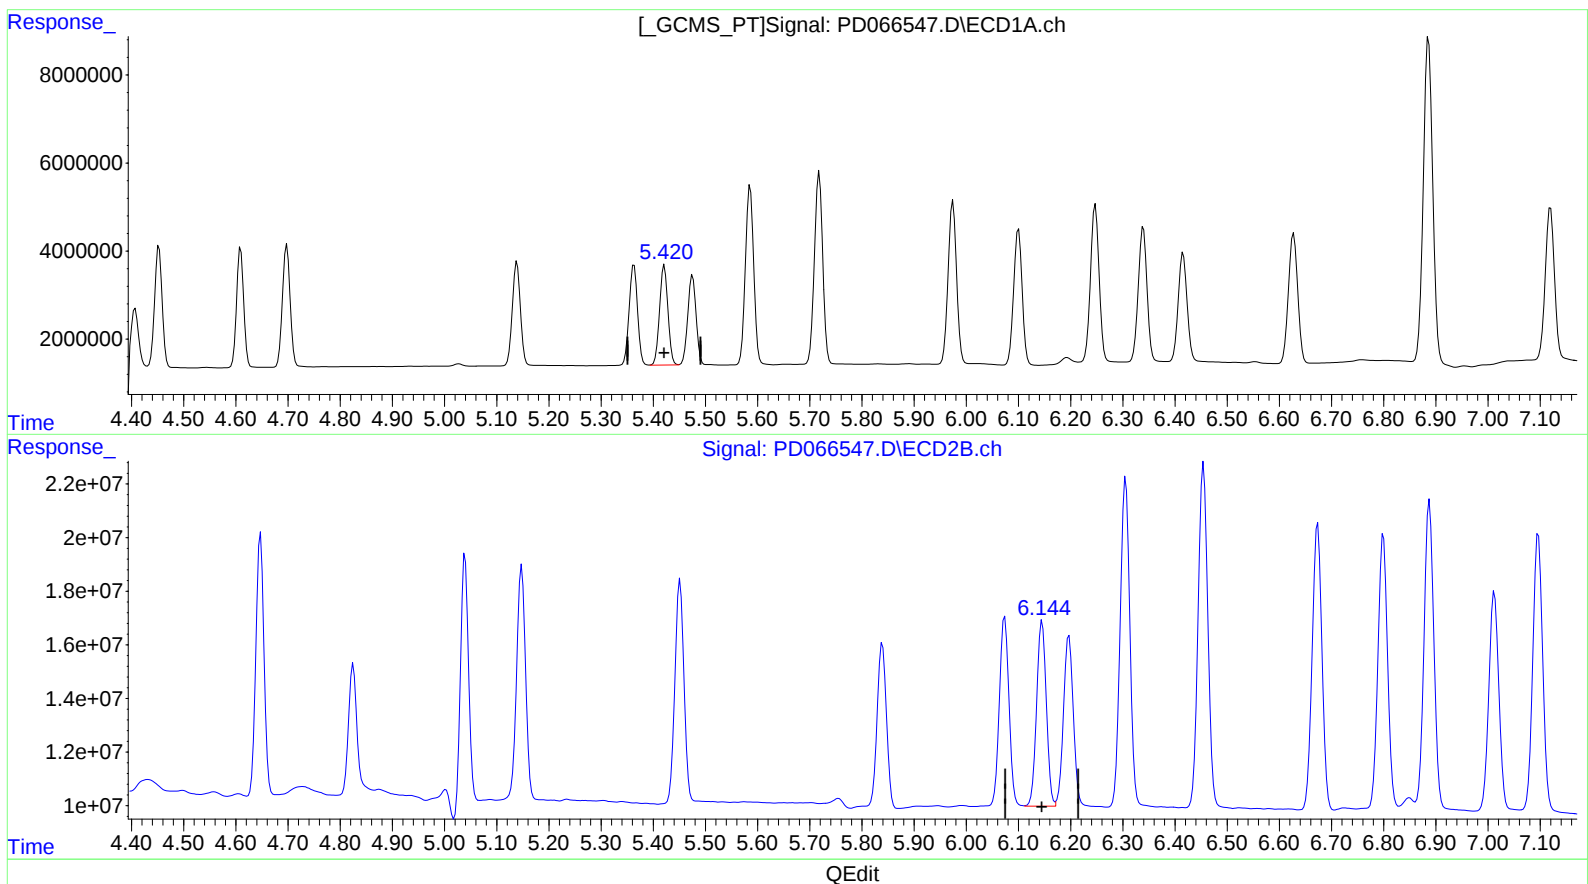

(11) cis-Chlordane (B)

5.421min 9.950 ng/ml

response 25349127

(11) cis-Chlordane #2 (B)

6.145min 10.394 ng/ml

response 89192236