

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
 Data File : PD079197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 11:36
 Operator : AR\AJ
 Sample : PB156257BL
 Misc : WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB156257BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:06:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	30247086	45501925	18.734	19.653
28)	SA Decachlor...	9.116	7.955	39471465	50792886	19.676	20.838

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
Data File : PD079197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 11:36
Operator : AR\AJ
Sample : PB156257BL
Misc : WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB156257BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:06:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

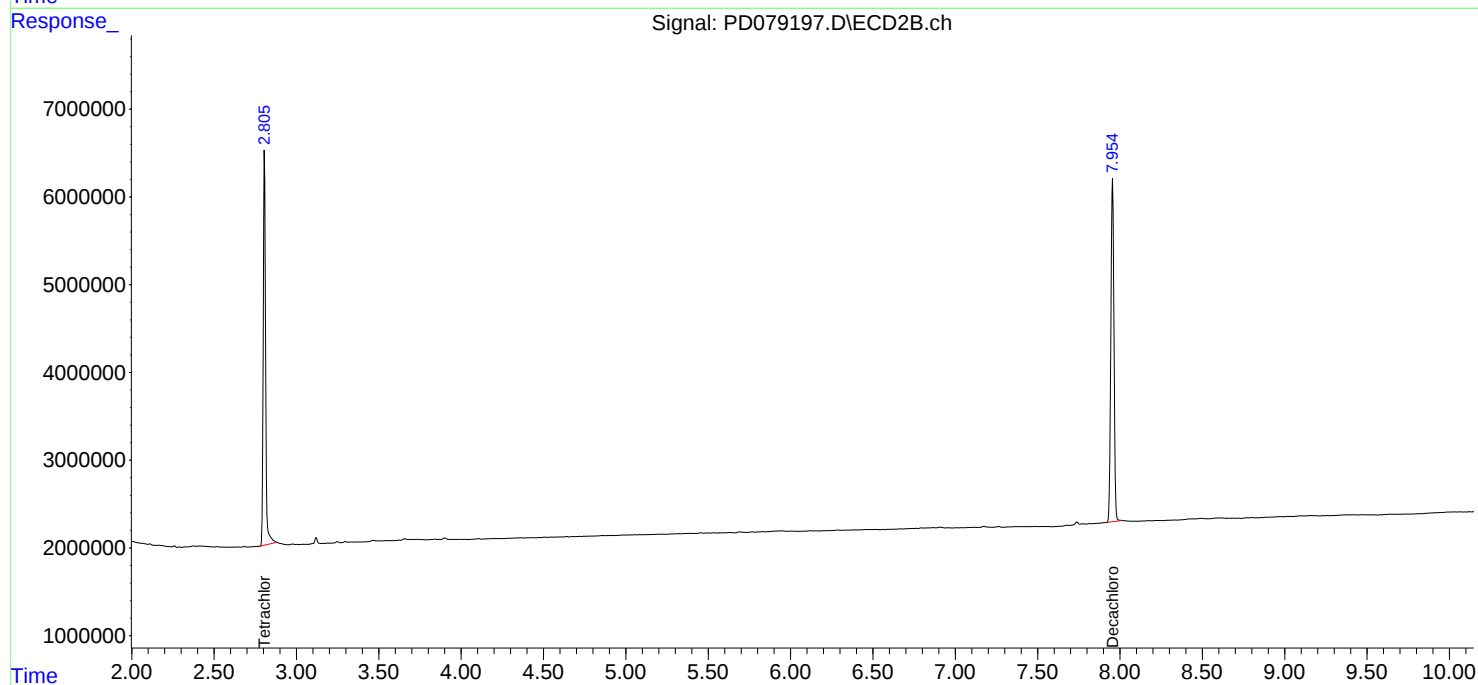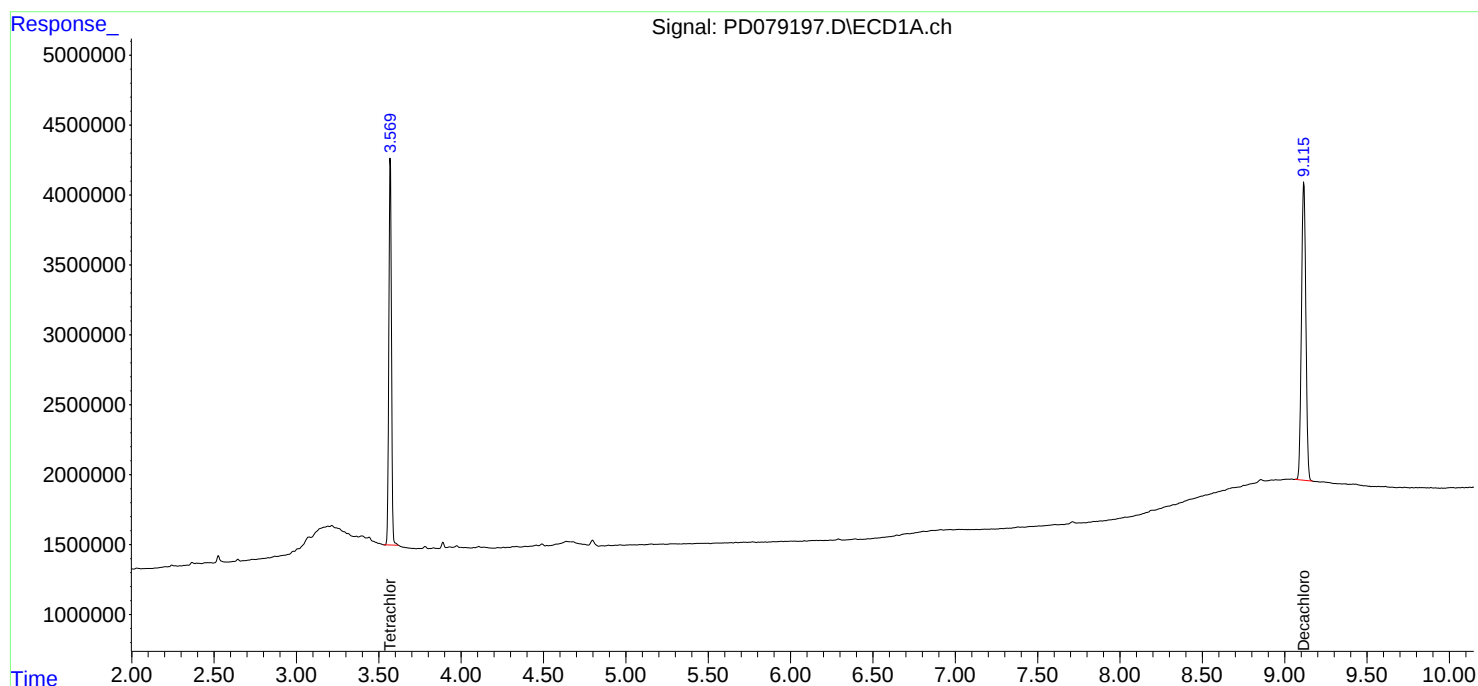


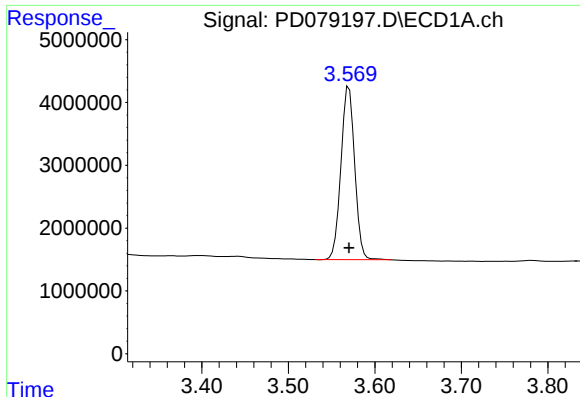

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 30247086
Conc: 18.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB156257BL

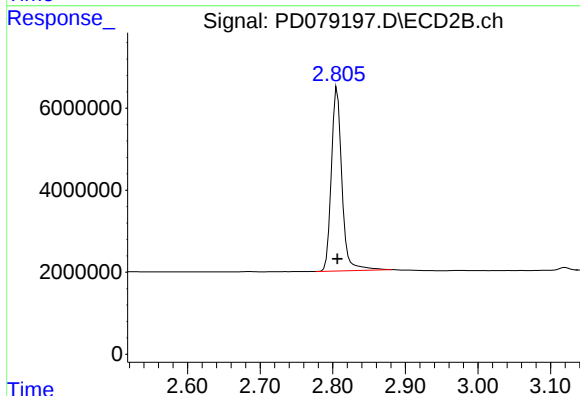


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 45501925
Conc: 19.65 ng/ml

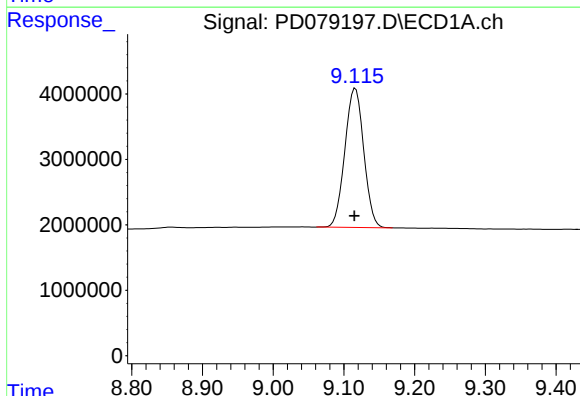

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.002 min
Response: 39471465
Conc: 19.68 ng/ml

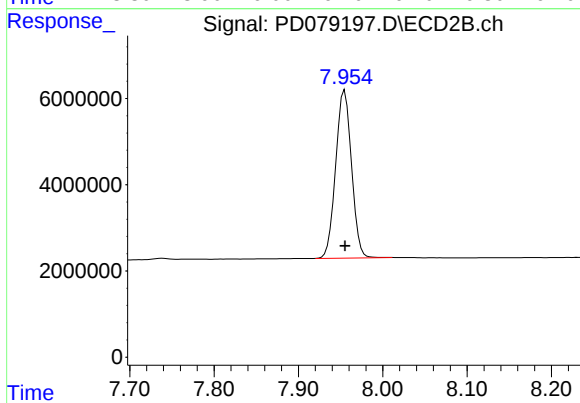

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 50792886
Conc: 20.84 ng/ml