

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
 Data File : PD079201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 12:30
 Operator : AR\AJ
 Sample : 04699-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:07:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.806	26728392	40943356	16.554	17.684
28)	SA Decachlor...	9.117	7.954	35454279	45262829	17.674	18.569
Target Compounds							
23)	Chlordane-1	4.738	3.808	1993881	2222608	25.645	25.590
24)	Chlordane-2	5.268	4.386	2327034	2571483	29.151	28.302
25)	Chlordane-3	5.980	5.017	8267287	6872639	26.668	25.766
26)	Chlordane-4	6.062	5.080	10267685	6555292	27.637	26.715
27)	Chlordane-5	6.913	5.975	1828193	2636104	26.018	26.450



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
Data File : PD079201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 12:30
Operator : AR\AJ
Sample : 04699-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:07:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

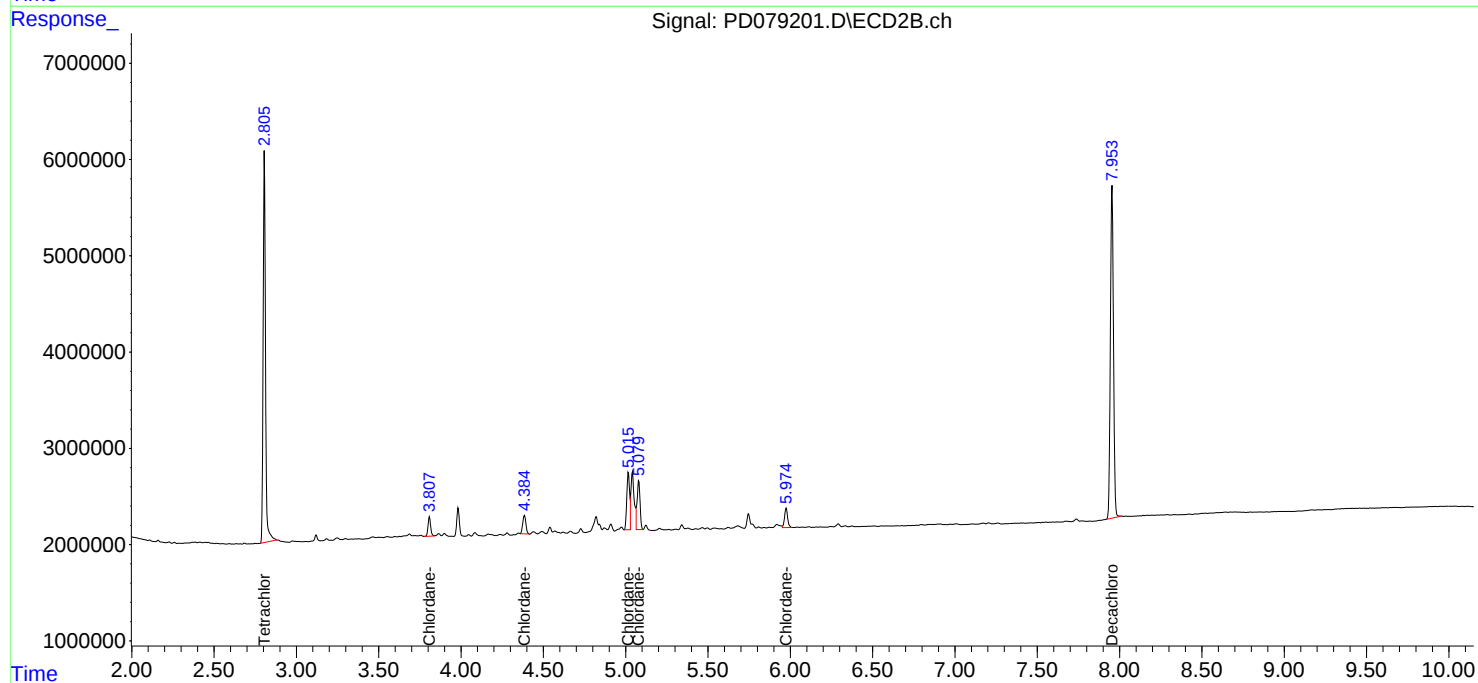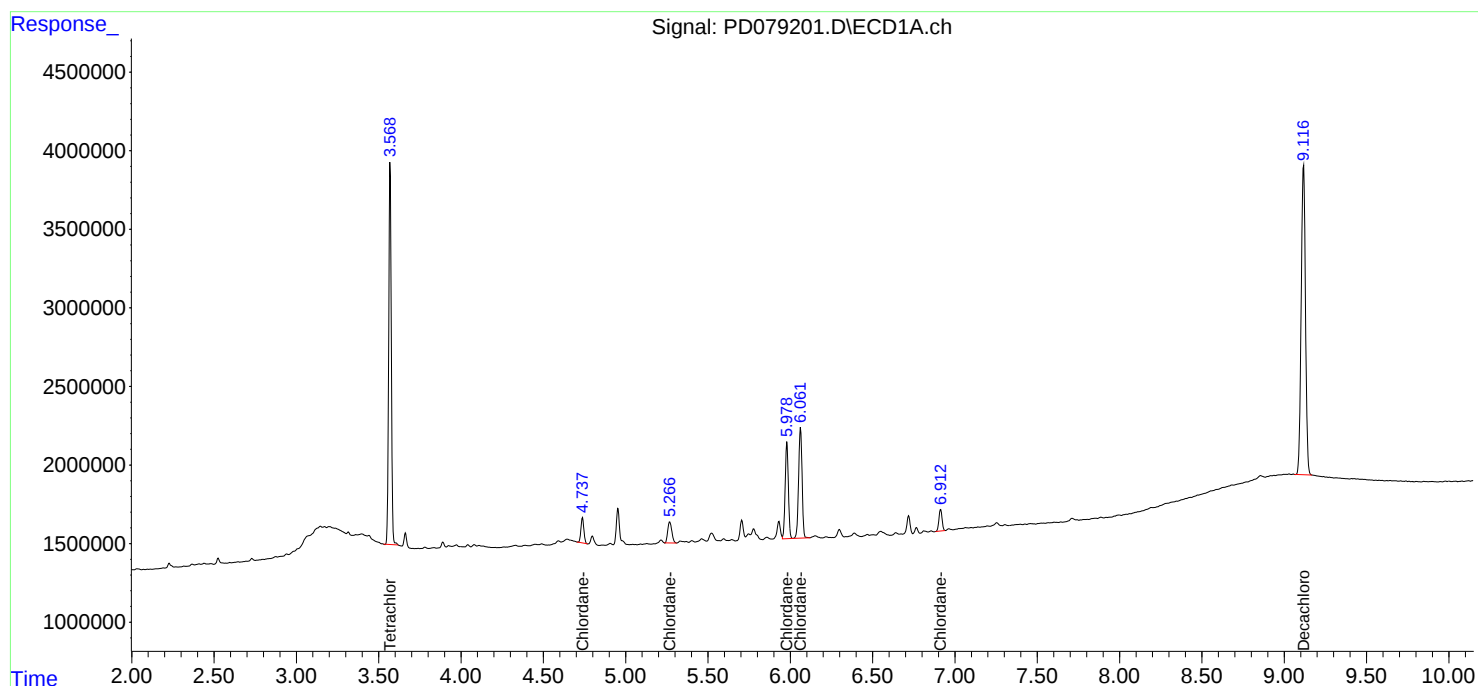


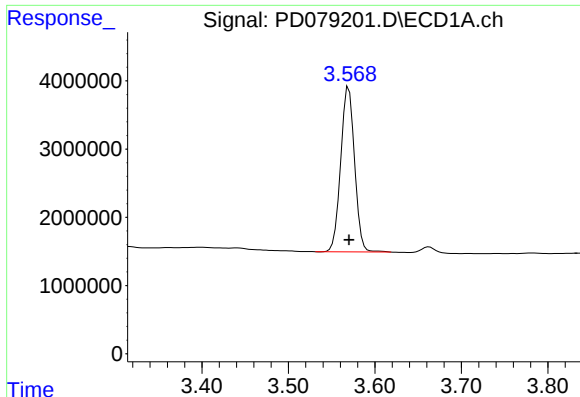

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 26728392
Conc: 16.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT4-2023

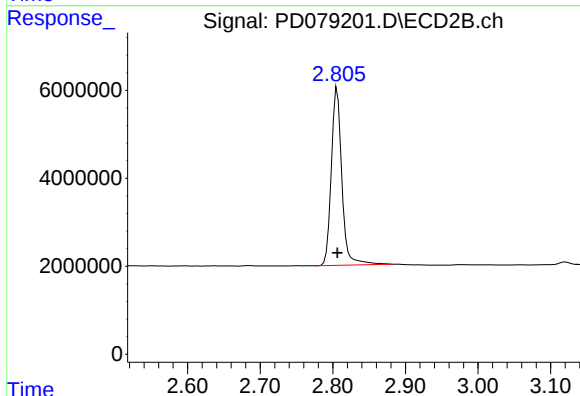


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 40943356
Conc: 17.68 ng/ml

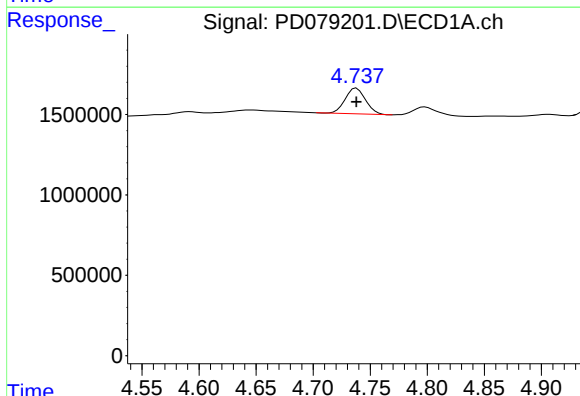


#23 Chlordane-1

R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 1993881
Conc: 25.65 ng/ml

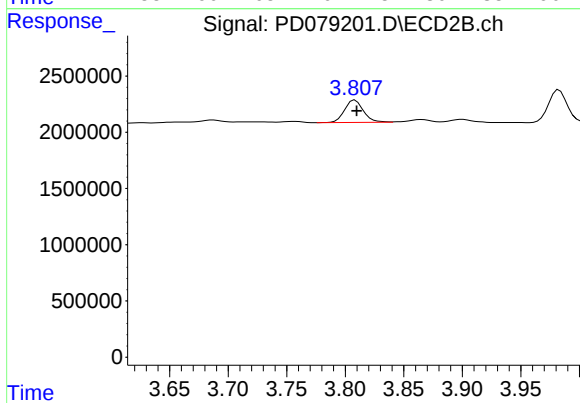

#23 Chlordane-1


R.T.: 3.808 min
Delta R.T.: -0.001 min
Response: 2222608
Conc: 25.59 ng/ml

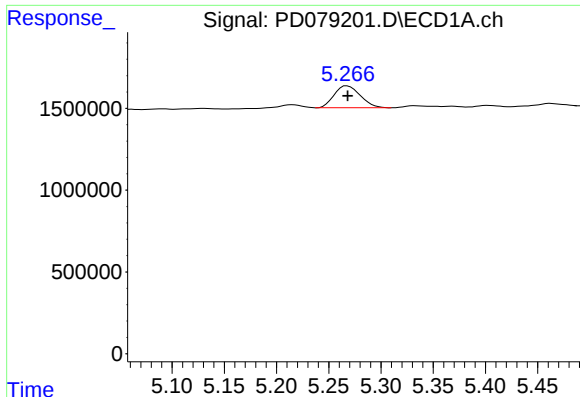

#24 Chlordane-2


R.T.: 5.268 min
Delta R.T.: 0.000 min
Response: 2327034
Conc: 29.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT4-2023

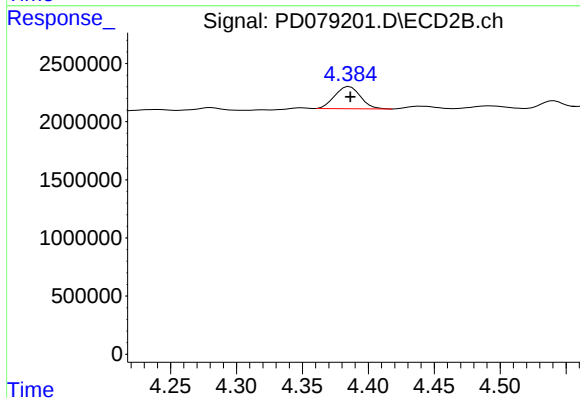


#24 Chlordane-2

R.T.: 4.386 min
Delta R.T.: 0.000 min
Response: 2571483
Conc: 28.30 ng/ml

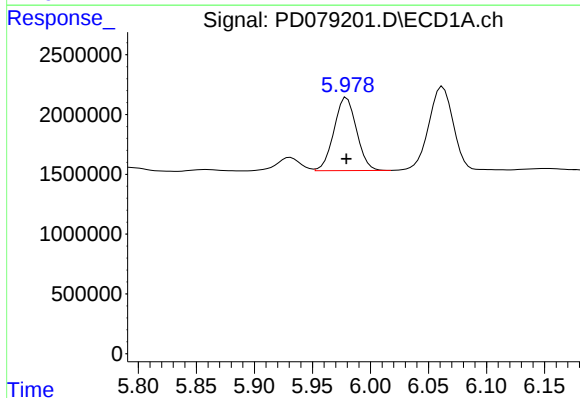


#25 Chlordane-3

R.T.: 5.980 min
Delta R.T.: 0.000 min
Response: 8267287
Conc: 26.67 ng/ml

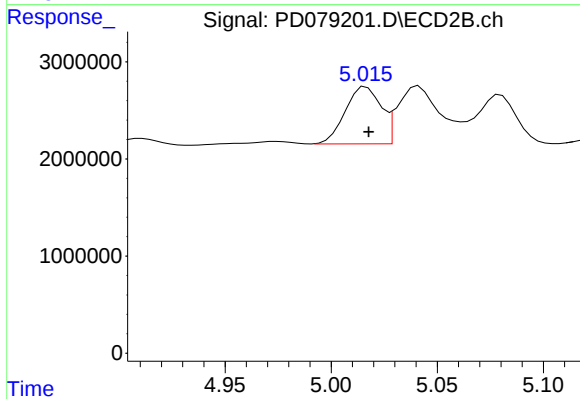

#25 Chlordane-3


R.T.: 5.017 min
Delta R.T.: -0.001 min
Response: 6872639
Conc: 25.77 ng/ml

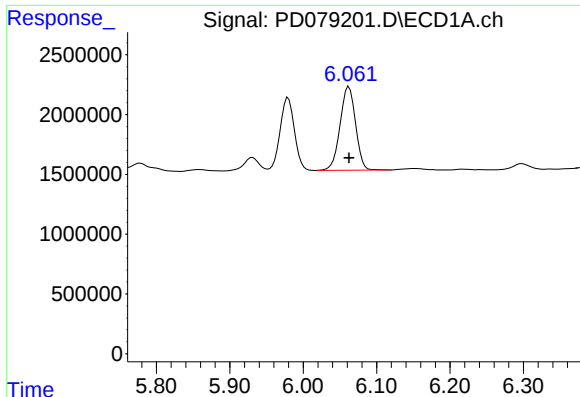

#26 Chlordane-4


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 10267685
Conc: 27.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT4-2023

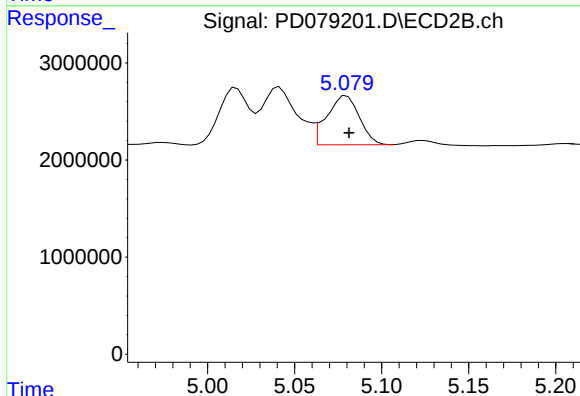


#26 Chlordane-4

R.T.: 5.080 min
Delta R.T.: -0.001 min
Response: 6555292
Conc: 26.71 ng/ml

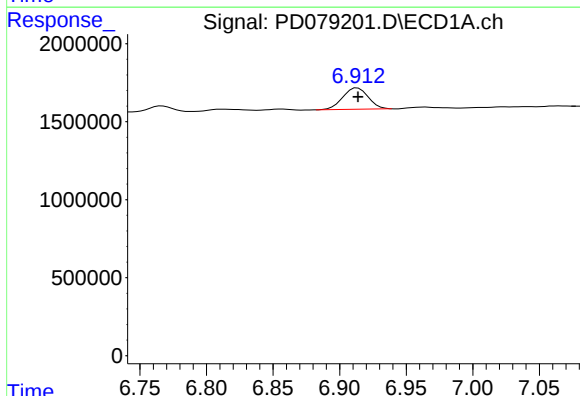


#27 Chlordane-5

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 1828193
Conc: 26.02 ng/ml

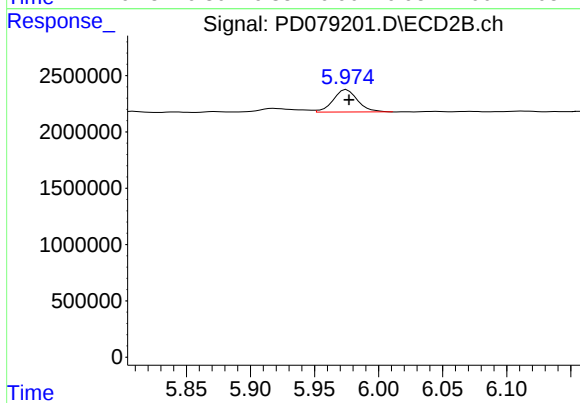

#27 Chlordane-5


R.T.: 5.975 min
Delta R.T.: -0.002 min
Response: 2636104
Conc: 26.45 ng/ml

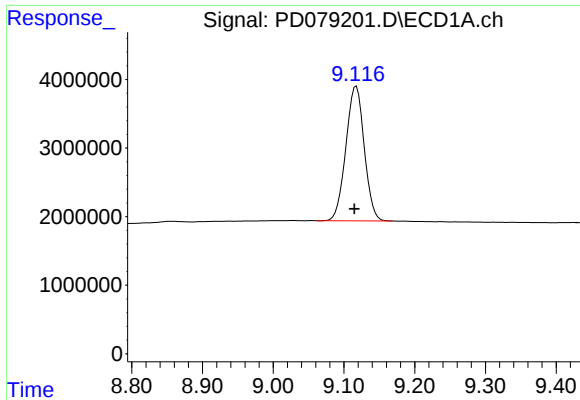

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.003 min
Response: 35454279
Conc: 17.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT4-2023

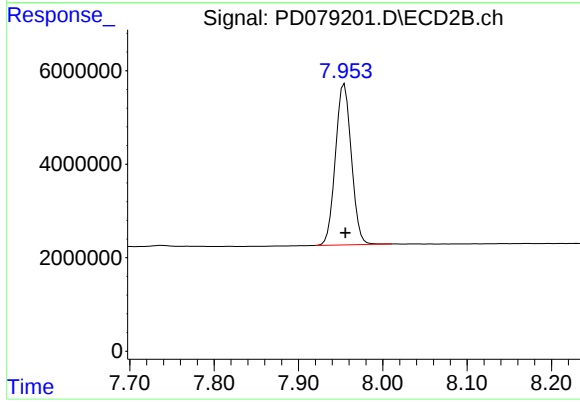

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.000 min
Response: 45262829
Conc: 18.57 ng/ml