

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
 Data File : PD079216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 17:22
 Operator : AR\AJ
 Sample : 05092-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CHRT-25651

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/30/2023
 Supervised By : mohammad ahmed 10/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 22:11:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 20 04:44:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.807	13502456	21146116	8.363m	9.133
28) SA Decachlor...	9.114	7.954	9764175	11914309	4.867	4.888

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102723\
Data File : PD079216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 17:22
Operator : AR\AJ
Sample : 05092-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CHRT-25651


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/30/2023
Supervised By : mohammad ahmed 10/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 22:11:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102023.M
Quant Title : GC Extractables
QLast Update : Fri Oct 20 04:44:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

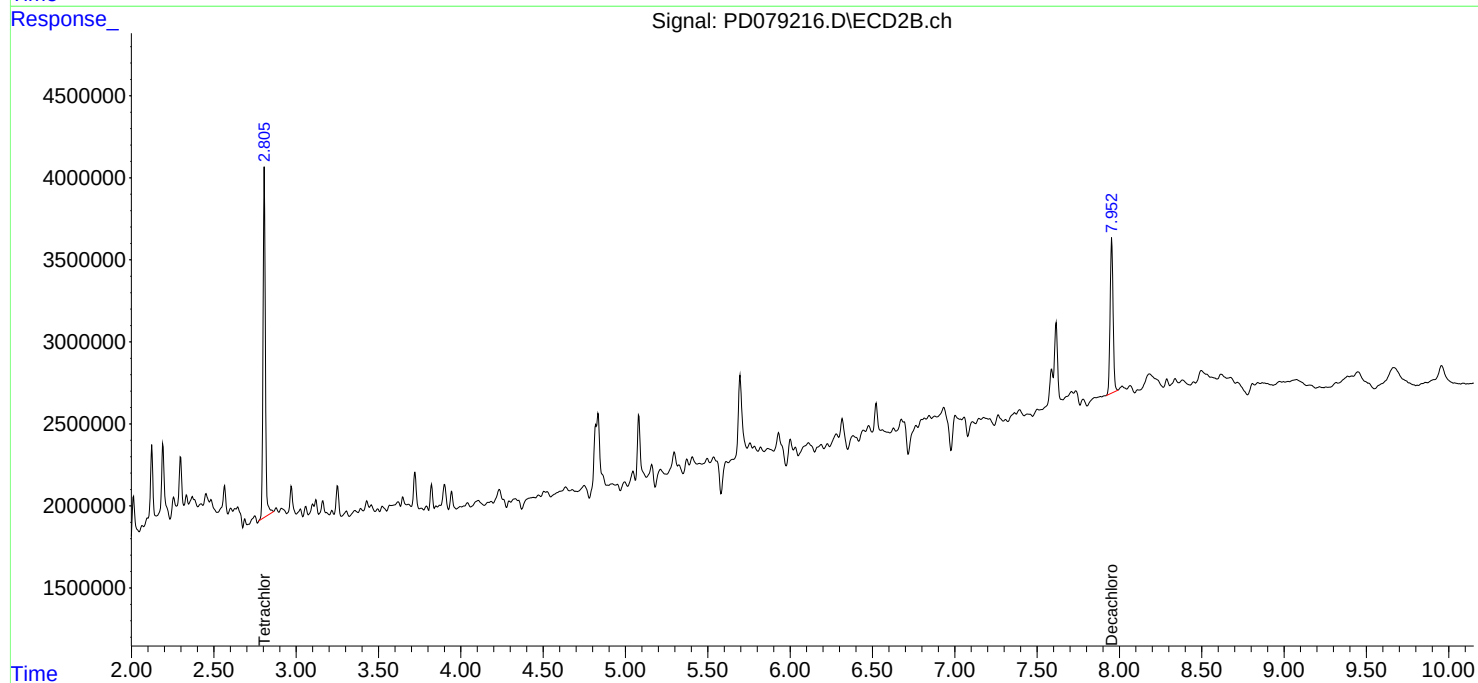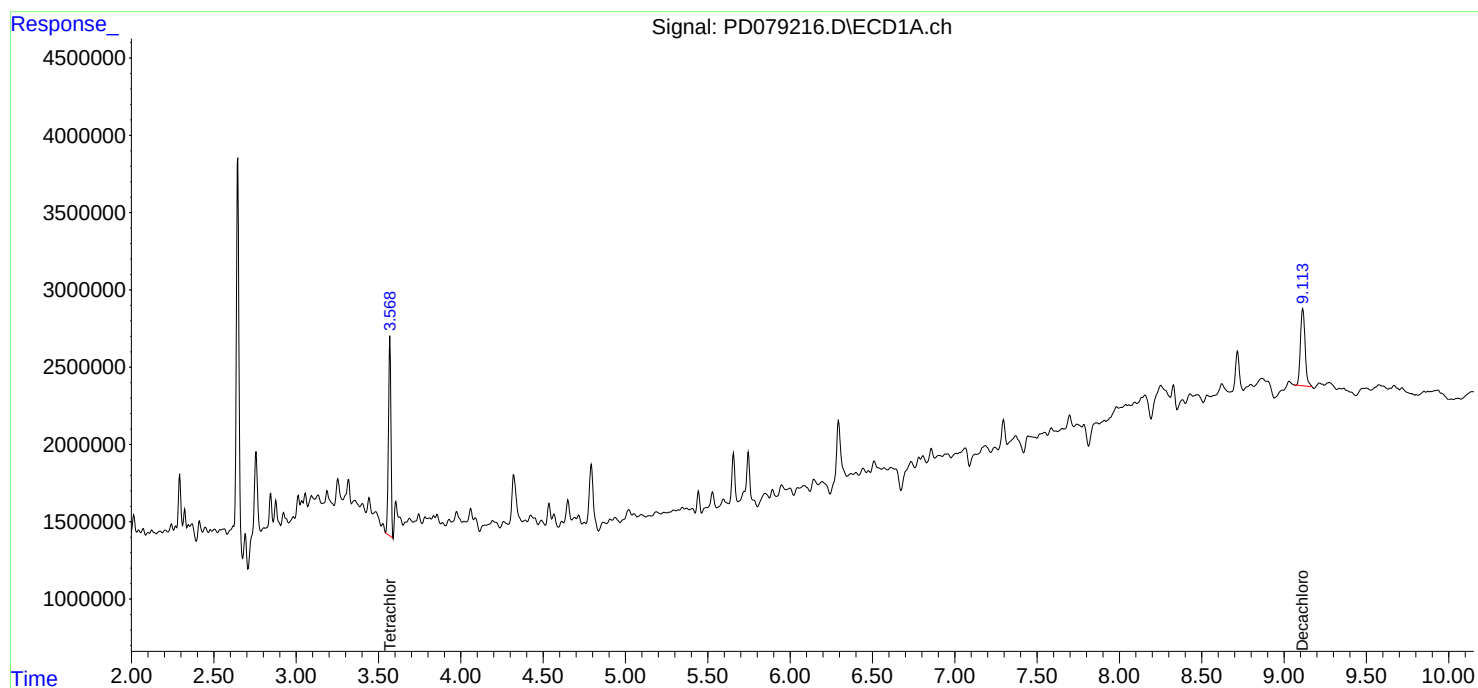

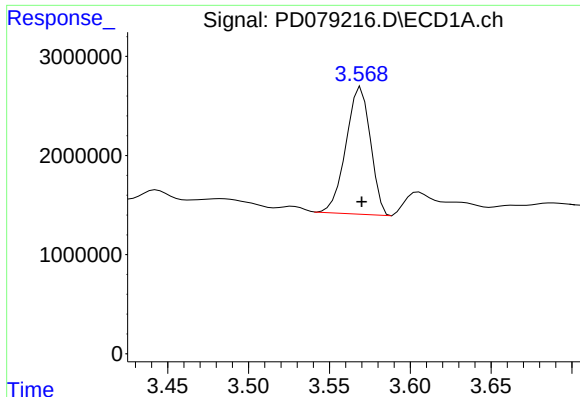


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.002 min
Response: 13502456
Conc: 8.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
CHRT-25651


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/30/2023
Supervised By :mohammad ahmed 10/30/2023

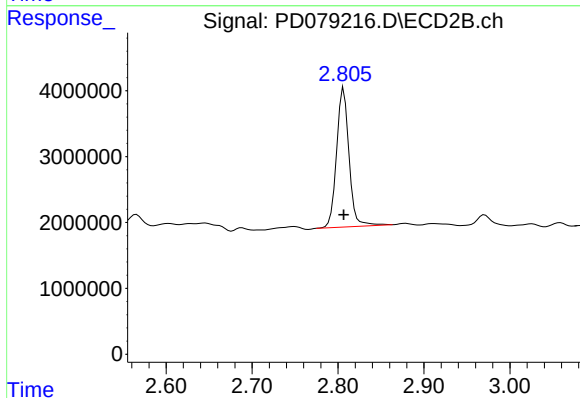


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 21146116
Conc: 9.13 ng/ml

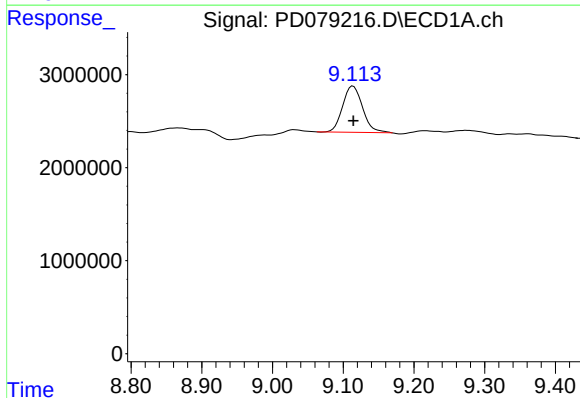

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.000 min
Response: 9764175
Conc: 4.87 ng/ml

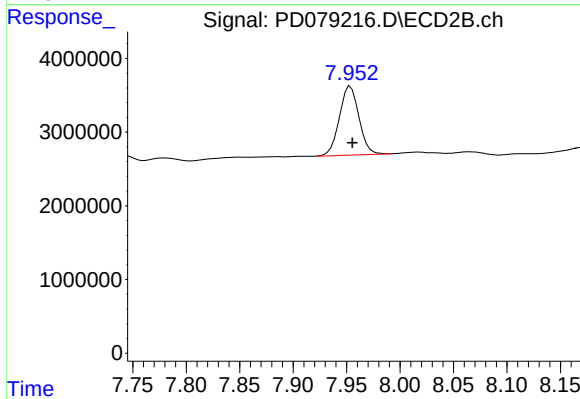

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: -0.002 min
Response: 11914309
Conc: 4.89 ng/ml