

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102725\
 Data File : PD090863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 21:32
 Operator : AR\AJ
 Sample : Q3447-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P001-TW4-251023-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/28/2025
 Supervised By : mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:14:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 17 17:43:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.872	55142778	517.5E6	17.707m	17.380m
28) SA Decachlor...	9.061	8.058	86876446	588.1E6	18.571	19.416

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102725\
Data File : PD090863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 21:32
Operator : AR\AJ
Sample : Q3447-08
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
P001-TW4-251023-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/28/2025
Supervised By : mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:14:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101725.M
Quant Title : GC Extractables
QLast Update : Fri Oct 17 17:43:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

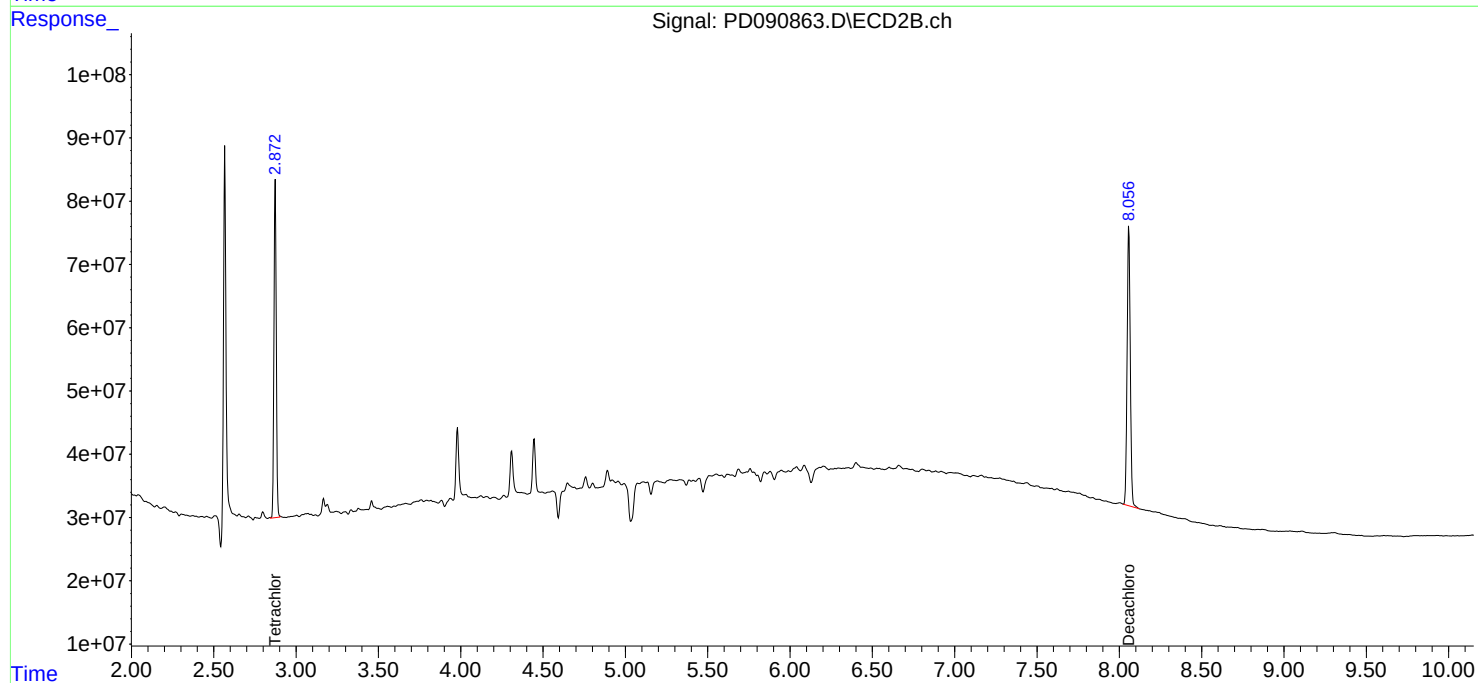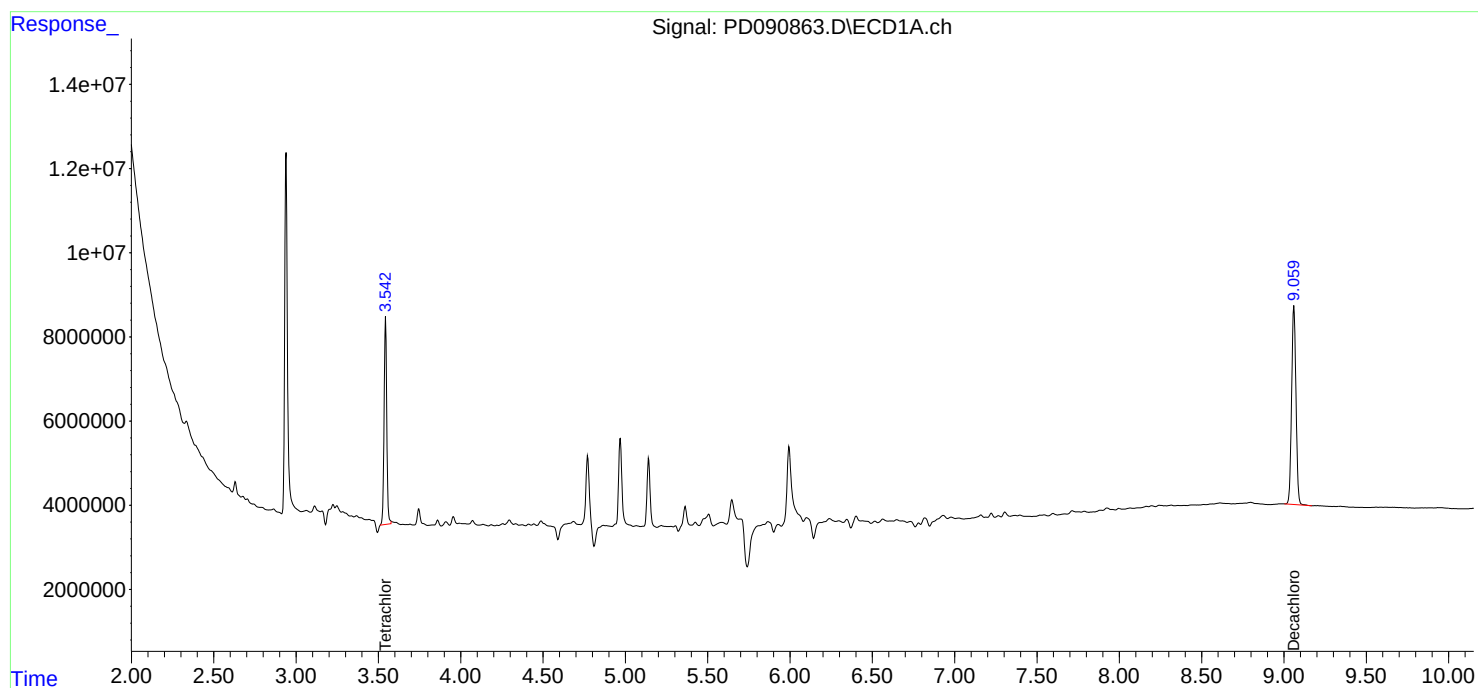

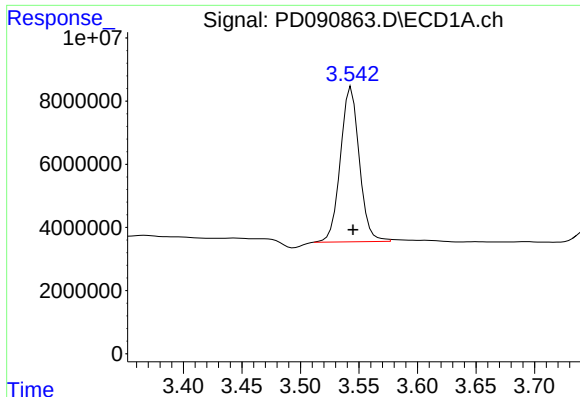

#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.003 min
Response: 55142778
Conc: 17.71 ng/ml

Instrument :

ECD_D


ClientSampleId :

P001-TW4-251023-01

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

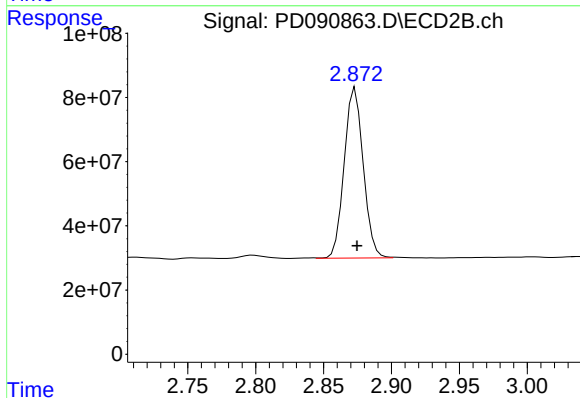


#1 Tetrachloro-m-xylene

R.T.: 2.872 min
Delta R.T.: -0.003 min
Response: 517514858
Conc: 17.38 ng/ml m

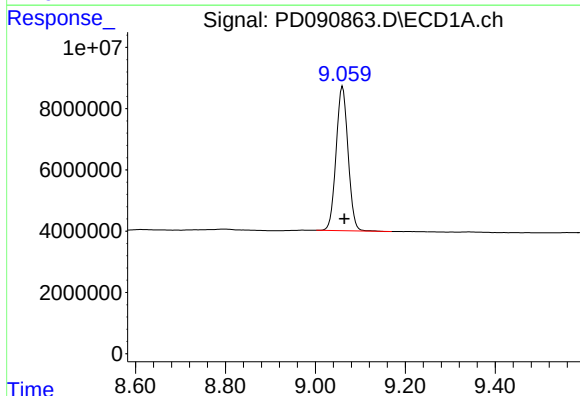

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.004 min
Response: 86876446
Conc: 18.57 ng/ml

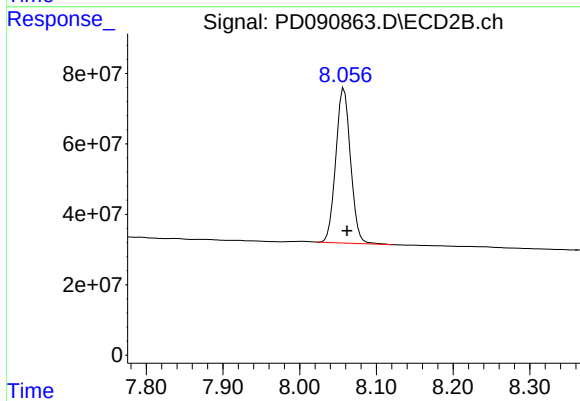

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: -0.004 min
Response: 588137712
Conc: 19.42 ng/ml