

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102819\
Data File : PD055617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 11:58
Operator : SG\AJ
Sample : K5433-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
JLNFO

Manual Integrations
APPROVED

Ankita
10/31/2019 9:26:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:40:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

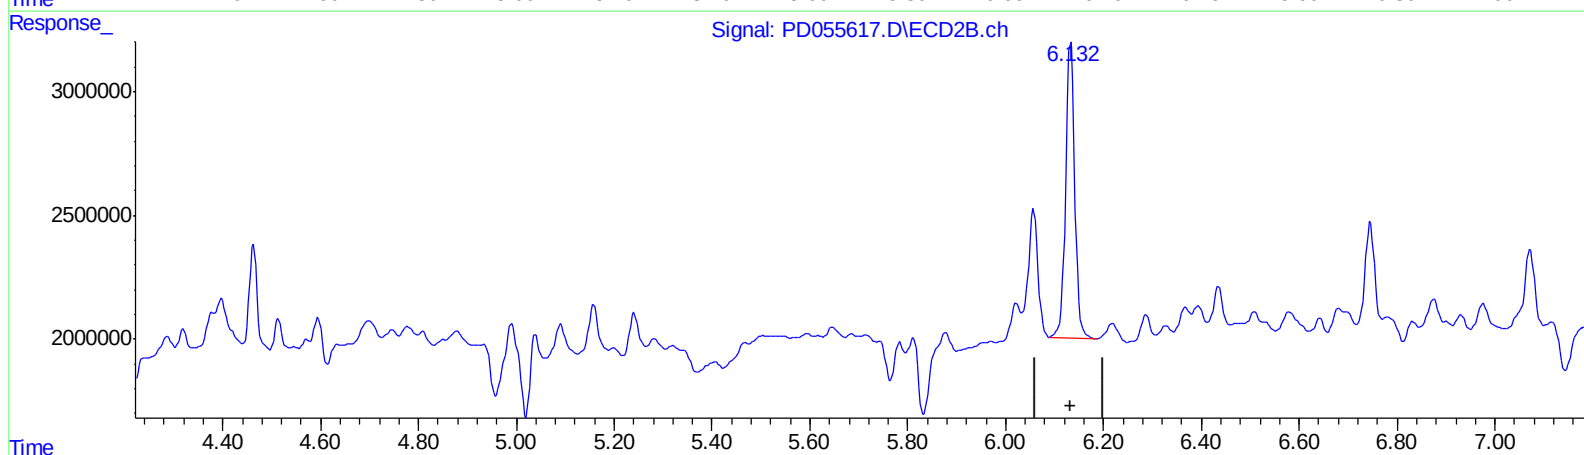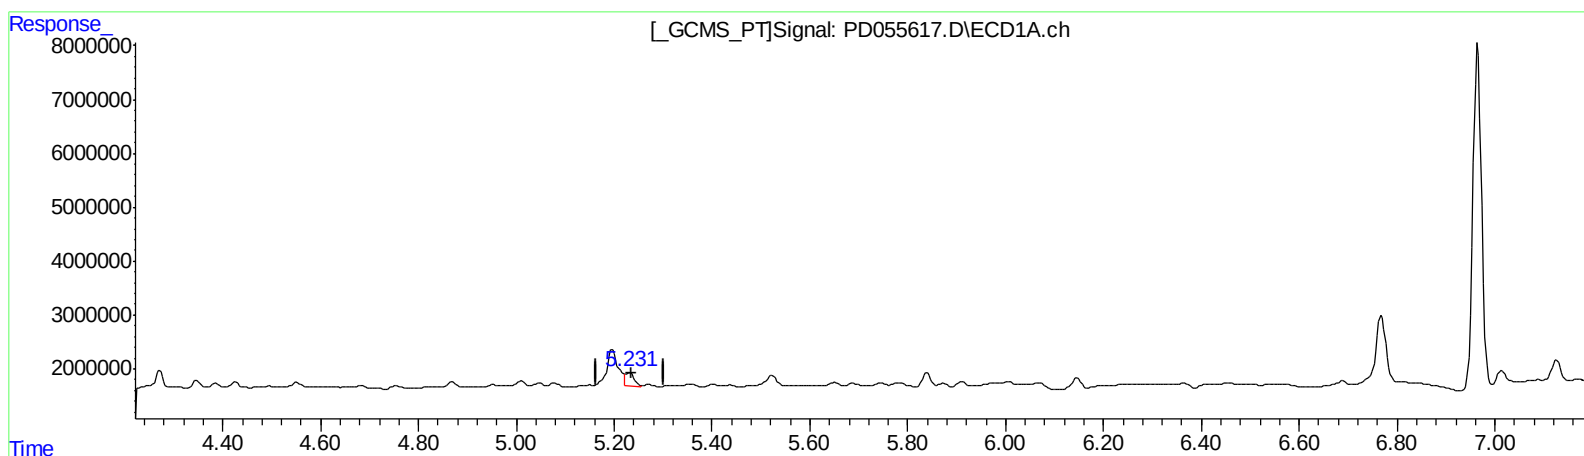

QEdit

(11) cis-Chlordane (B)

5.231min 3.018 ng/ml m

response 3031603

(11) cis-Chlordane #2 (B)

6.133min 9.132 ng/ml

response 15699737

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102819\
Data File : PD055617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 11:58
Operator : SG\AJ
Sample : K5433-03
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
JLNFO

Manual Integrations
APPROVED

Ankita
10/31/2019 9:26:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:58:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

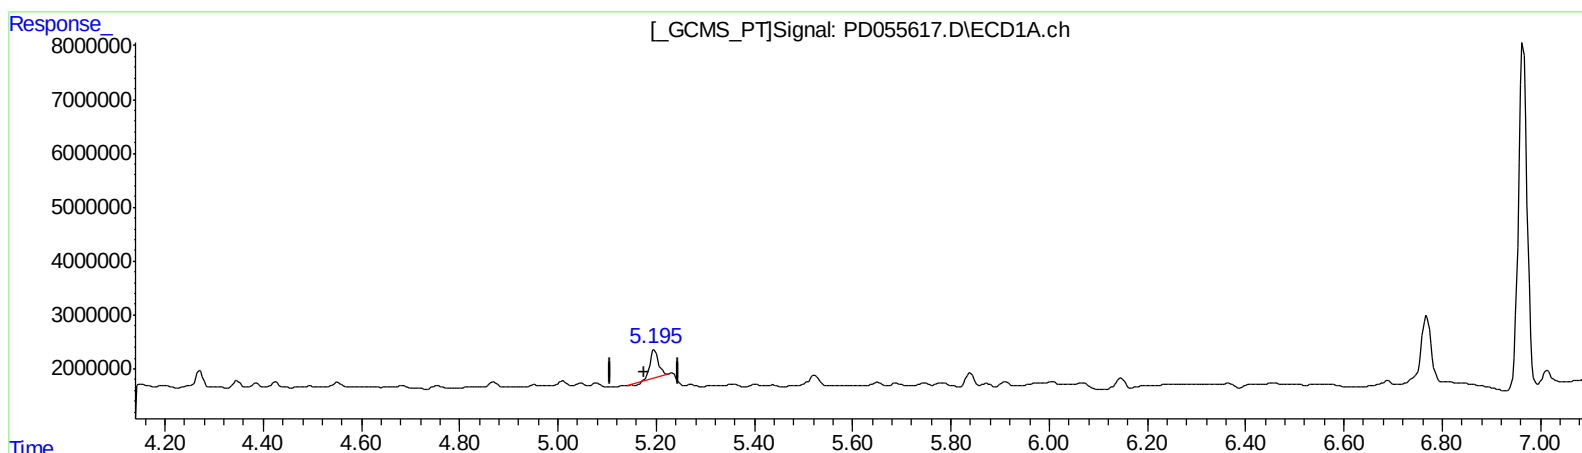

(10) trans-Chlordane (B)

5.196min 5.858 ng/ml

response 6057069

(10) trans-Chlordane #2 (B)

6.058min 3.050 ng/ml

response 5371820

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102819\
Data File : PD055617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 11:58
Operator : SG\AJ
Sample : K5433-03
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
JLNFO

Manual Integrations
APPROVED

Ankita
10/31/2019 9:26:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:40:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
Quant Title : GC Extractables
QLast Update : Sat Oct 19 00:42:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

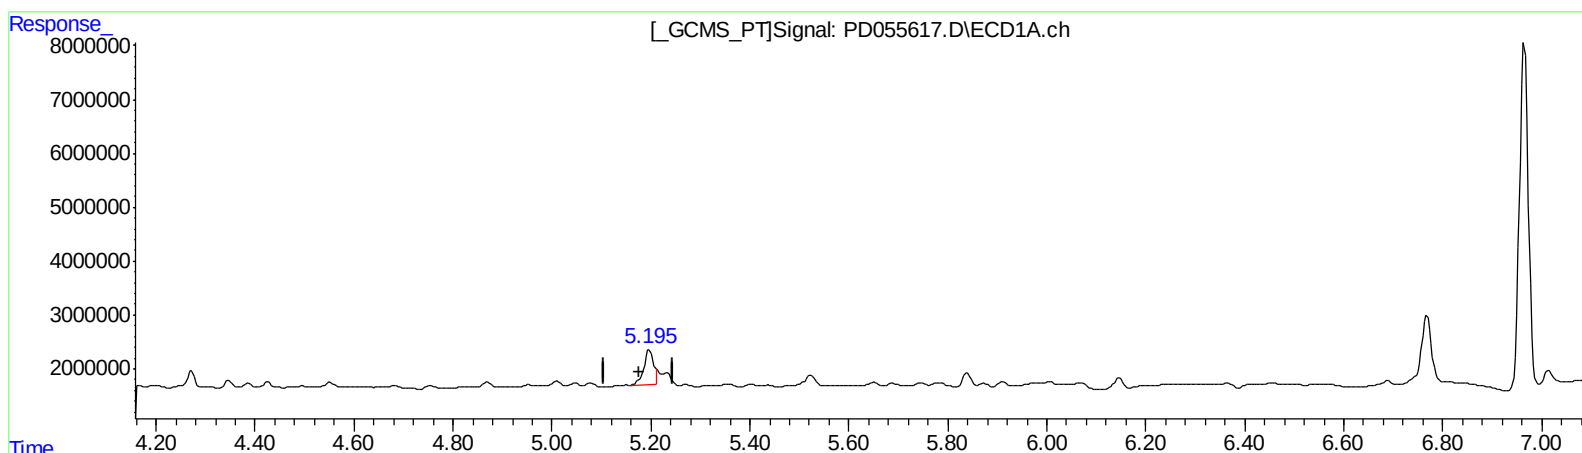

(10) trans-Chlordane (B)

5.195min 8.838 ng/ml m

response 9137840

(10) trans-Chlordane #2 (B)

6.056min 4.604 ng/ml m

response 8108216

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102819\
 Data File : PD055617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 11:58
 Operator : SG\AJ
 Sample : K5433-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLNFO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:40:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101819CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 19 00:42:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Ankita
 10/31/2019 9:26:09 AM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.290	3.963	12874997	18025037	14.441	13.388
27) SA Decachlor...	7.960	8.998	437.8E6	26646527	478.164	20.422 #
Target Compounds						
10) B trans-Chl...	5.195	6.056	9137840	8108216	8.838m	4.604m#
11) B cis-Chlor...	5.231	6.133	3031603	15699737	3.018m	9.132 #
17) MA 4,4'-DDT	6.147	7.072	2517721	4332332	3.714	3.196

A-J
 11/02/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.