

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 16:43
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:51:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	10329906	26838394	10.456	10.178
27)	SA Decachlor...	8.307	9.110	26976926	45093112	21.374	20.865
Target Compounds							
2)	A alpha-BHC	3.949	4.415	15022635	39103404	10.343	10.096
3)	MA gamma-BHC...	4.235	4.701	14439961	35551371	10.433	10.045
4)	MA Heptachlor	4.543	5.213	14819430	35437569	10.272	10.239
9)	A Endosulfan I	5.584	6.265	12907858	28933872	10.414	10.275
13)	MA Dieldrin	5.830	6.522	27870042	62241930	20.480	20.115
14)	MA Endrin	6.089	6.740	23892923	52157175	20.692	20.134
16)	A 4,4'-DDD	6.214	6.859	22377003	48024166	20.684	20.096
17)	MA 4,4'-DDT	6.457	7.159	24005053	49842390	20.302	20.063
20)	A Methoxychlor	7.006	7.615	64500501	135.9E6	104.843	104.232

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 16:43
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:51:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

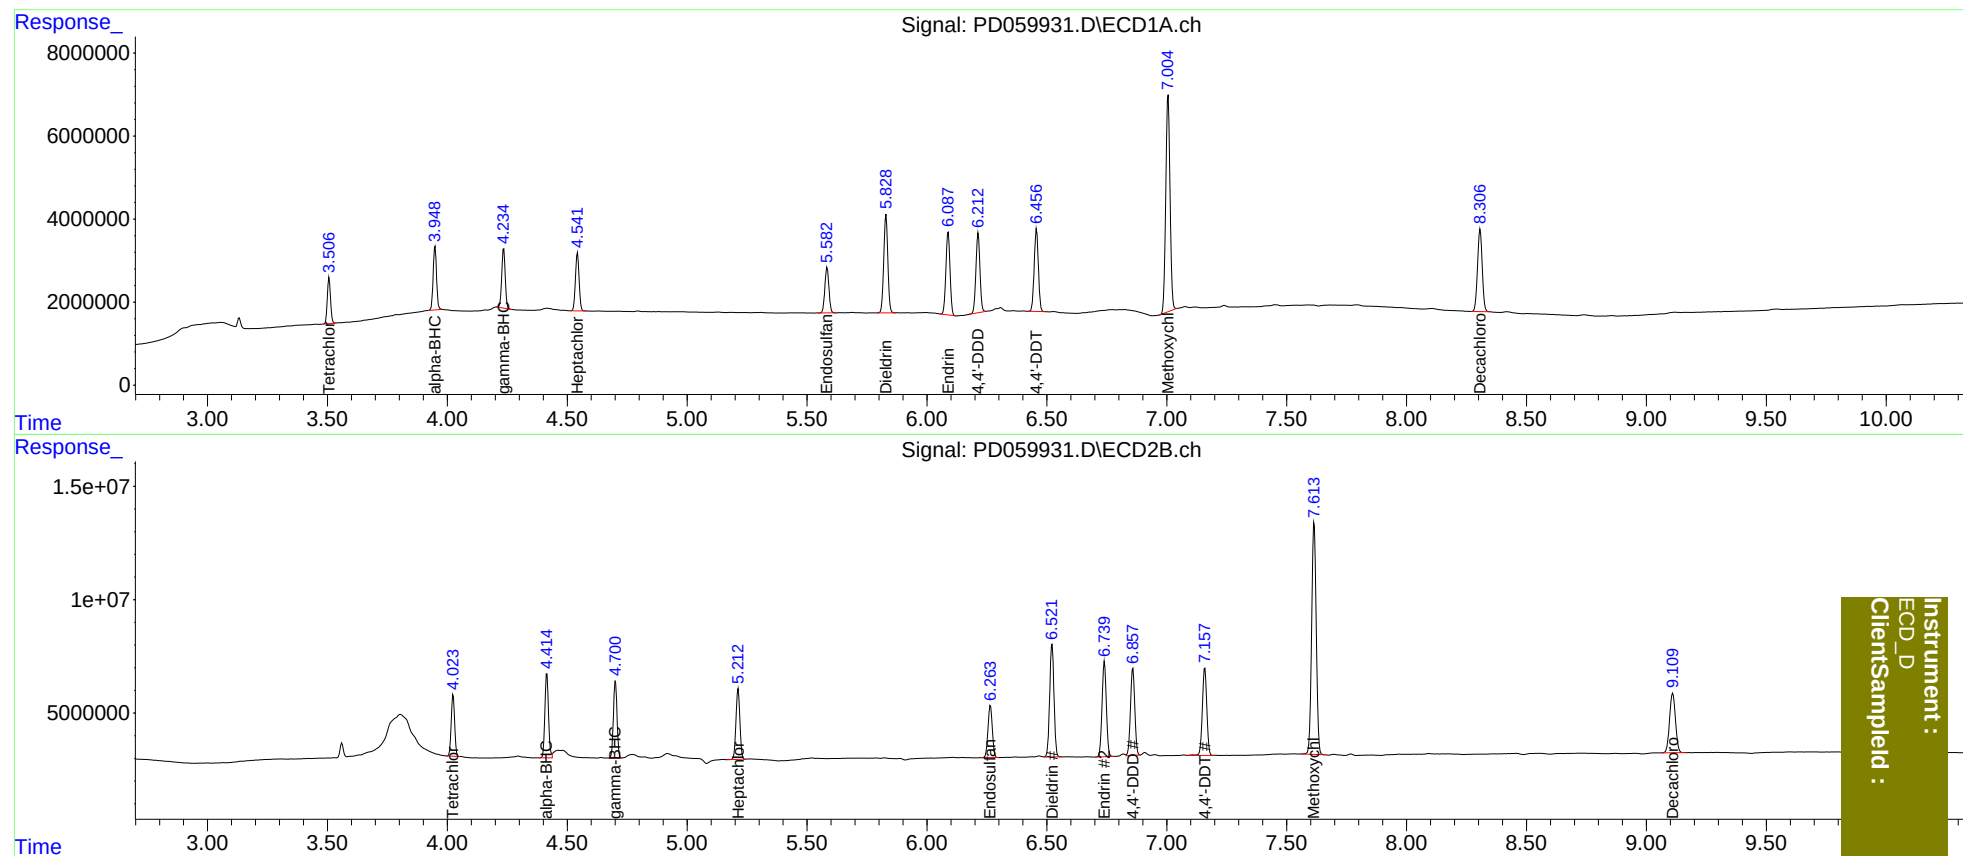


Instrument :
ECD_D
ClientSampled :

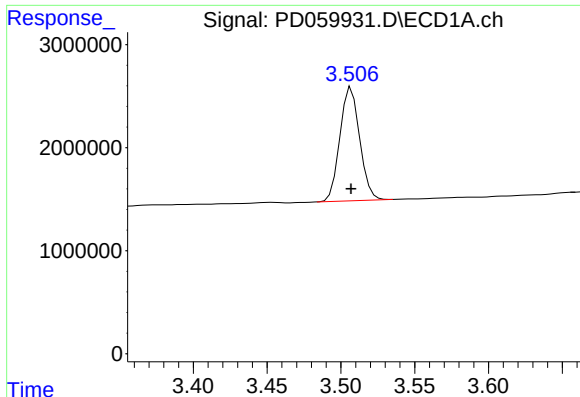

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 10329906
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

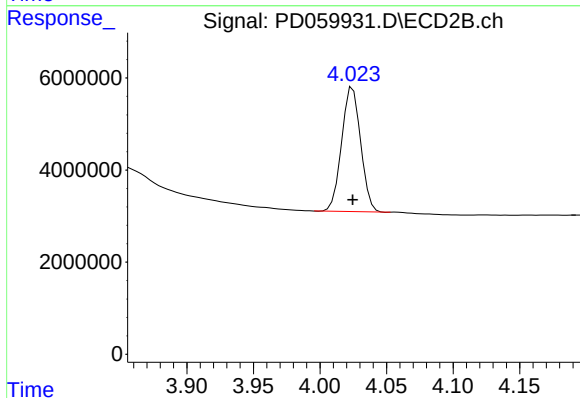


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 26838394
Conc: 10.18 ng/ml

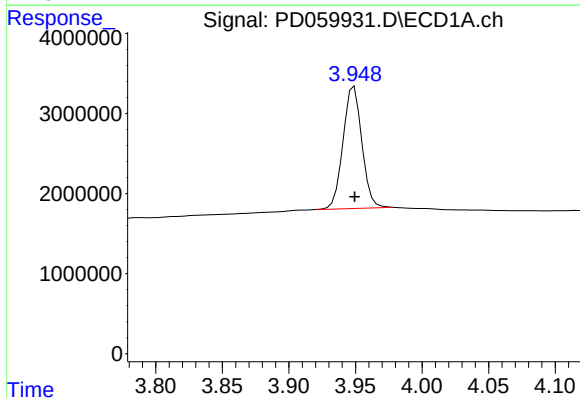


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 15022635
Conc: 10.34 ng/ml

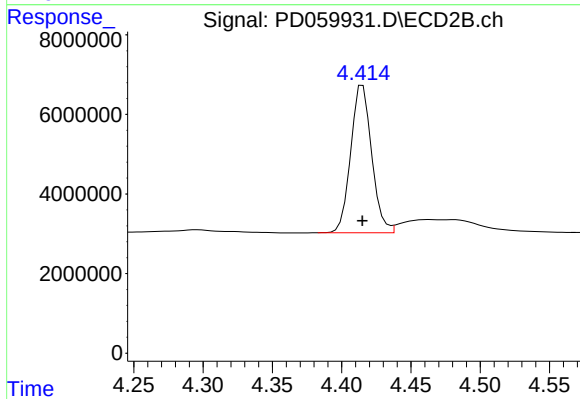

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 39103404
Conc: 10.10 ng/ml

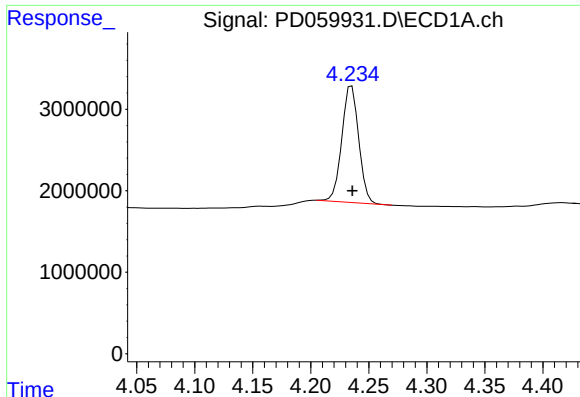

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 14439961
Conc: 10.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

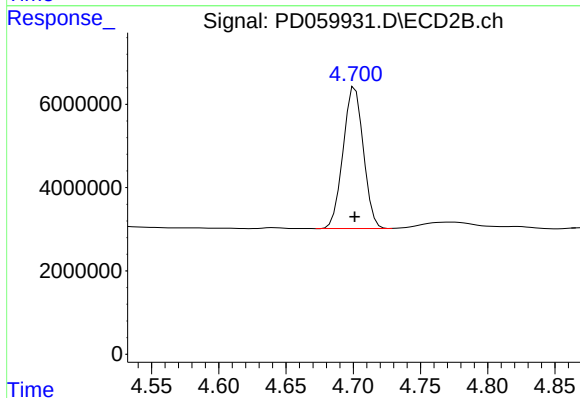


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 35551371
Conc: 10.05 ng/ml

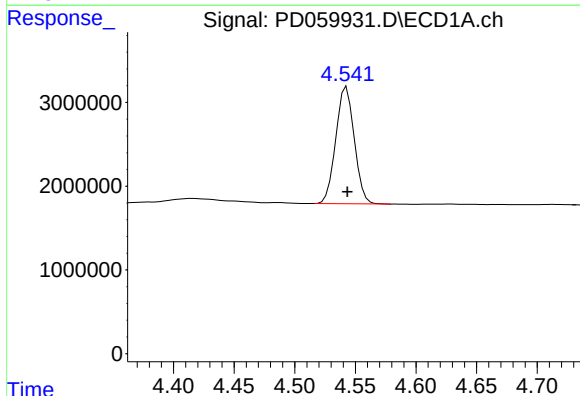


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 14819430
Conc: 10.27 ng/ml

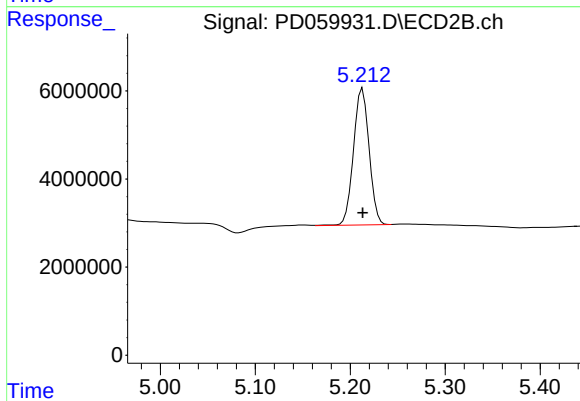

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 35437569
Conc: 10.24 ng/ml

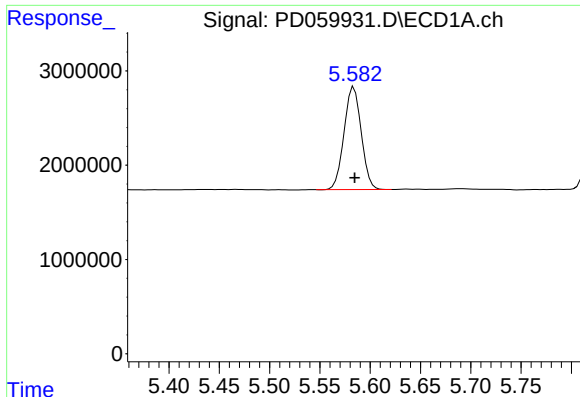

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 12907858
Conc: 10.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

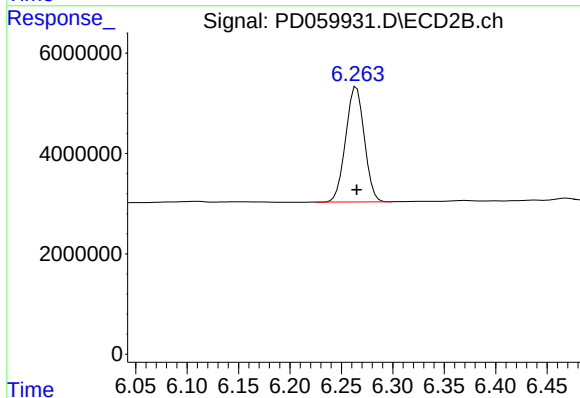


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 28933872
Conc: 10.28 ng/ml

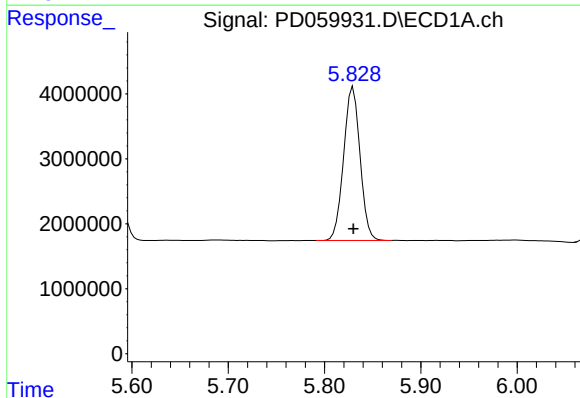


#13 Dieldrin

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 27870042
Conc: 20.48 ng/ml

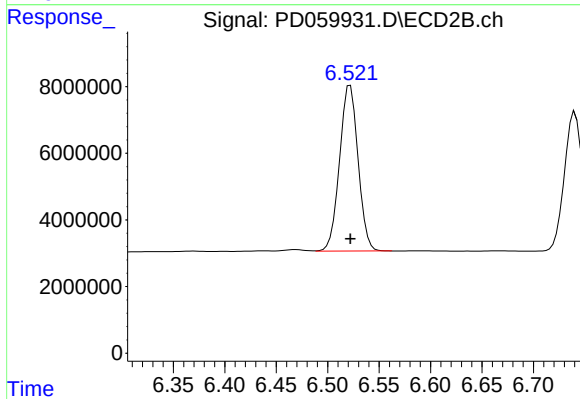

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 62241930
Conc: 20.11 ng/ml

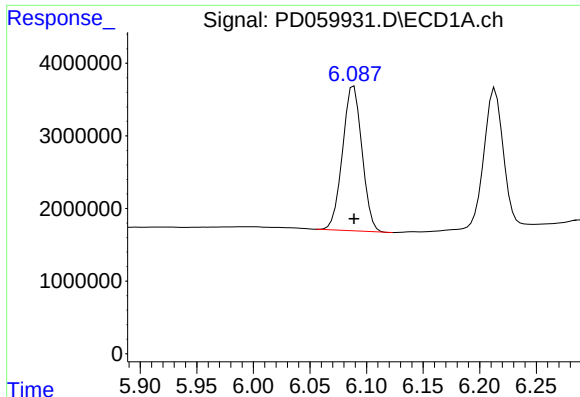

#14 Endrin


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 23892923
Conc: 20.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

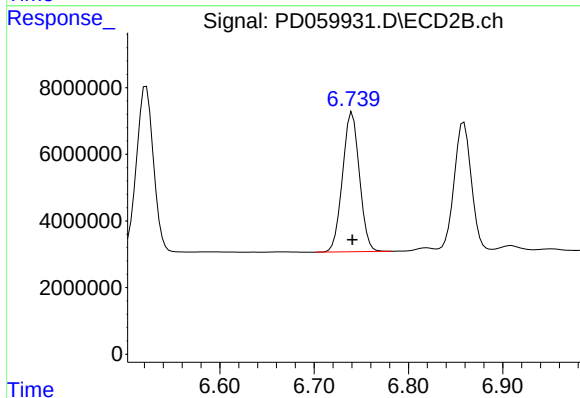


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 52157175
Conc: 20.13 ng/ml

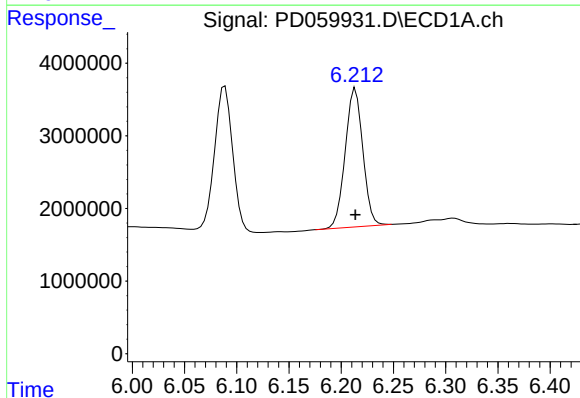


#16 4,4'-DDD

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 22377003
Conc: 20.68 ng/ml

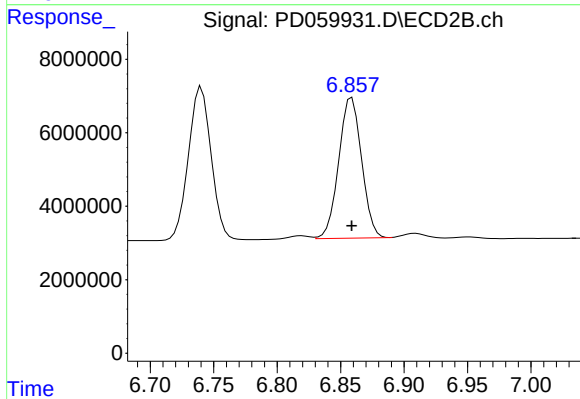

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 48024166
Conc: 20.10 ng/ml

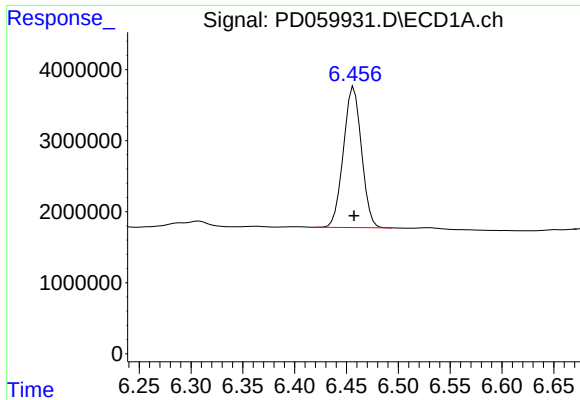

#17 4,4'-DDT


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 24005053
Conc: 20.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

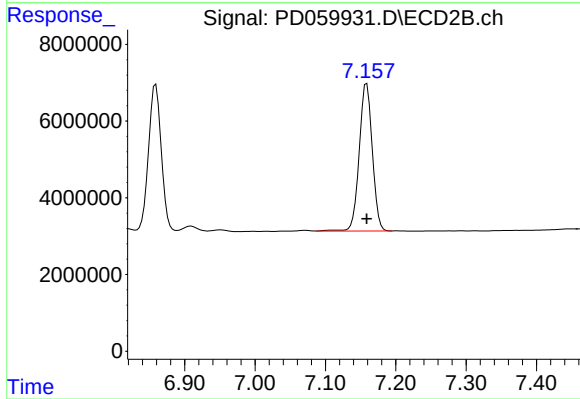


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 49842390
Conc: 20.06 ng/ml

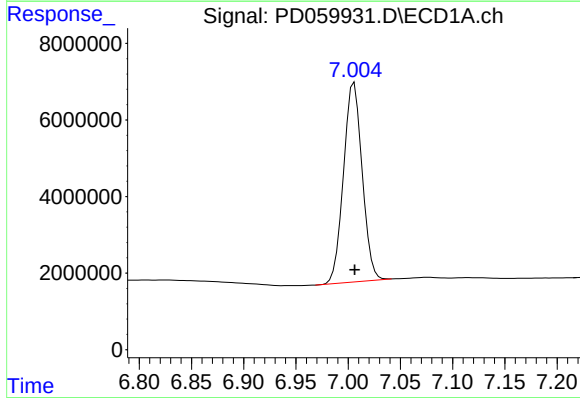


#20 Methoxychlor

R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 64500501
Conc: 104.84 ng/ml

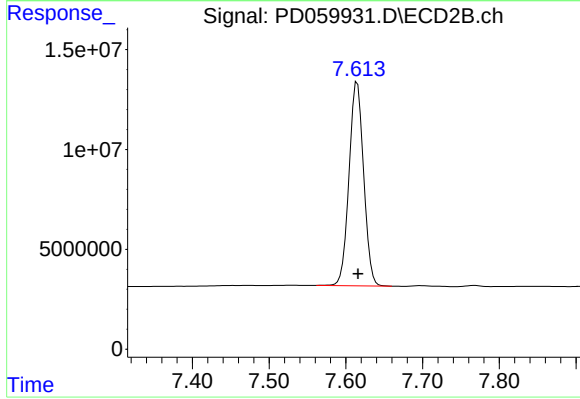

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: -0.001 min
Response: 135941598
Conc: 104.23 ng/ml

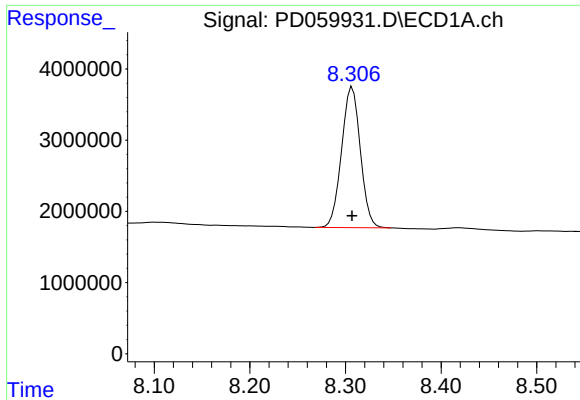

#27 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 26976926
Conc: 21.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

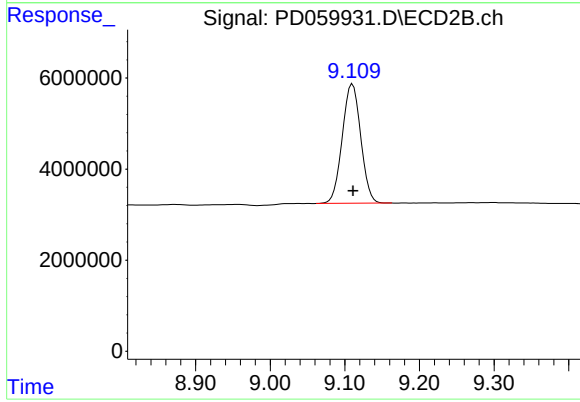

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 45093112
Conc: 20.86 ng/ml