

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 17:11
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:52:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	19758078	52740129	20.000	20.000
27)	SA Decachlor...	8.307	9.111	50486292	86448991	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.949	4.415	29049344	77465322	20.000	20.000
3)	MA gamma-BHC...	4.236	4.701	27680857	70782163	20.000	20.000
4)	MA Heptachlor	4.543	5.213	28855297	69221483	20.000	20.000
9)	A Endosulfan I	5.585	6.265	24788885	56317555	20.000	20.000
13)	MA Dieldrin	5.830	6.522	54432412	123.8E6	40.000	40.000
14)	MA Endrin	6.089	6.741	46188121	103.6E6	40.000	40.000
16)	A 4,4'-DDD	6.214	6.859	43274242	95590441	40.000	40.000
17)	MA 4,4'-DDT	6.457	7.159	47295455	99373433	40.000	40.000
20)	A Methoxychlor	7.006	7.616	123.0E6	260.8E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 17:11
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:52:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

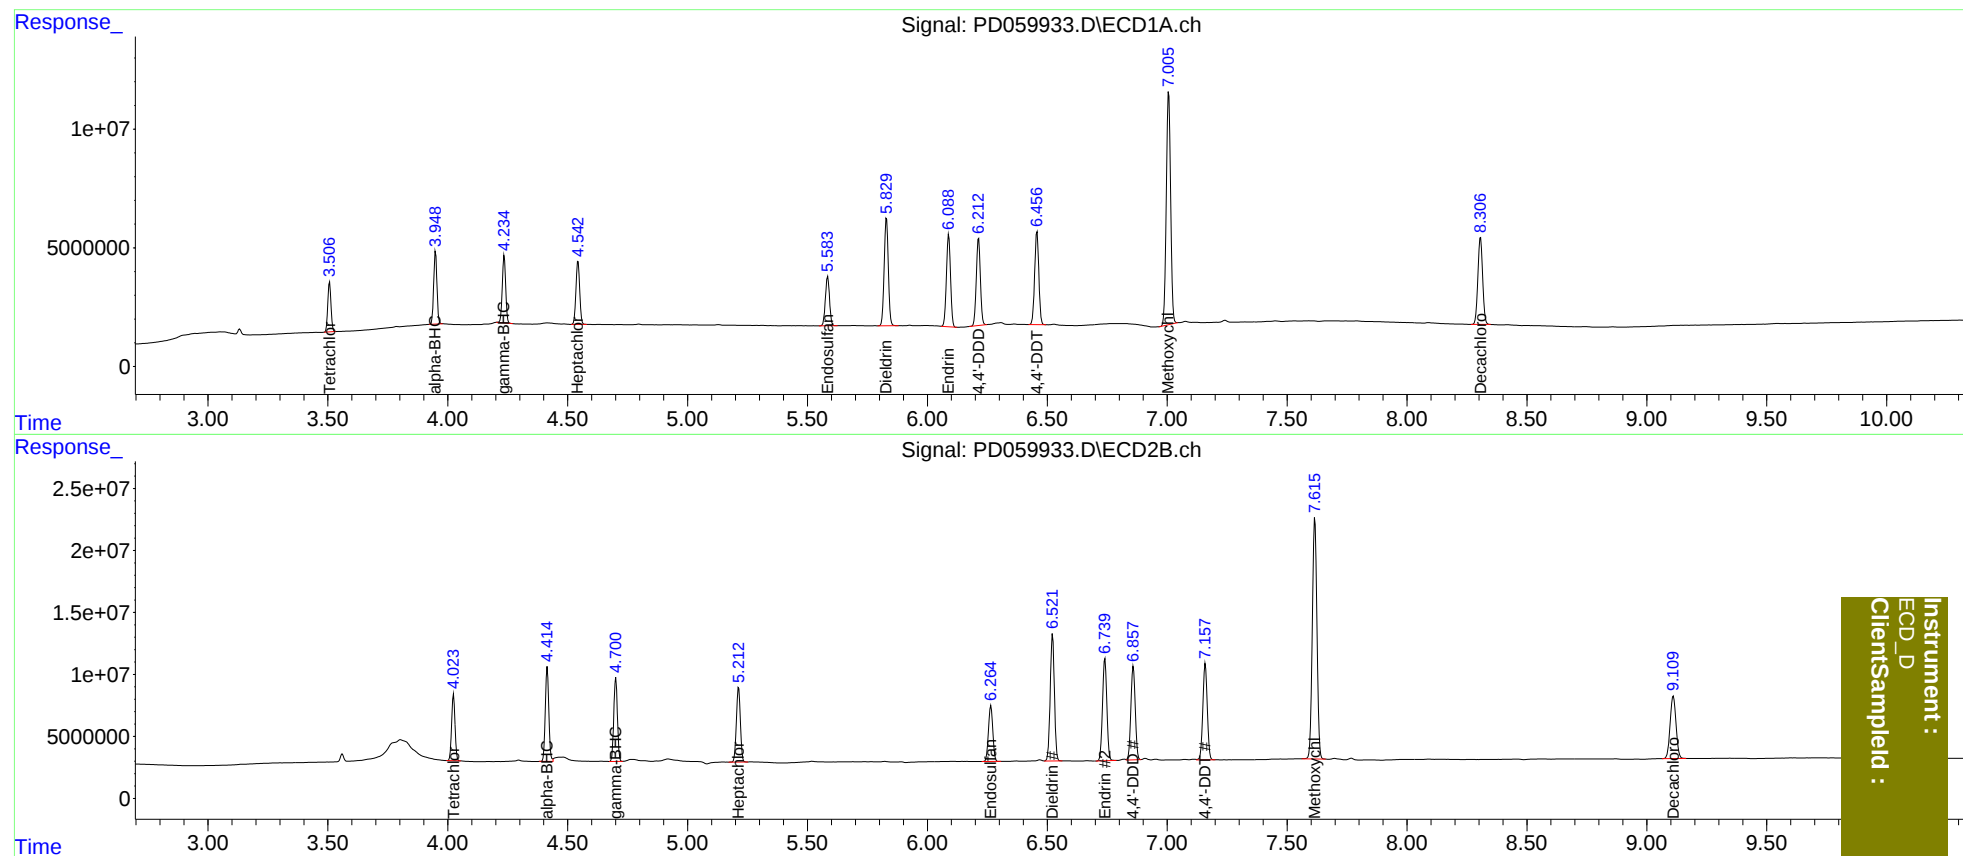


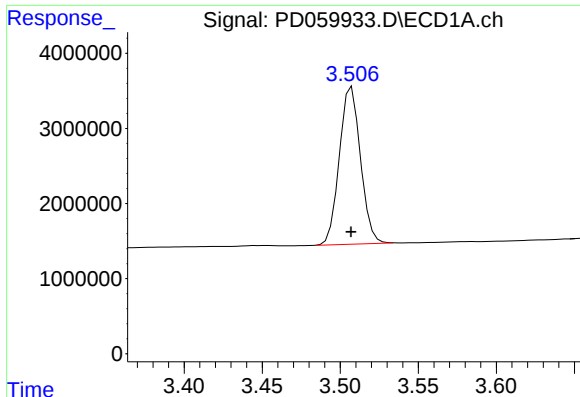

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 19758078
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

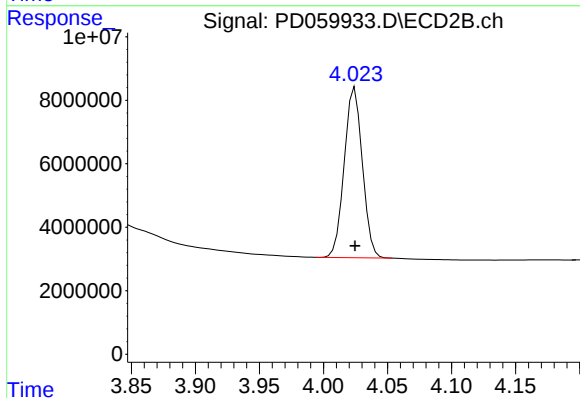


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 52740129
Conc: 20.00 ng/ml

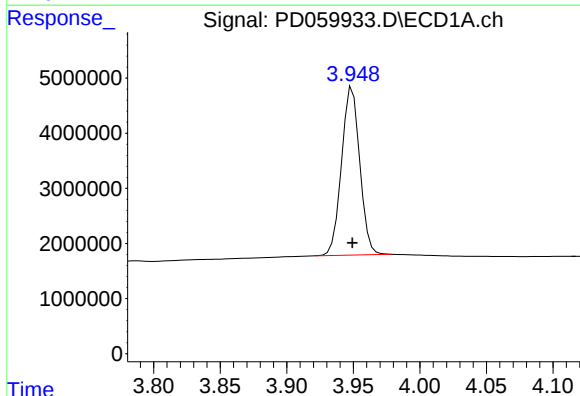


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 29049344
Conc: 20.00 ng/ml

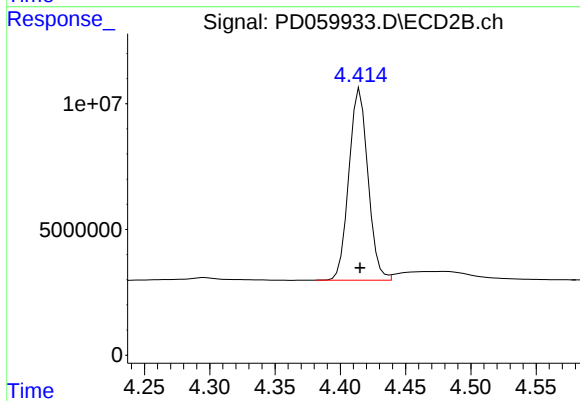

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 77465322
Conc: 20.00 ng/ml

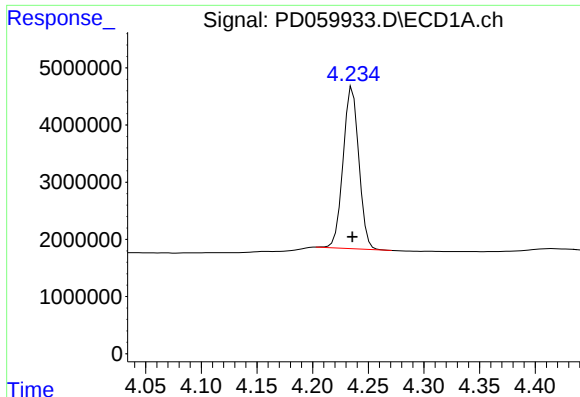

#3 gamma-BHC (Lindane)


R.T.: 4.236 min
Delta R.T.: 0.000 min
Response: 27680857
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

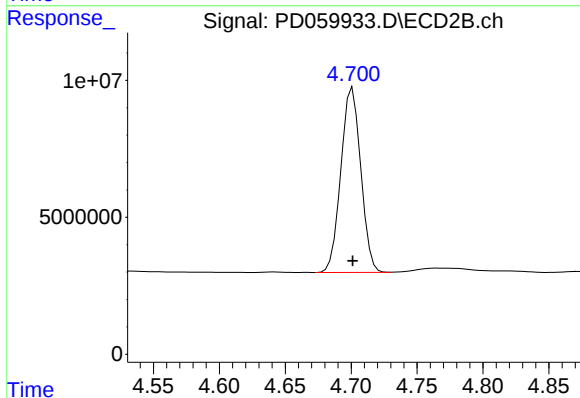


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 70782163
Conc: 20.00 ng/ml

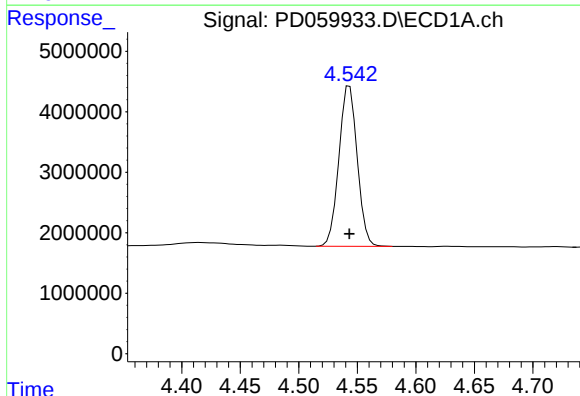


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 28855297
Conc: 20.00 ng/ml

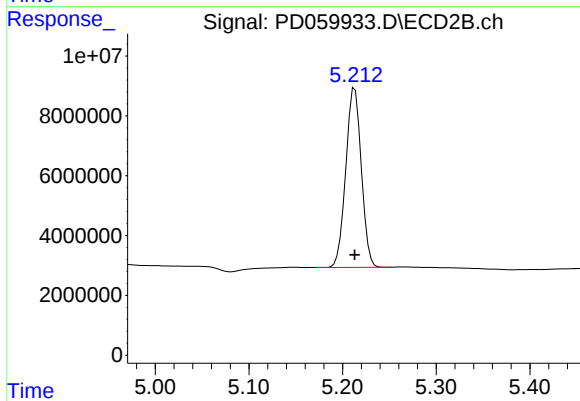

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 69221483
Conc: 20.00 ng/ml

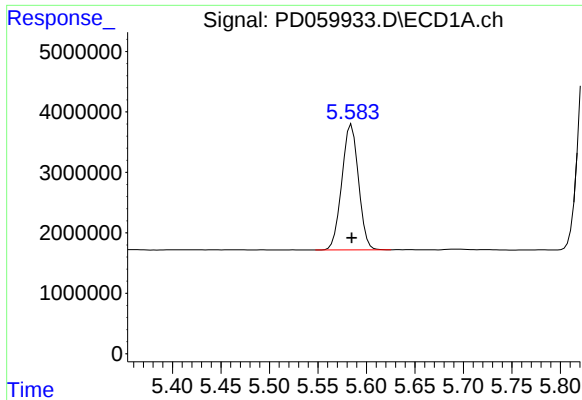

#9 Endosulfan I


R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 24788885
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

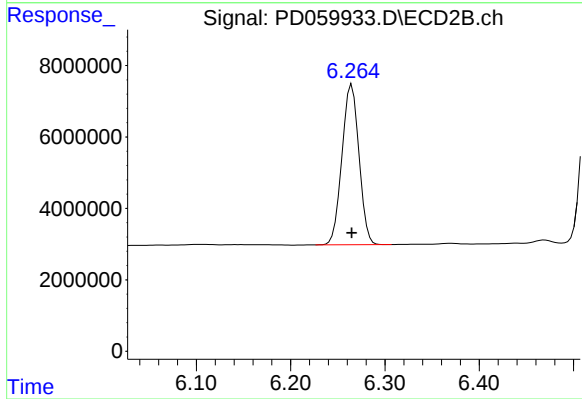


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 56317555
Conc: 20.00 ng/ml

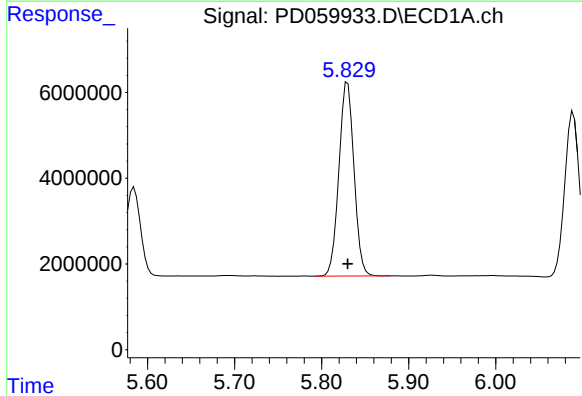


#13 Dieldrin

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 54432412
Conc: 40.00 ng/ml

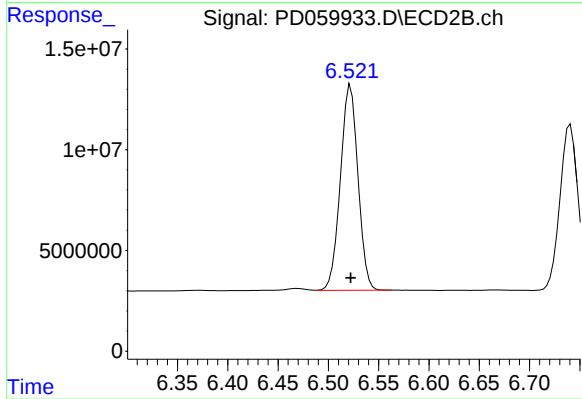

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 123774131
Conc: 40.00 ng/ml

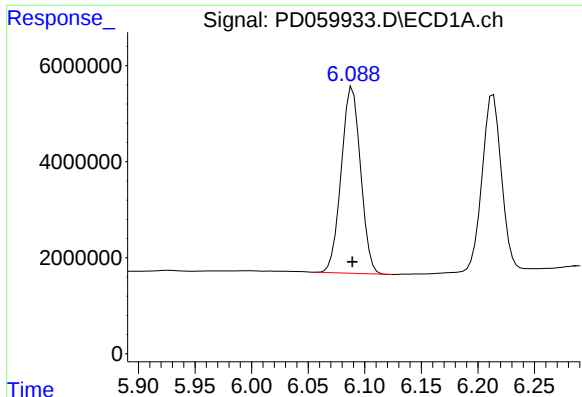

#14 Endrin


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 46188121
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

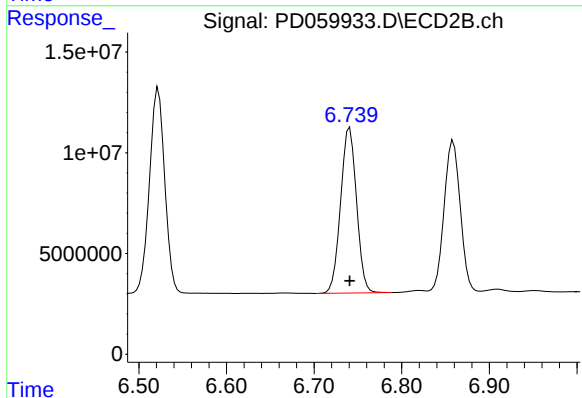


#14 Endrin

R.T.: 6.741 min
Delta R.T.: 0.000 min
Response: 103618692
Conc: 40.00 ng/ml

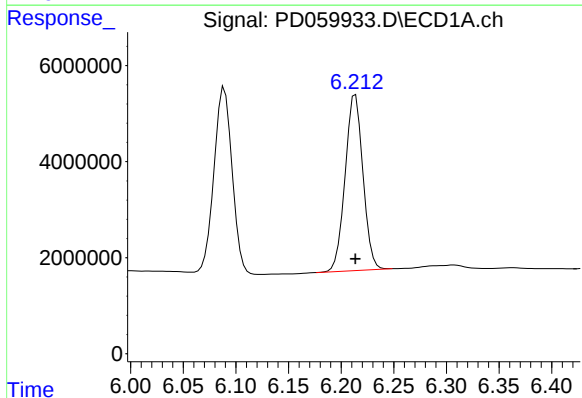


#16 4,4'-DDD

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 43274242
Conc: 40.00 ng/ml

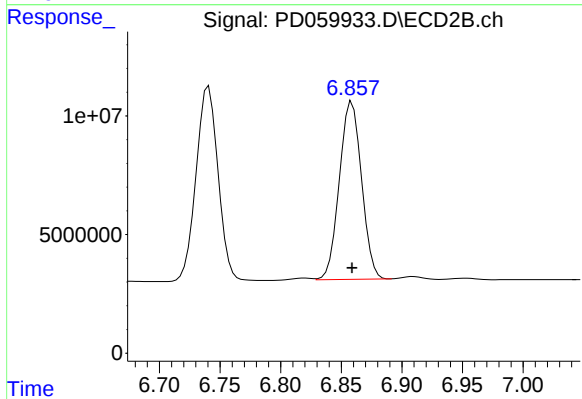

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 95590441
Conc: 40.00 ng/ml

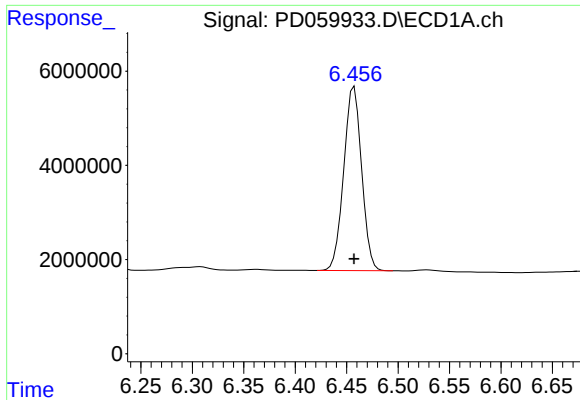

#17 4,4'-DDT


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 47295455
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

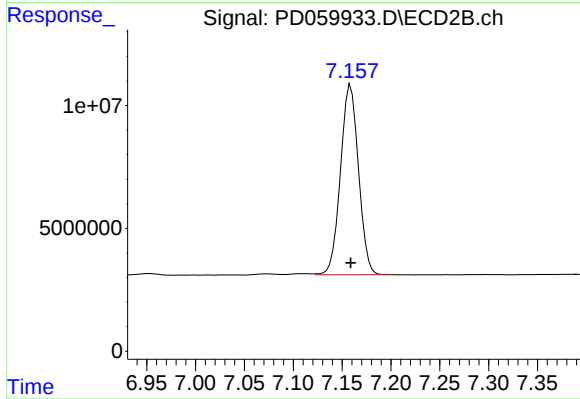


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 99373433
Conc: 40.00 ng/ml

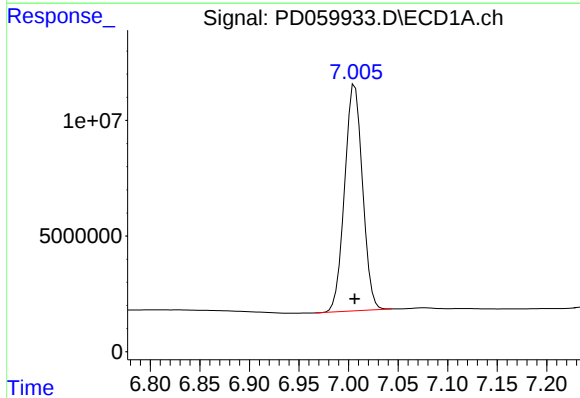


#20 Methoxychlor

R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 123042267
Conc: 200.00 ng/ml

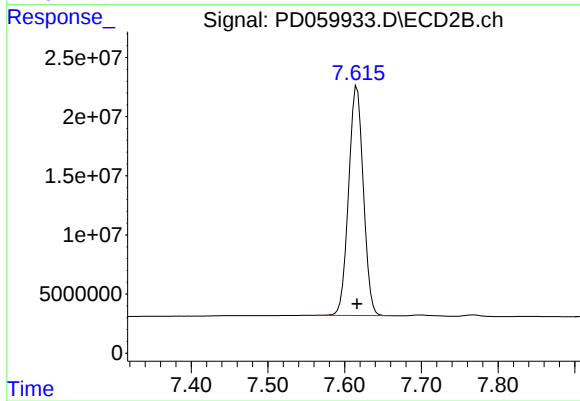

#20 Methoxychlor


R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 260843831
Conc: 200.00 ng/ml

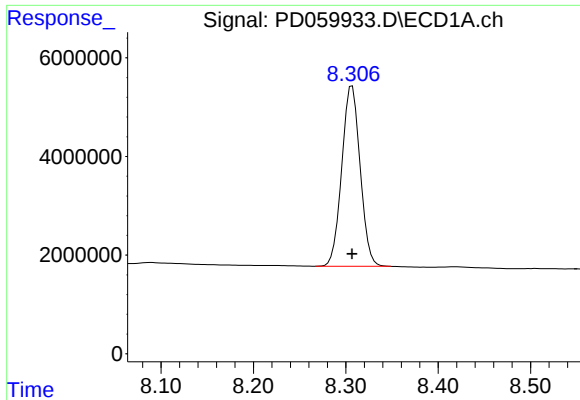

#27 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 50486292
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

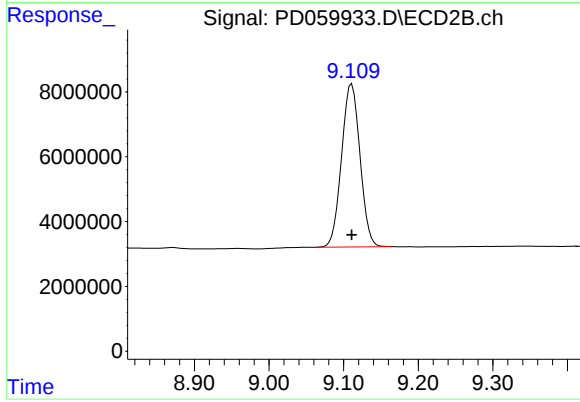

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 86448991
Conc: 40.00 ng/ml