

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 17:39
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:52:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	38651229	105.1E6	39.124	39.866
27)	SA Decachlor...	8.307	9.111	98570378	170.2E6	78.097	78.767
Target Compounds							
2)	A alpha-BHC	3.949	4.415	58884193	158.3E6	40.541	40.868
3)	MA gamma-BHC...	4.235	4.701	55715566	144.4E6	40.256	40.804
4)	MA Heptachlor	4.543	5.213	58221115	141.8E6	40.354	40.977
9)	A Endosulfan I	5.584	6.264	49839471	113.0E6	40.211	40.138
13)	MA Dieldrin	5.830	6.522	112.8E6	254.3E6	82.909	82.169
14)	MA Endrin	6.089	6.740	94447777	214.4E6	81.794	82.778
16)	A 4,4'-DDD	6.214	6.859	89166781	197.4E6	82.420	82.585
17)	MA 4,4'-DDT	6.457	7.159	97825291	207.3E6	82.735	83.439
20)	A Methoxychlor	7.006	7.615	245.4E6	516.2E6	398.880	395.786


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 17:39
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:52:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

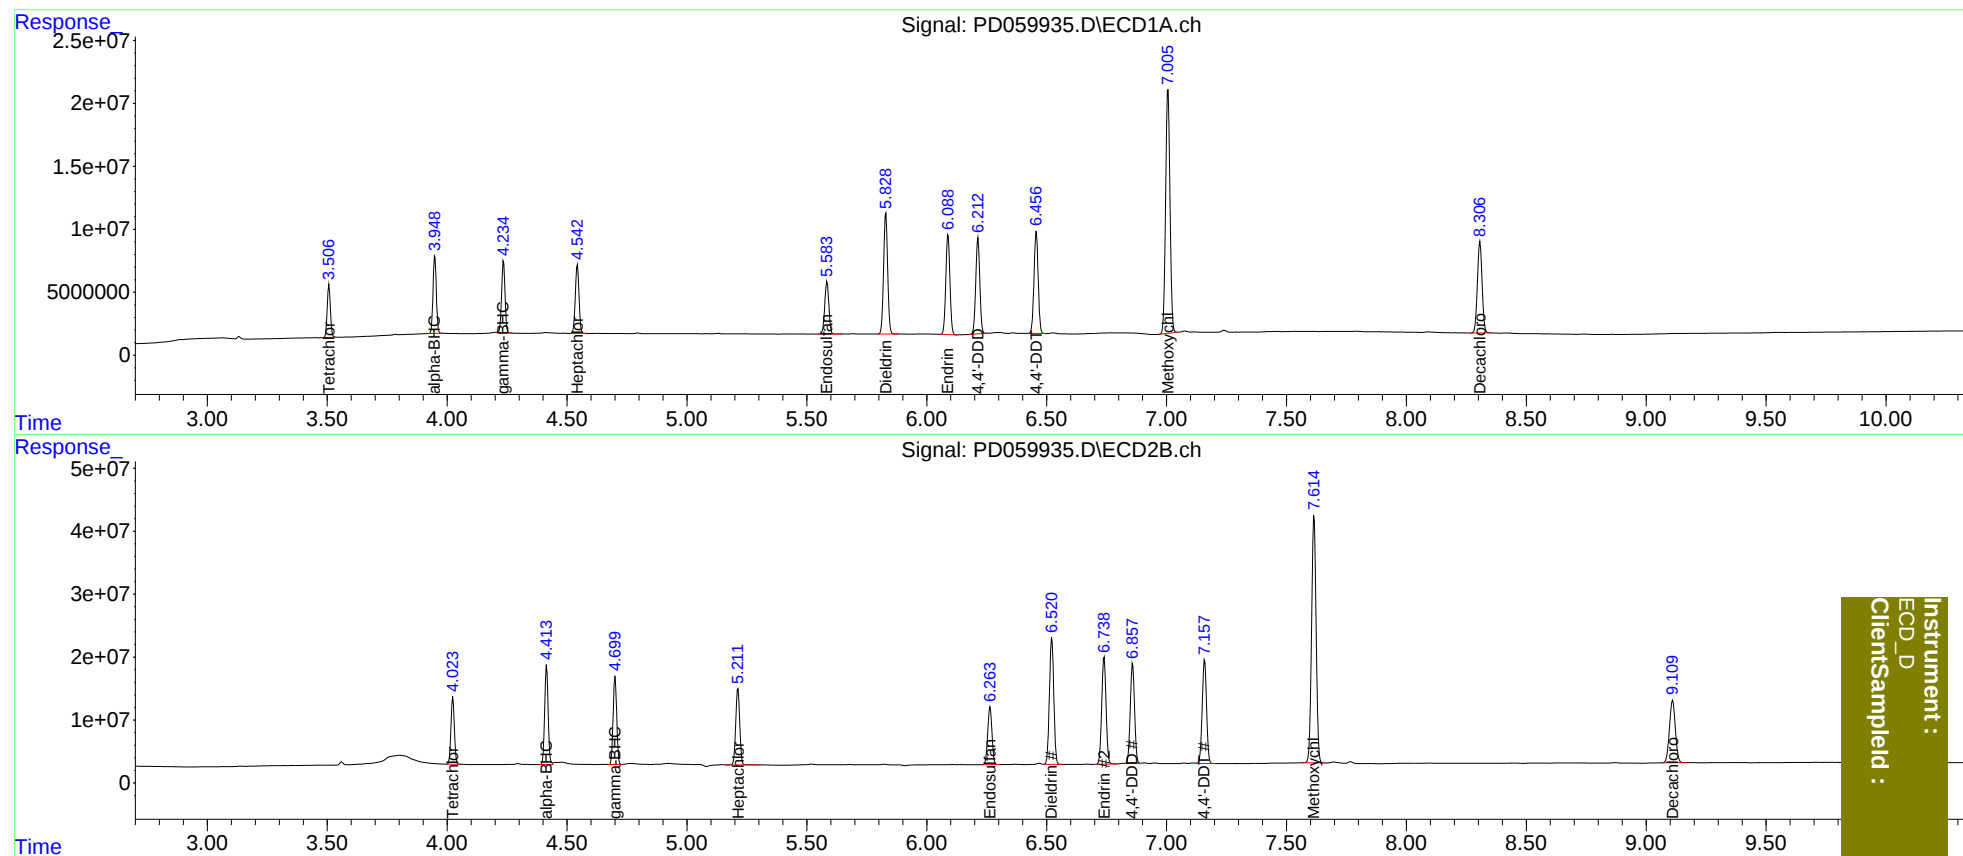


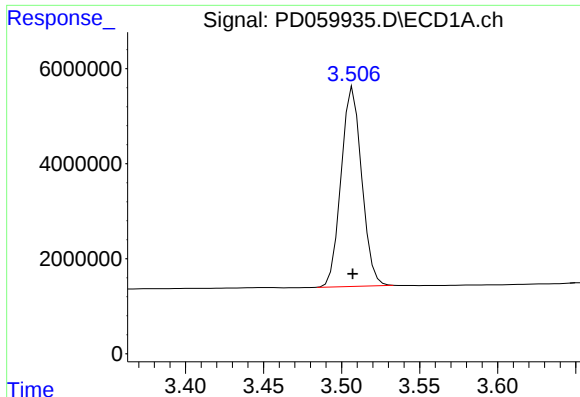

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 38651229
Conc: 39.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

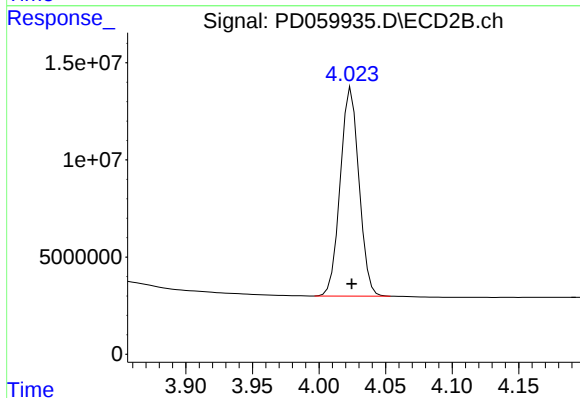


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 105127312
Conc: 39.87 ng/ml

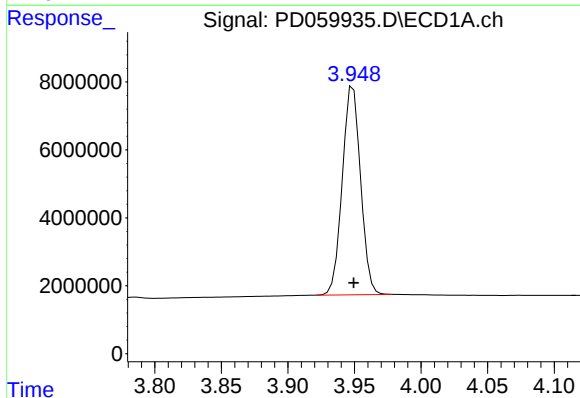


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 58884193
Conc: 40.54 ng/ml

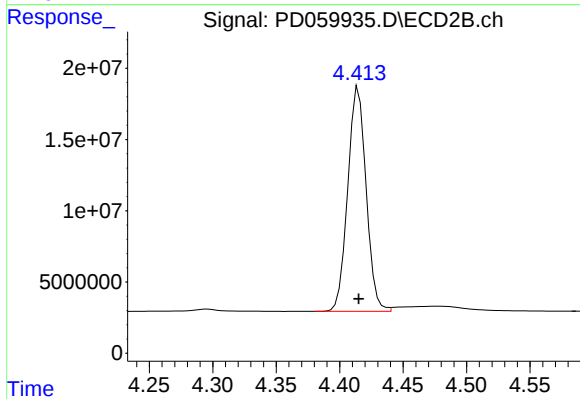

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 158294159
Conc: 40.87 ng/ml

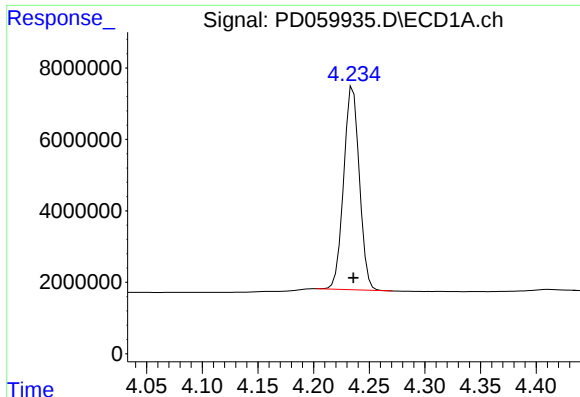

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 55715566
Conc: 40.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

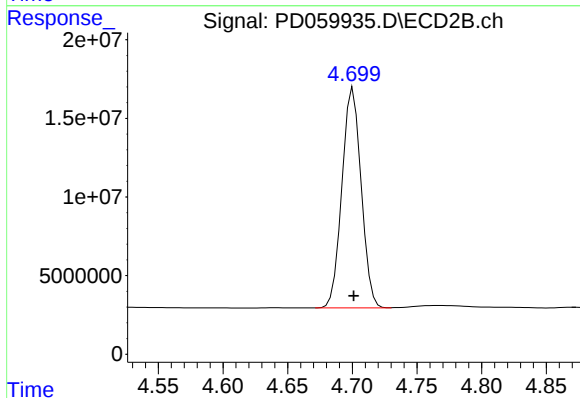


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 144409201
Conc: 40.80 ng/ml

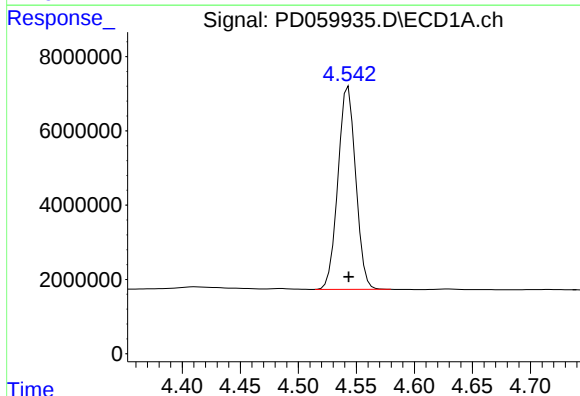


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 58221115
Conc: 40.35 ng/ml

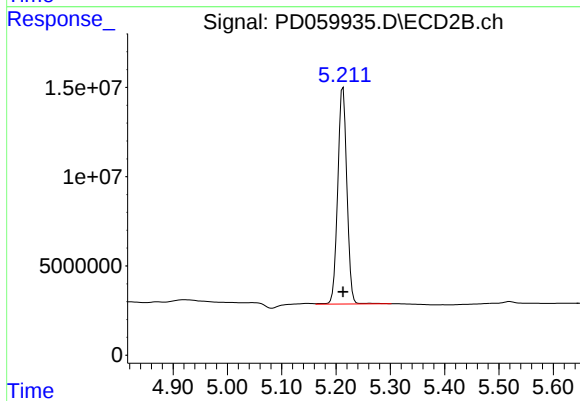

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 141825450
Conc: 40.98 ng/ml

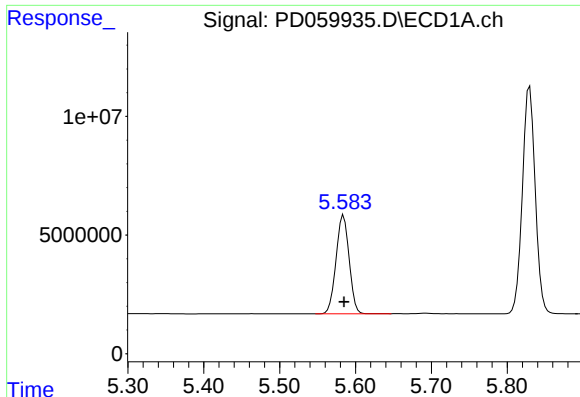

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 49839471
Conc: 40.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

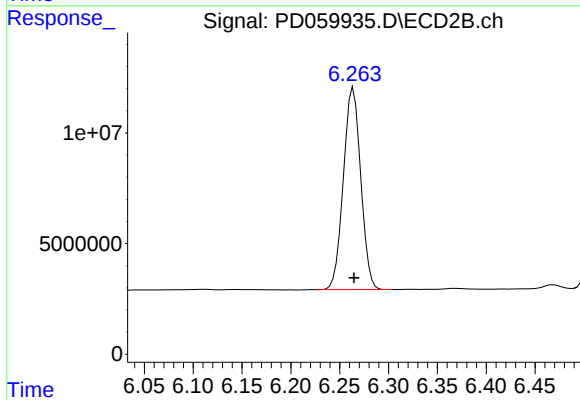


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 113023687
Conc: 40.14 ng/ml

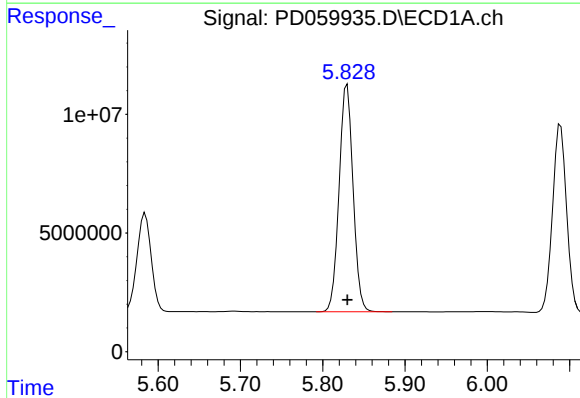


#13 Dieldrin

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 112823379
Conc: 82.91 ng/ml

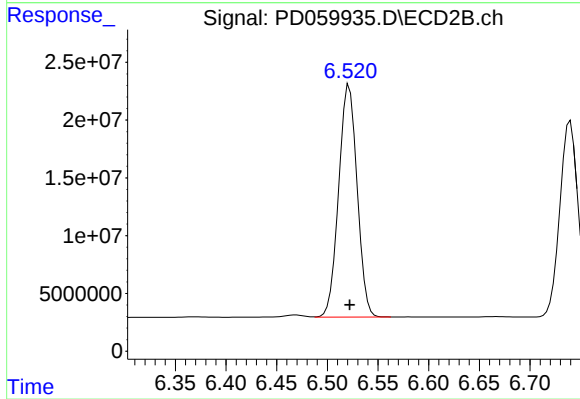

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 254260611
Conc: 82.17 ng/ml

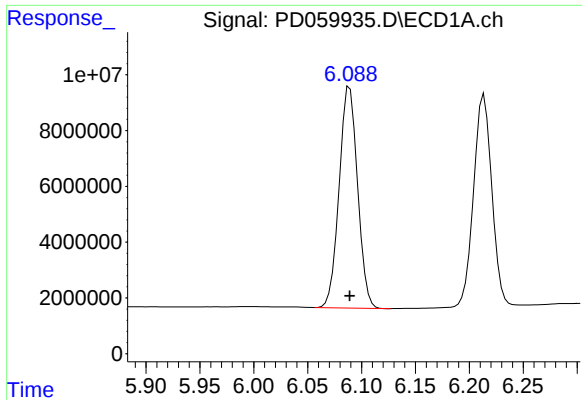

#14 Endrin


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 94447777
Conc: 81.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

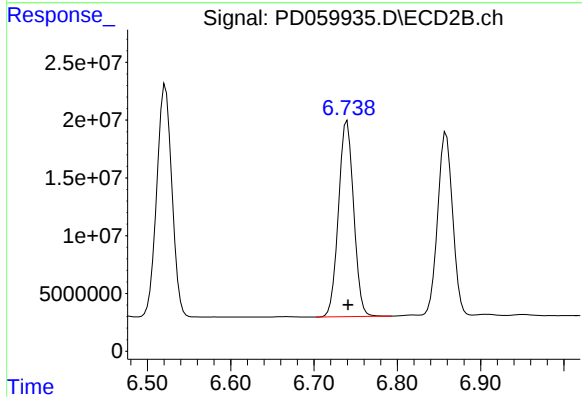


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 214433772
Conc: 82.78 ng/ml

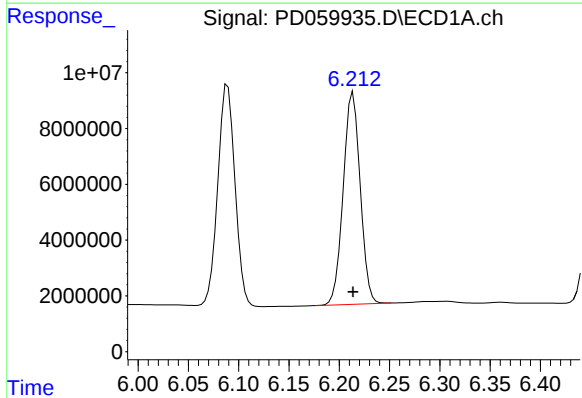


#16 4,4'-DDD

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 89166781
Conc: 82.42 ng/ml

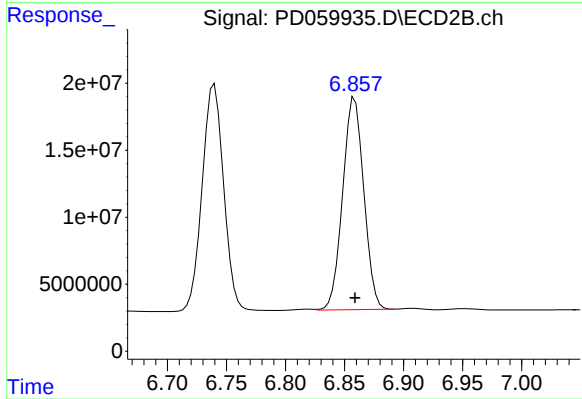

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 197357963
Conc: 82.58 ng/ml

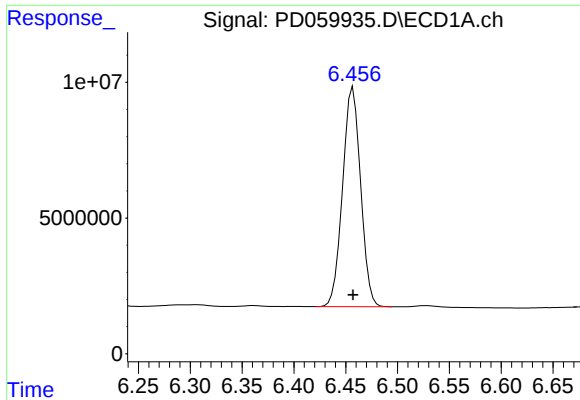

#17 4,4'-DDT


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 97825291
Conc: 82.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

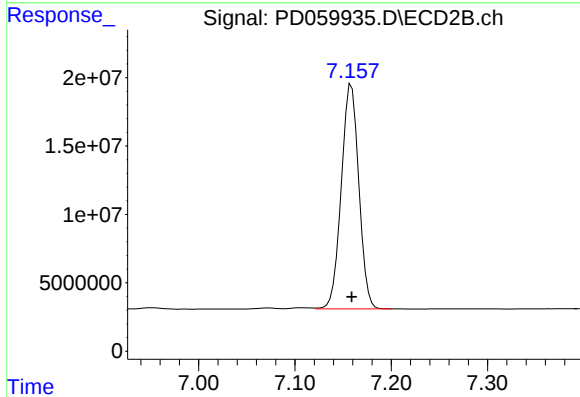


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 207291125
Conc: 83.44 ng/ml

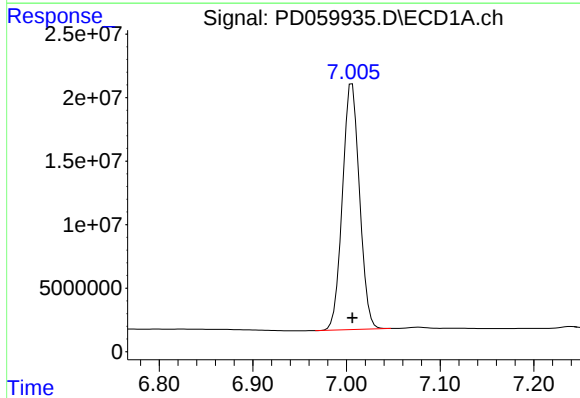


#20 Methoxychlor

R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 245395196
Conc: 398.88 ng/ml

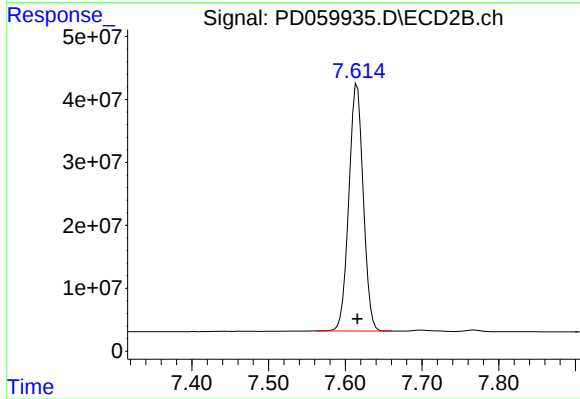

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 516192157
Conc: 395.79 ng/ml

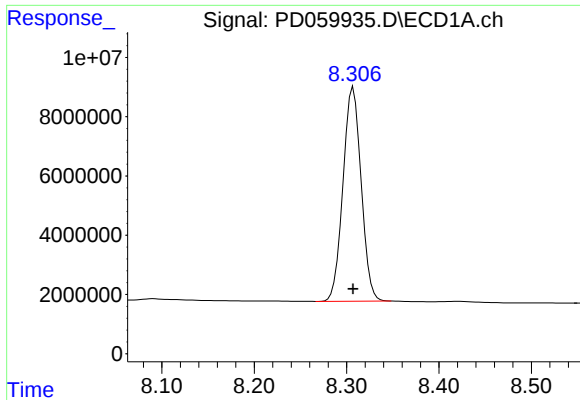

#27 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 98570378
Conc: 78.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

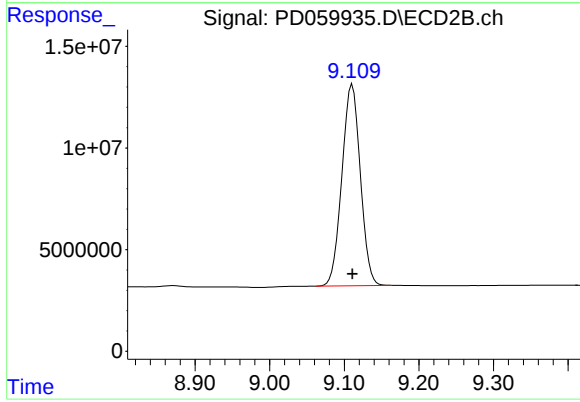

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 170233783
Conc: 78.77 ng/ml