

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 18:08
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:52:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	73532291	202.4E6	74.433	76.750
27)	SA Decachlor...	8.307	9.111	184.2E6	336.7E6	145.901	155.805
Target Compounds							
2)	A alpha-BHC	3.949	4.415	116.3E6	310.8E6	80.064	80.235
3)	MA gamma-BHC...	4.235	4.701	108.9E6	283.3E6	78.714	80.059
4)	MA Heptachlor	4.543	5.213	113.3E6	271.4E6	78.519	78.406
9)	A Endosulfan I	5.584	6.265	96645573	219.1E6	77.975	77.797
13)	MA Dieldrin	5.830	6.522	222.8E6	494.0E6	163.724	159.647
14)	MA Endrin	6.089	6.740	183.2E6	412.4E6	158.677	159.216
16)	A 4,4'-DDD	6.214	6.860	175.0E6	384.2E6	161.754	160.764
17)	MA 4,4'-DDT	6.457	7.160	193.0E6	405.0E6	163.236	163.034
20)	A Methoxychlor	7.006	7.616	458.6E6	953.1E6	745.481	730.750

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 18:08
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:52:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

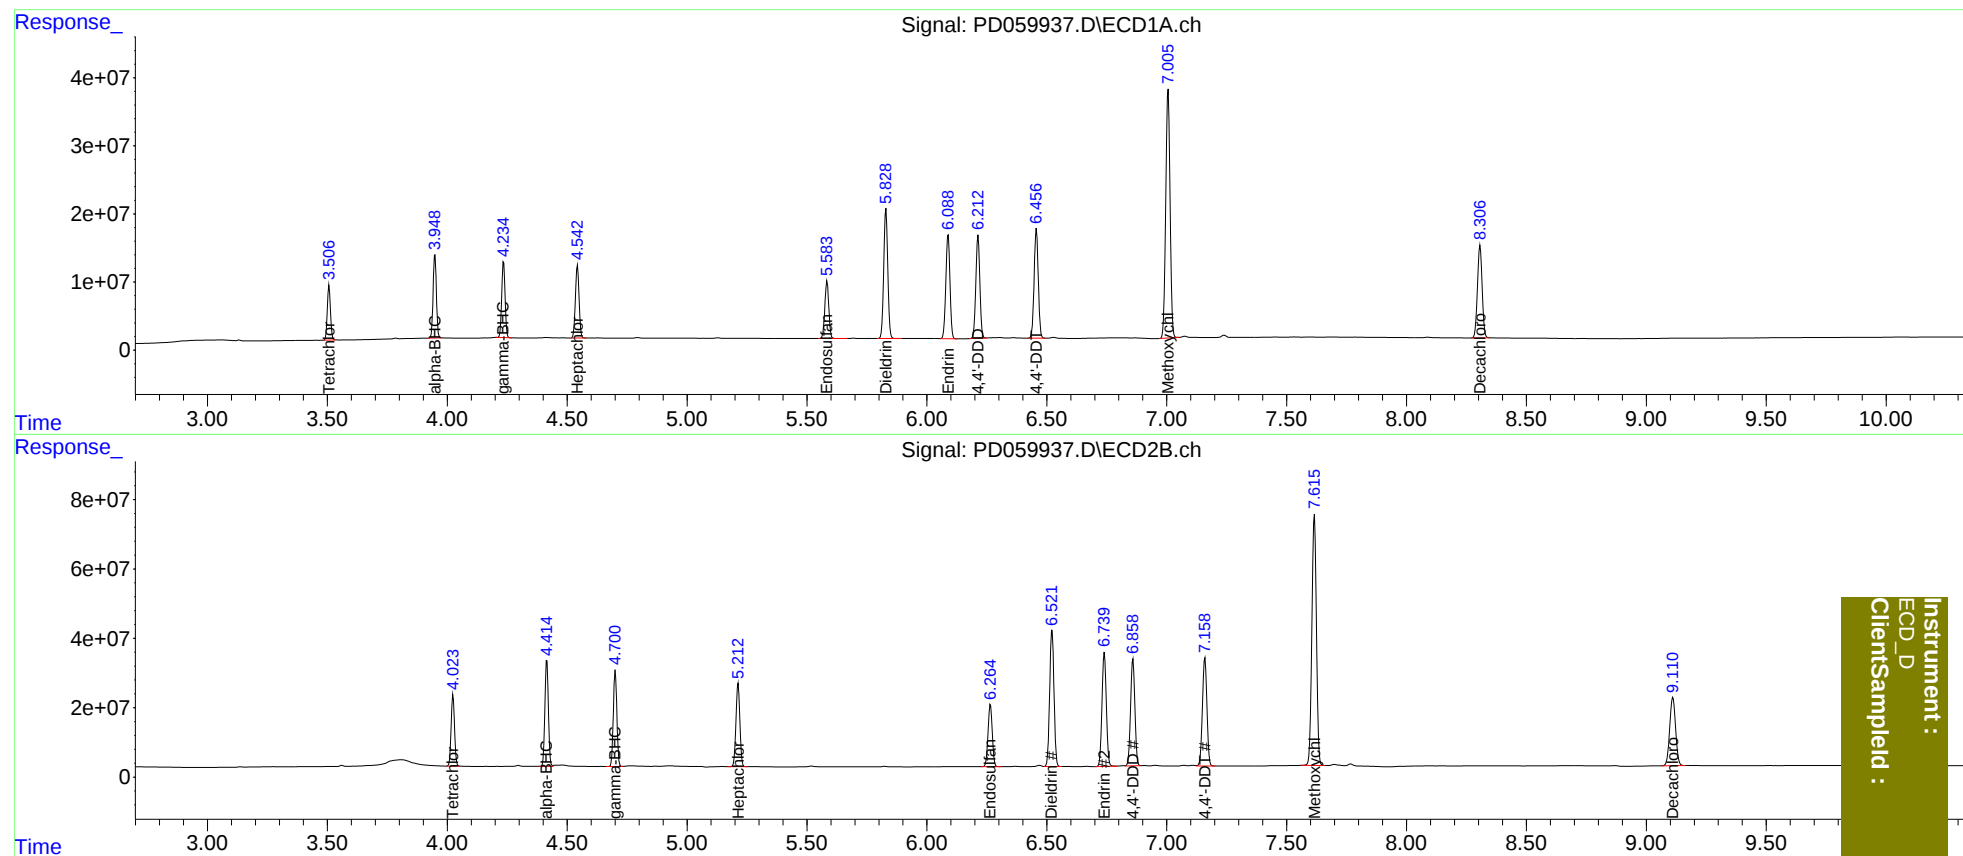


Instrument :
ECD_D
ClientSampled :

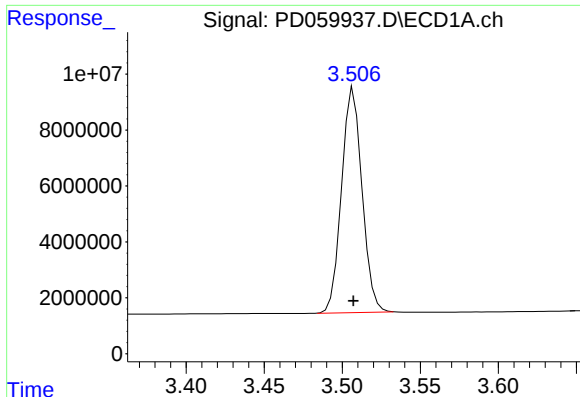

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 73532291
Conc: 74.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

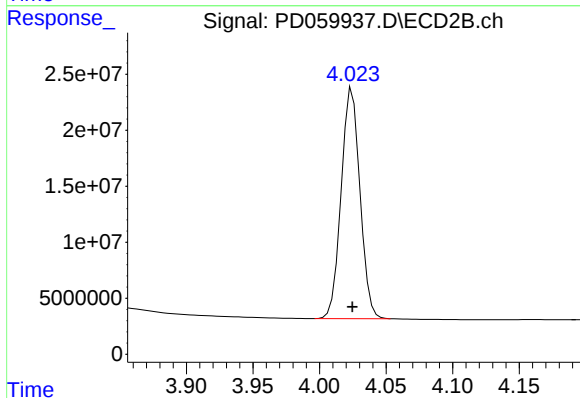


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 202391440
Conc: 76.75 ng/ml

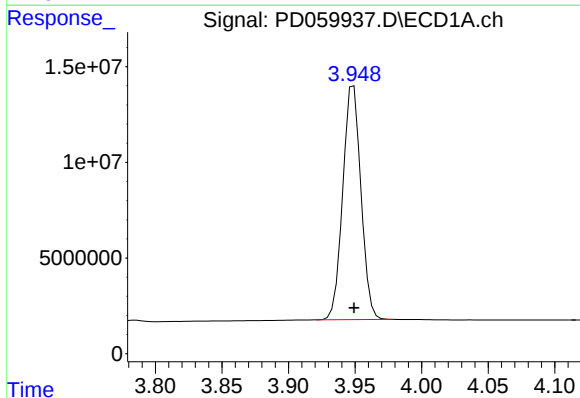


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 116289837
Conc: 80.06 ng/ml

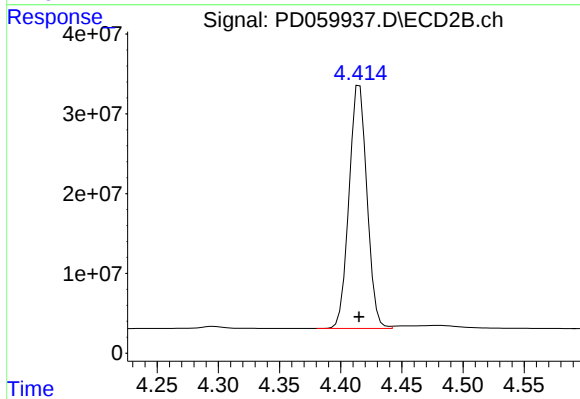

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 310771903
Conc: 80.24 ng/ml

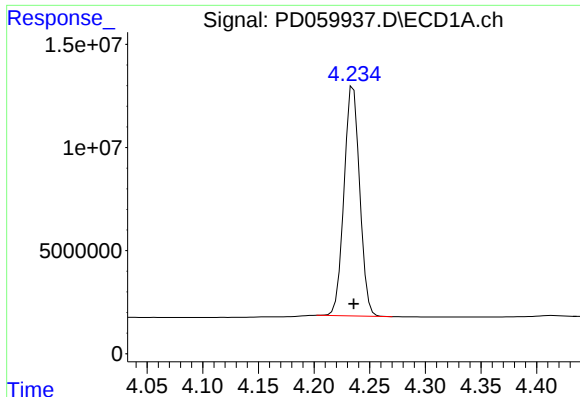

#3 gamma-BHC (Lindane)


R.T.: 4.235 min
Delta R.T.: 0.000 min
Response: 108943498
Conc: 78.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

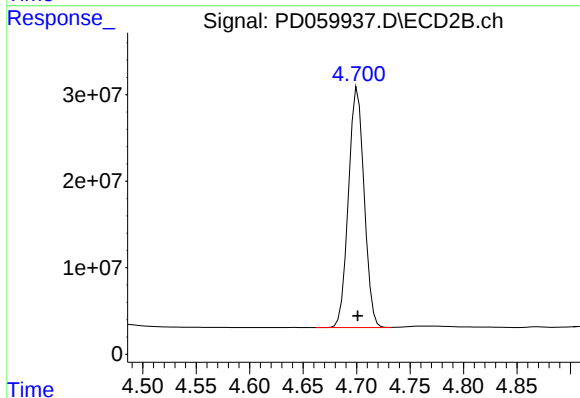


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 283337320
Conc: 80.06 ng/ml

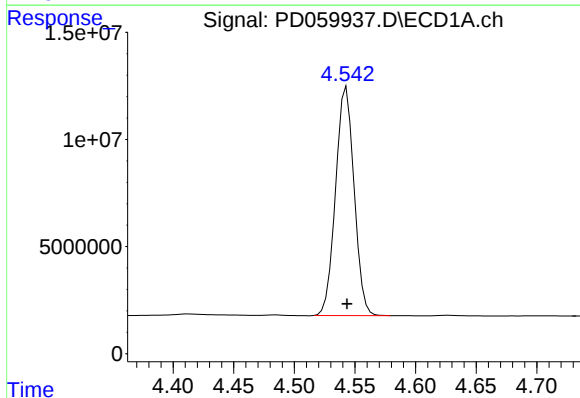


#4 Heptachlor

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 113283801
Conc: 78.52 ng/ml

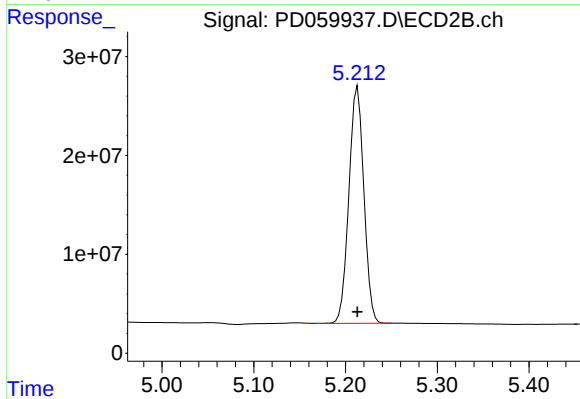

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 271368955
Conc: 78.41 ng/ml

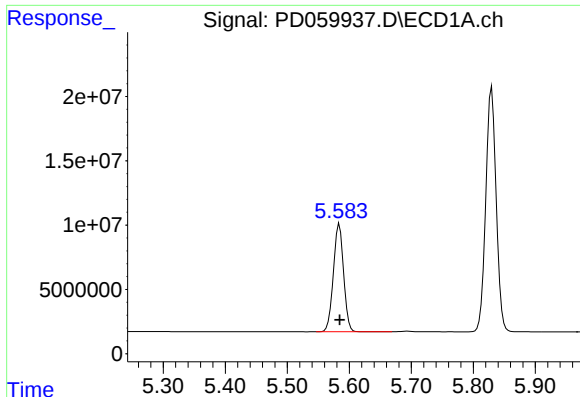

#9 Endosulfan I


R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 96645573
Conc: 77.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

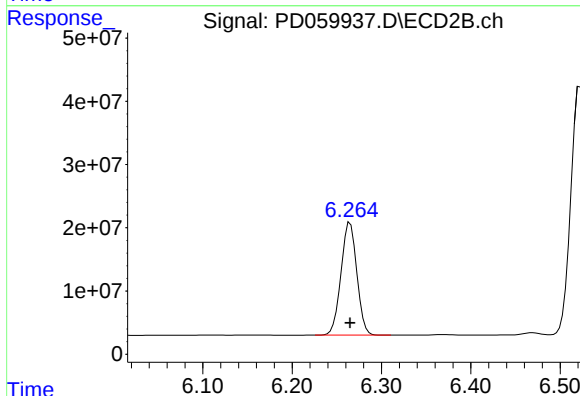


#9 Endosulfan I

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 219065769
Conc: 77.80 ng/ml

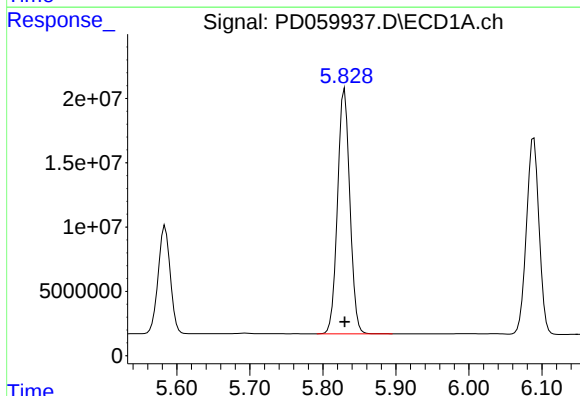


#13 Dieldrin

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 222797004
Conc: 163.72 ng/ml

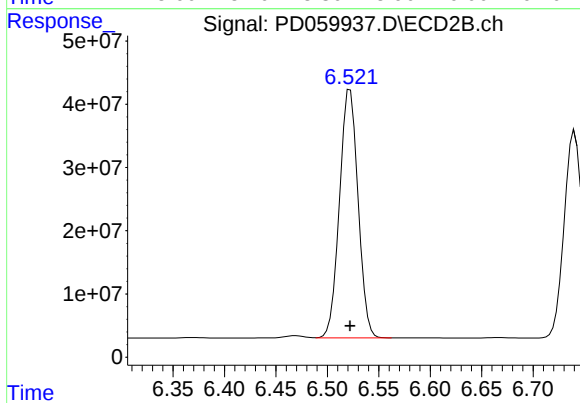

#13 Dieldrin


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 494003651
Conc: 159.65 ng/ml

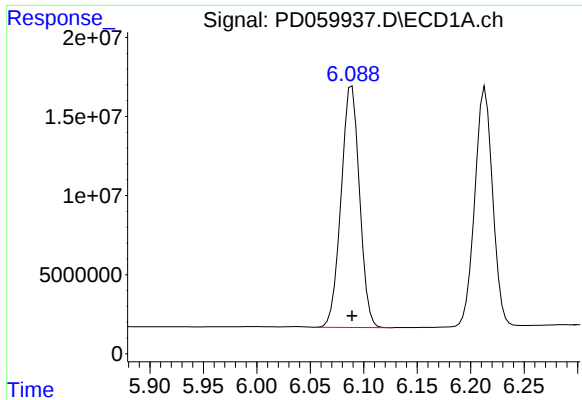

#14 Endrin


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 183224368
Conc: 158.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

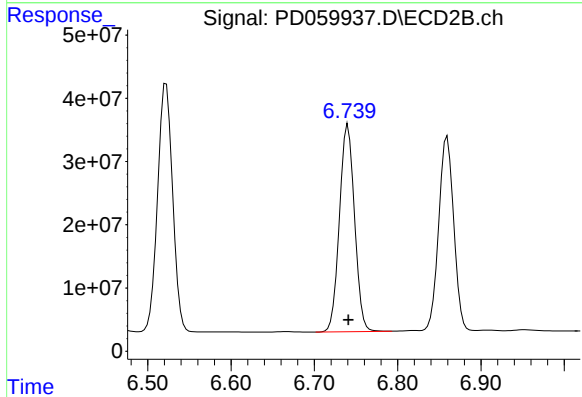


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 412442695
Conc: 159.22 ng/ml

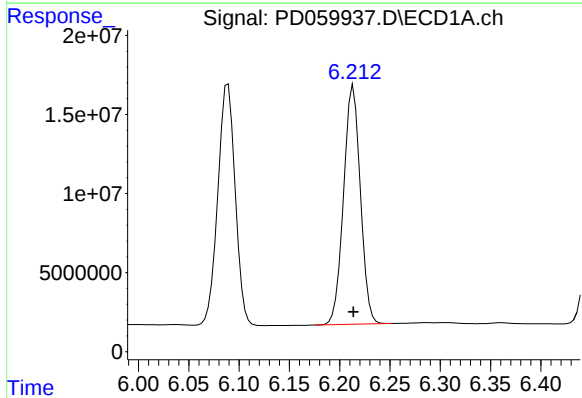


#16 4,4'-DDD

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 174994526
Conc: 161.75 ng/ml

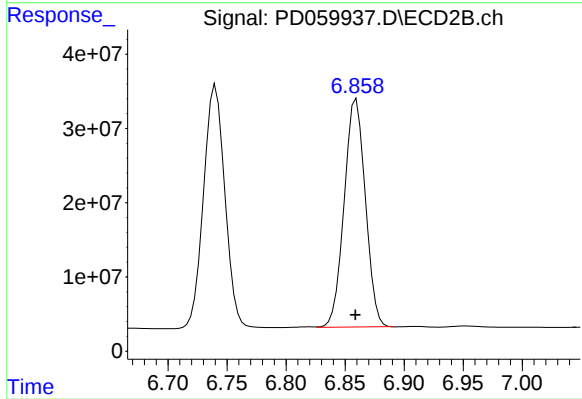

#16 4,4'-DDD


R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 384187546
Conc: 160.76 ng/ml

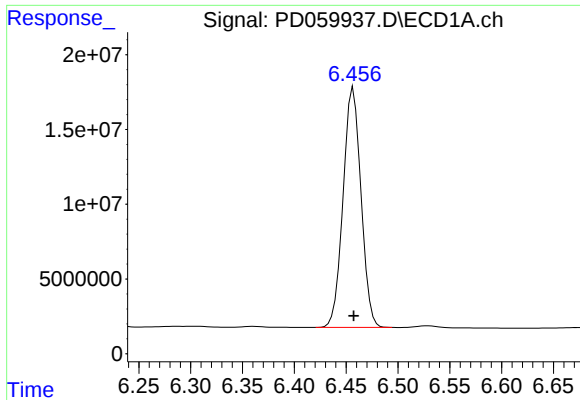

#17 4,4'-DDT


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 193007569
Conc: 163.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

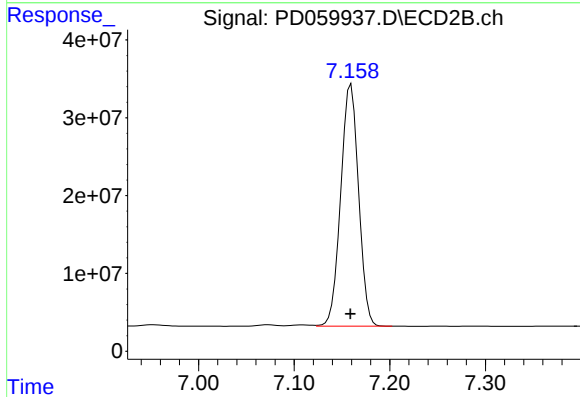


#17 4,4'-DDT

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 405031272
Conc: 163.03 ng/ml

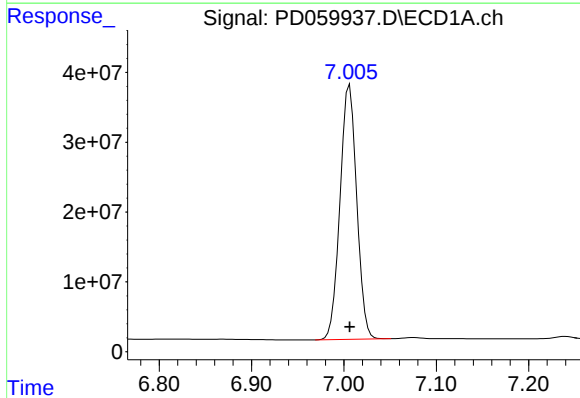


#20 Methoxychlor

R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 458628262
Conc: 745.48 ng/ml

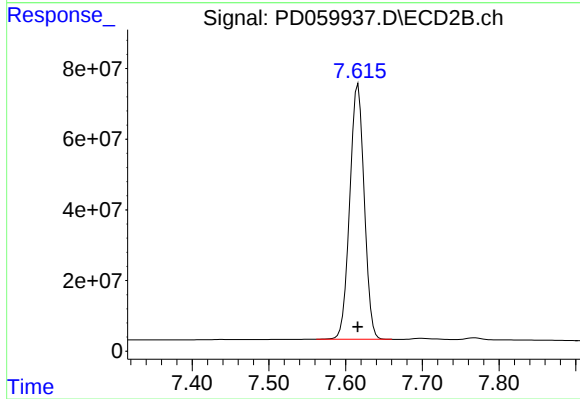

#20 Methoxychlor


R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 953058152
Conc: 730.75 ng/ml

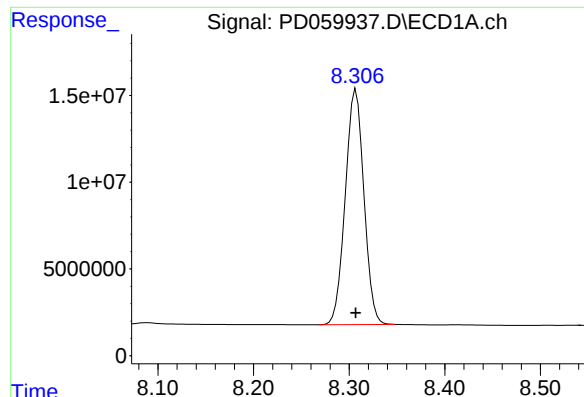

#27 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 184150548
Conc: 145.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

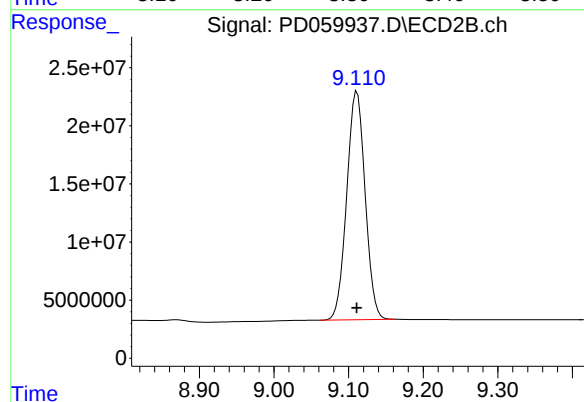

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 336729093
Conc: 155.80 ng/ml