

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 19:33
 Operator : DD\AJ
 Sample : L4499-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 03:55:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 03:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	20081255	54833769	20.120	20.775
2)	SA Decachlor...	8.306	9.110	33338140	60119933	26.104	27.385
Target Compounds							
16)	A 4,4'-DDD	0.000	6.818f	0	1402127	N.D.	0.583
19)	B Endosulfa...	6.686f	0.000	374011	0	0.336	N.D. #
20)	A Methoxychlor	7.060f	0.000	662845	0	1.066	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 19:33
Operator : DD\AJ
Sample : L4499-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 03:55:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 03:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

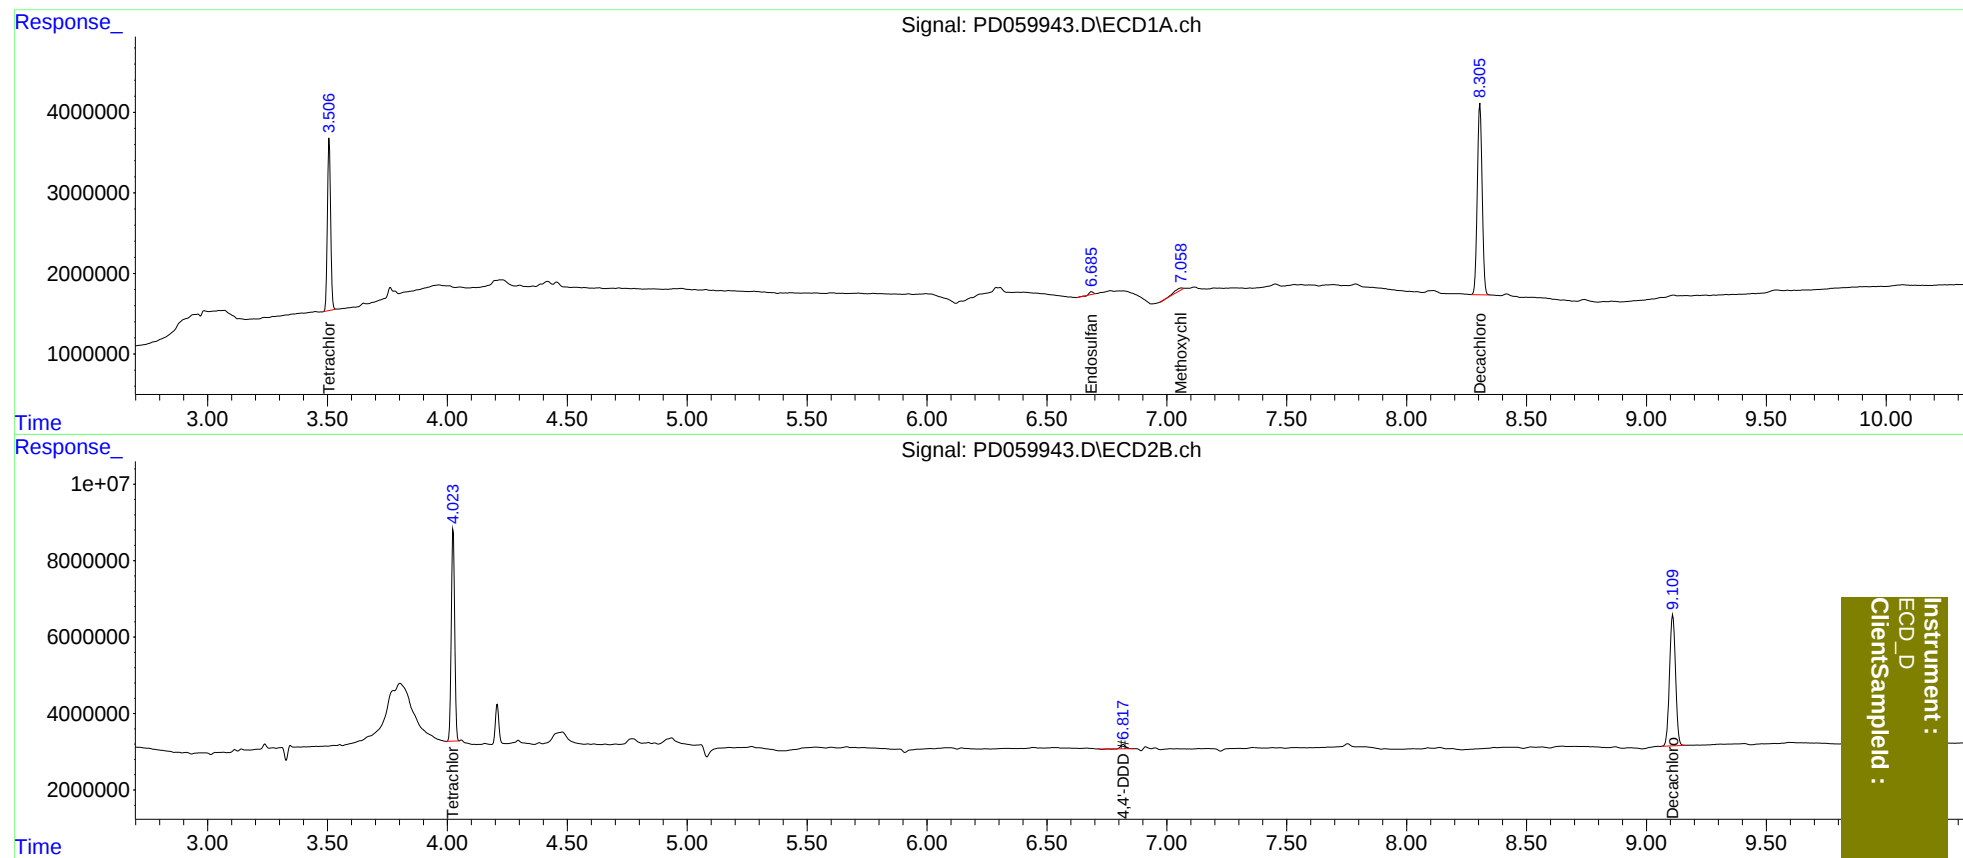


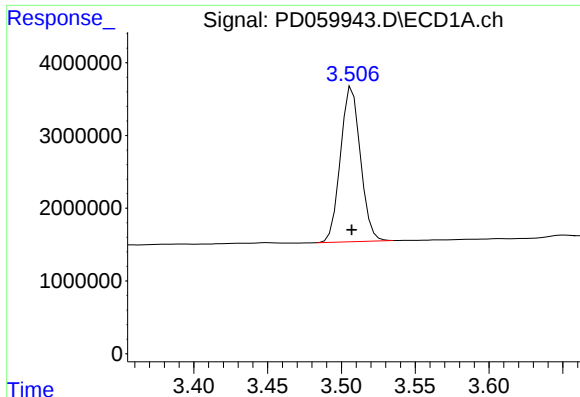

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.000 min
Response: 20081255
Conc: 20.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

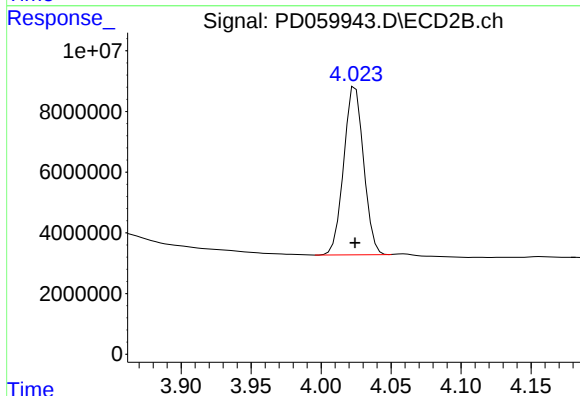


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 54833769
Conc: 20.77 ng/ml

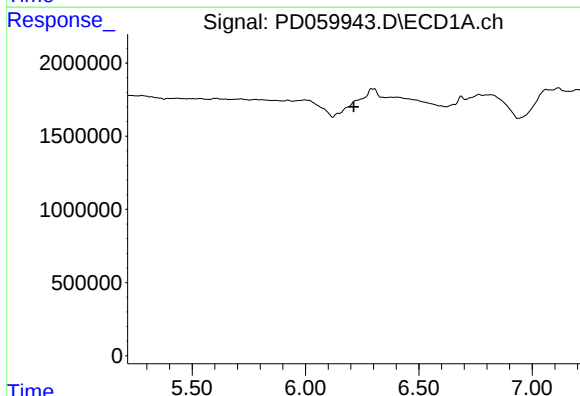


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.213 min
Response: 0
Conc: N.D.

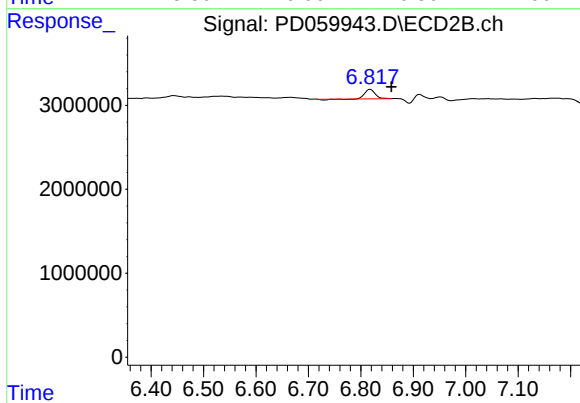

#16 4,4'-DDD


R.T.: 6.818 min
Delta R.T.: -0.040 min
Response: 1402127
Conc: 0.58 ng/ml

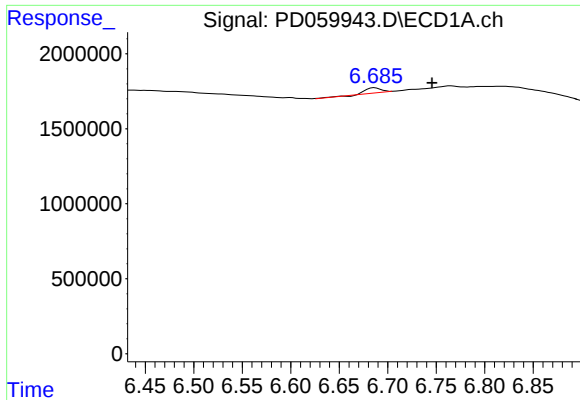

#19 Endosulfan Sulfate


R.T.: 6.686 min
Delta R.T.: -0.059 min
Response: 374011
Conc: 0.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

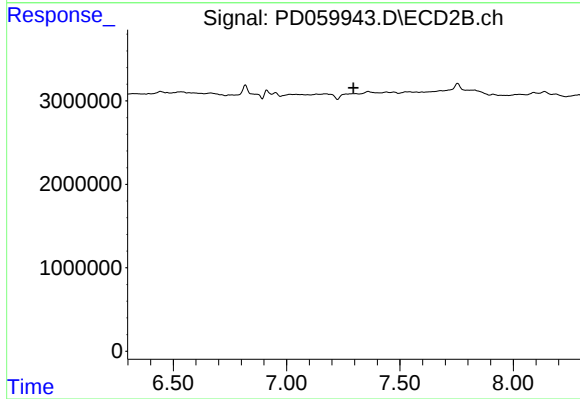


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.295 min
Response: 0
Conc: N.D.

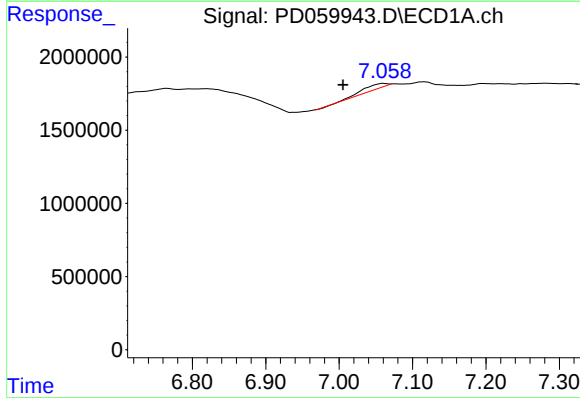


#20 Methoxychlor

R.T.: 7.060 min
Delta R.T.: 0.055 min
Response: 662845
Conc: 1.07 ng/ml

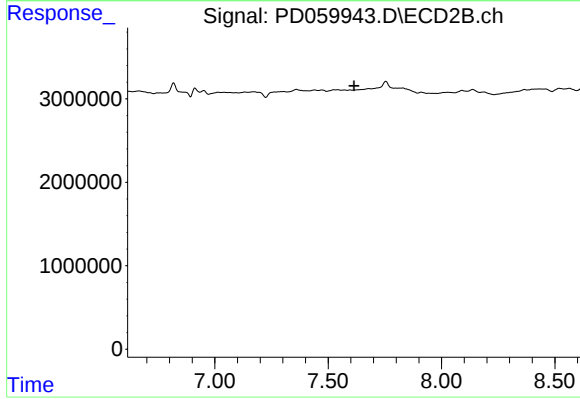

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

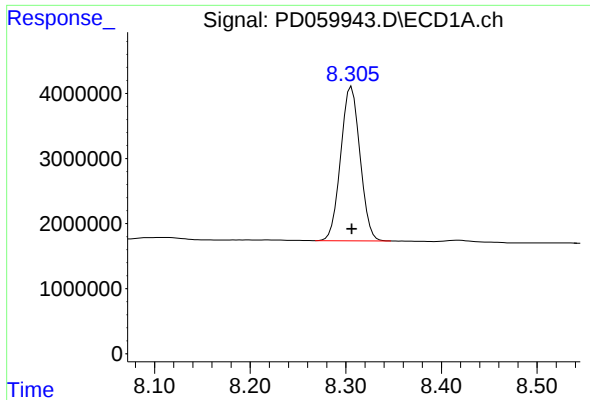

#27 Decachlorobiphenyl

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 33338140
Conc: 26.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

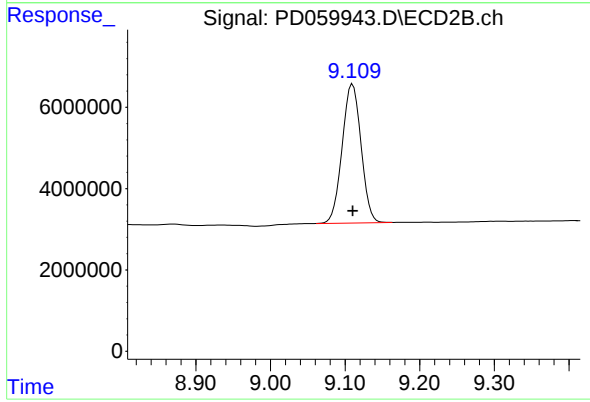

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 60119933
Conc: 27.39 ng/ml