

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 17:39
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:52:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	38651229	105.1E6	39.124	39.866
27)	SA Decachlor...	8.307	9.111	98570378	170.2E6	78.097	78.767
Target Compounds							
2)	A alpha-BHC	3.949	4.415	58884193	158.3E6	40.541	40.868
3)	MA gamma-BHC...	4.235	4.701	55715566	144.4E6	40.256	40.804
4)	MA Heptachlor	4.543	5.213	58221115	141.8E6	40.354	40.977
9)	A Endosulfan I	5.584	6.264	49839471	113.0E6	40.211	40.138
13)	MA Dieldrin	5.830	6.522	112.8E6	254.3E6	82.909	82.169
14)	MA Endrin	6.089	6.740	94447777	214.4E6	81.794	82.778
16)	A 4,4'-DDD	6.214	6.859	89166781	197.4E6	82.420	82.585
17)	MA 4,4'-DDT	6.457	7.159	97825291	207.3E6	82.735	83.439
20)	A Methoxychlor	7.006	7.615	245.4E6	516.2E6	398.880	395.786

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 17:39
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:52:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

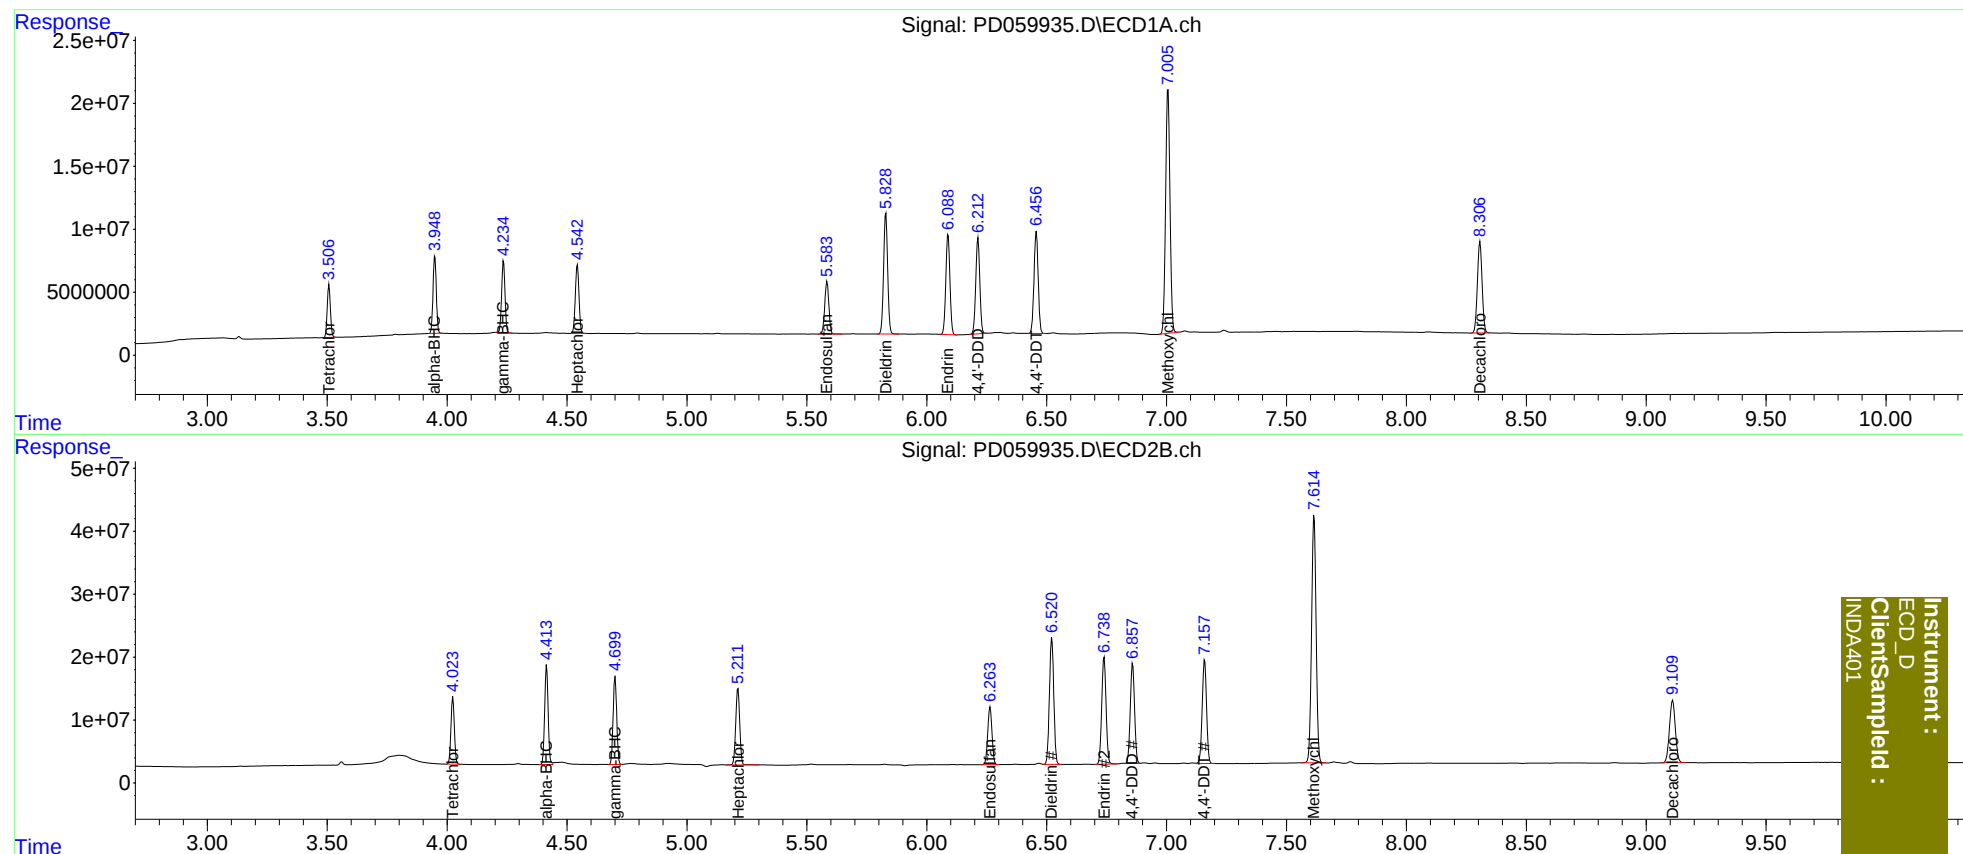

Instrument :
ECD_D
ClientSample :
INDA401