

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
 Data File : PD059937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 18:08
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:52:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 29 02:50:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.025	73532291	202.4E6	74.433	76.750
27)	SA Decachlor...	8.307	9.111	184.2E6	336.7E6	145.901	155.805
Target Compounds							
2)	A alpha-BHC	3.949	4.415	116.3E6	310.8E6	80.064	80.235
3)	MA gamma-BHC...	4.235	4.701	108.9E6	283.3E6	78.714	80.059
4)	MA Heptachlor	4.543	5.213	113.3E6	271.4E6	78.519	78.406
9)	A Endosulfan I	5.584	6.265	96645573	219.1E6	77.975	77.797
13)	MA Dieldrin	5.830	6.522	222.8E6	494.0E6	163.724	159.647
14)	MA Endrin	6.089	6.740	183.2E6	412.4E6	158.677	159.216
16)	A 4,4'-DDD	6.214	6.860	175.0E6	384.2E6	161.754	160.764
17)	MA 4,4'-DDT	6.457	7.160	193.0E6	405.0E6	163.236	163.034
20)	A Methoxychlor	7.006	7.616	458.6E6	953.1E6	745.481	730.750

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD102820\
Data File : PD059937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 18:08
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:52:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102820CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 29 02:50:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

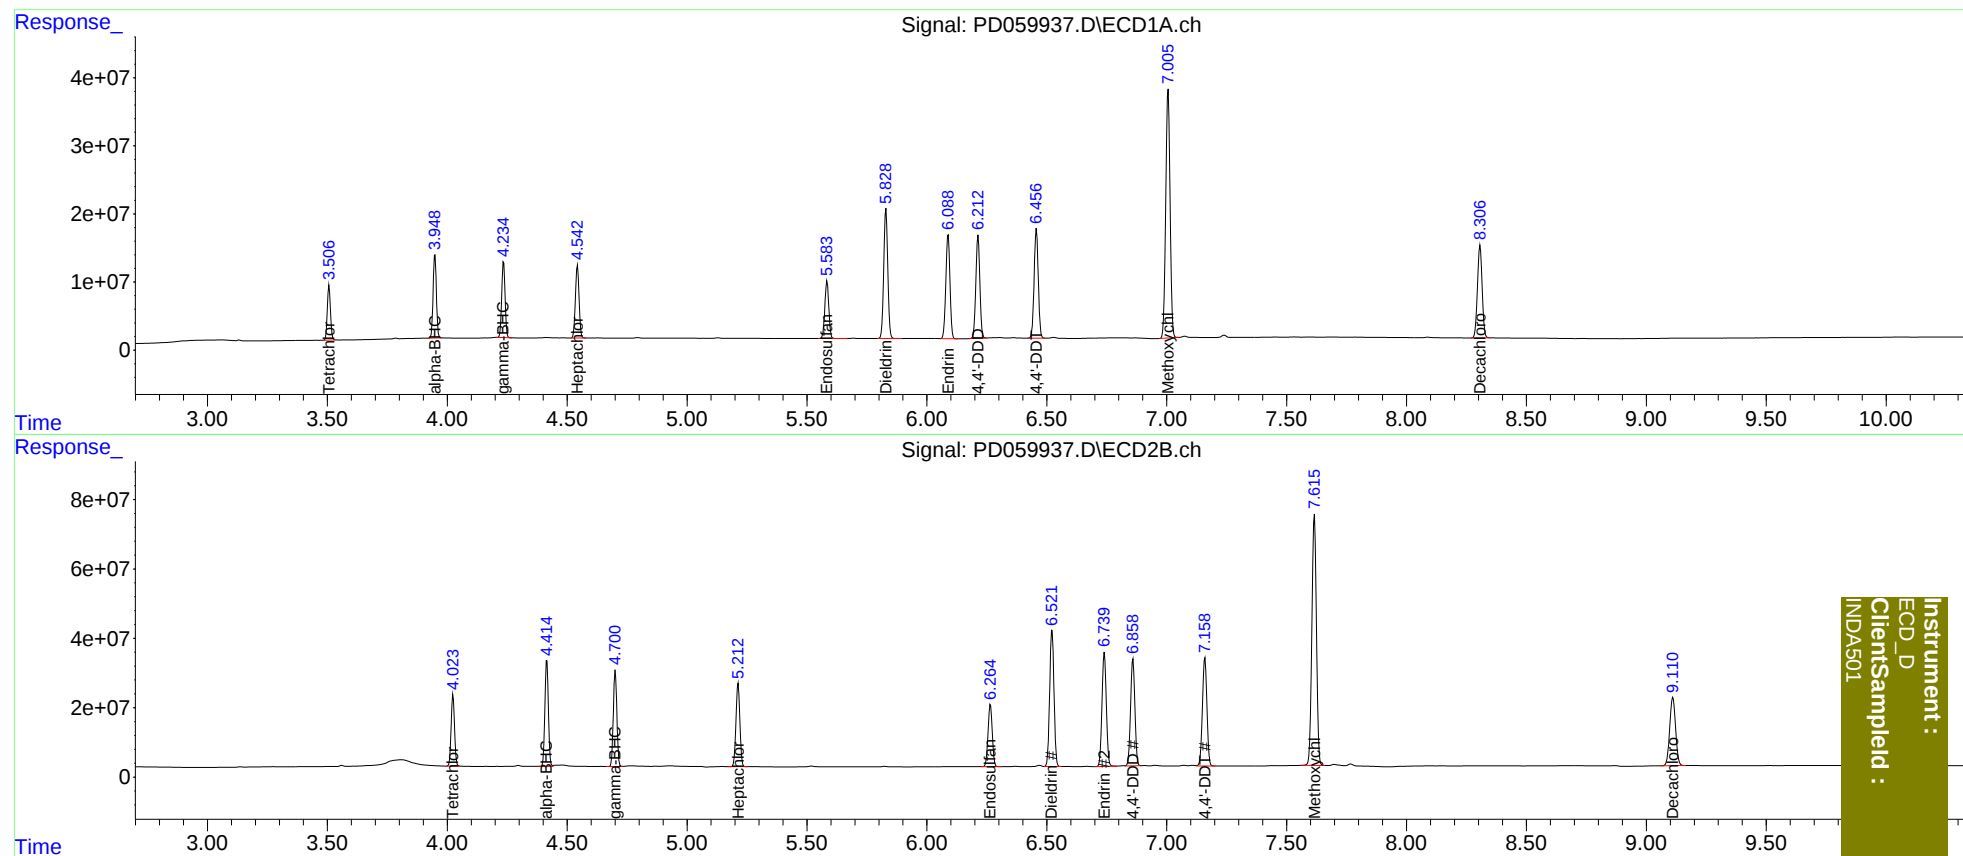

Instrument :
ECD_D
ClientSampled :
INDA501